

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040425\
 Data File : FB031624.D
 Signal(s) : FID2B.CH
 Acq On : 4 Apr 2025 12:38
 Operator : YP/AJ
 Sample : BSF0404S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0404S1

Integration File: Calibration.e
 Quant Time: Apr 05 00:24:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
 Quant Title :
 QLast Update : Wed Mar 26 12:17:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	457633	20.616 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.721	795155	31.228 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1154986	32.544 ng/ml
3) t n-Heptane	7.753	338942	10.430 ng/ml
4) t Benzene	7.892	455583	10.793 ng/ml
6) t Toluene	10.619	1288247	32.440 ng/ml
7) t Ethylbenzene	13.055	384462	10.740 ng/ml
8) t m-Xylene	13.188	842646	21.478 ng/ml
9) t O-Xylene	13.916	790504	21.376 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	590255	21.463 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040425\
Data File : FB031624.D
Signal(s) : FID2B.CH
Acq On : 4 Apr 2025 12:38
Operator : YP/AJ
Sample : BSF0404S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0404S1

Integration File: Calibration.e
Quant Time: Apr 05 00:24:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
Quant Title :
QLast Update : Wed Mar 26 12:17:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

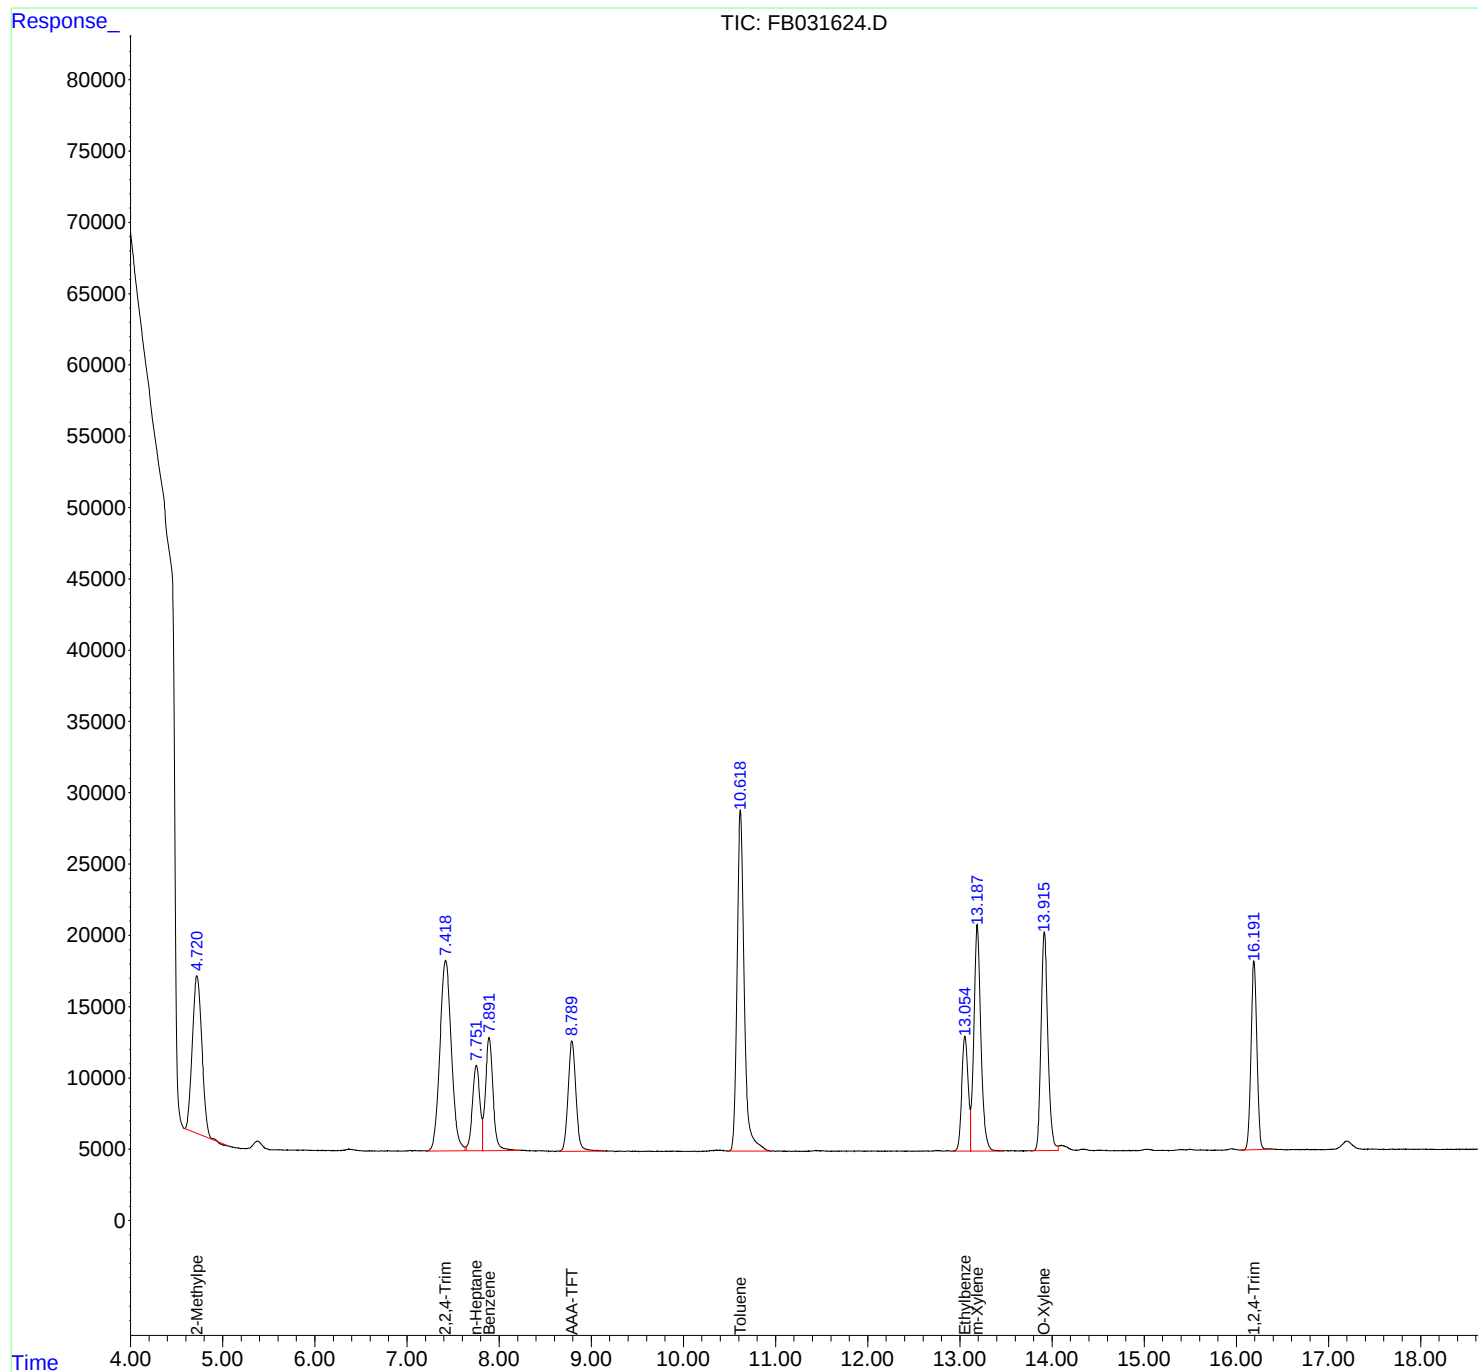


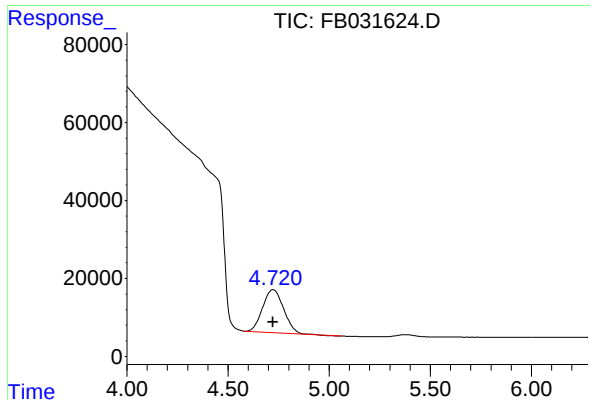

#1 2-Methylpentane


R.T.: 4.721 min
Delta R.T.: -0.002 min
Response: 795155
Conc: 31.23 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

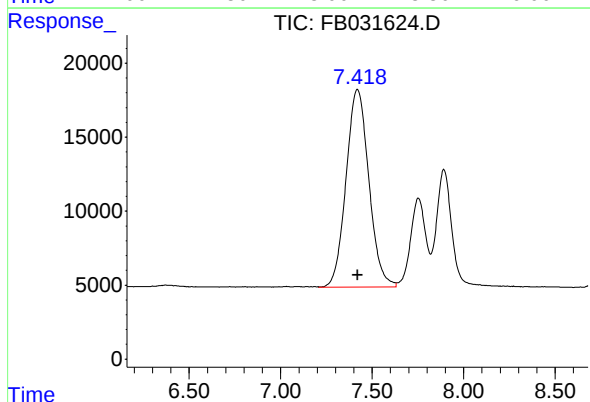


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.002 min
Response: 1154986
Conc: 32.54 ng/ml

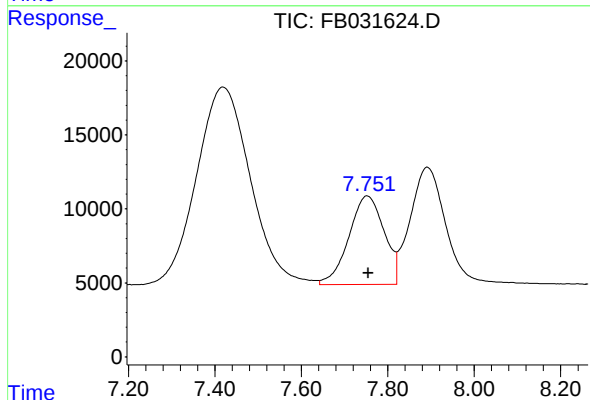


#3 n-Heptane

R.T.: 7.753 min
Delta R.T.: -0.002 min
Response: 338942
Conc: 10.43 ng/ml

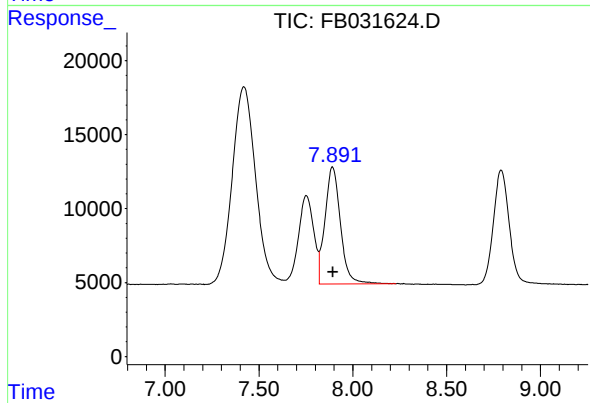

#4 Benzene


R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 455583
Conc: 10.79 ng/ml

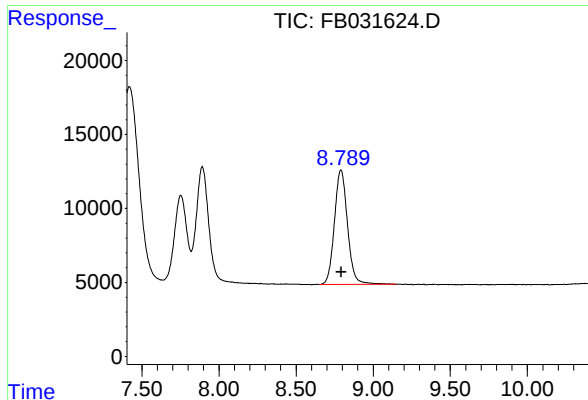

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.002 min
Response: 457633
Conc: 20.62 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

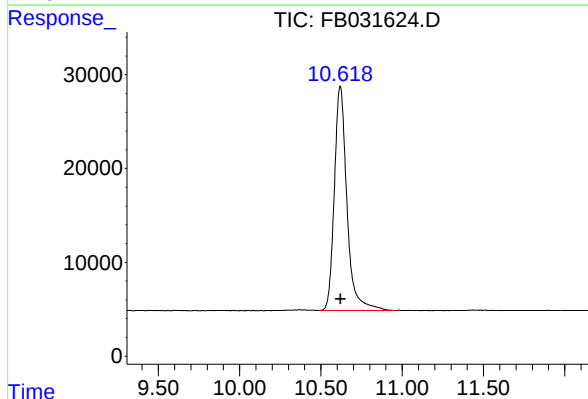


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 1288247
Conc: 32.44 ng/ml

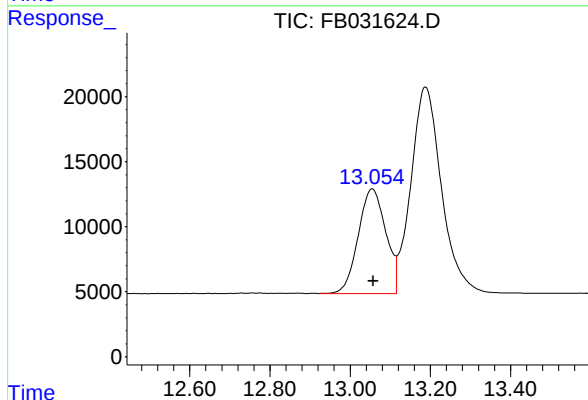


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.002 min
Response: 384462
Conc: 10.74 ng/ml

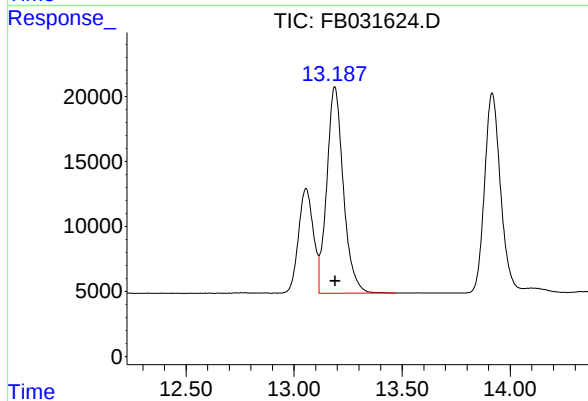

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 842646
Conc: 21.48 ng/ml

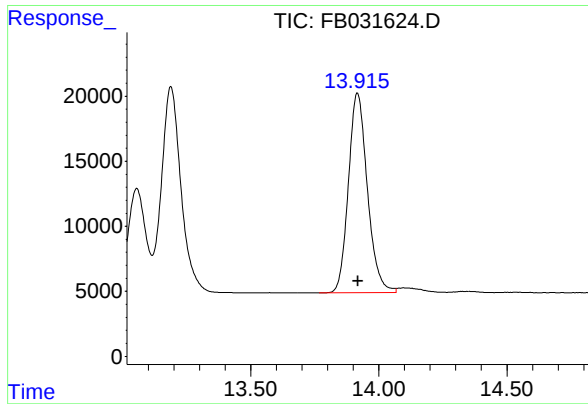

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 790504
Conc: 21.38 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

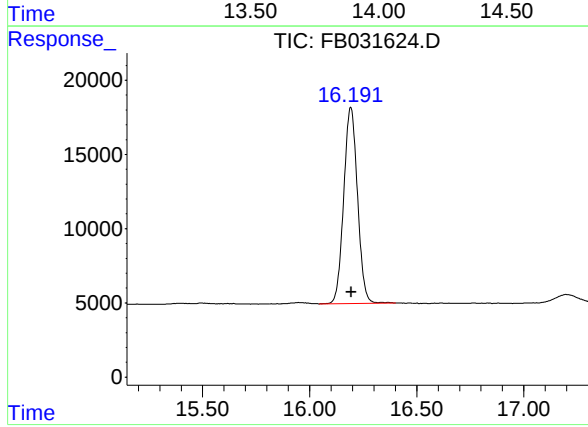

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.003 min
Response: 590255
Conc: 21.46 ng/ml