

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040425\
 Data File : FB031628.D
 Signal(s) : FID2B.CH
 Acq On : 4 Apr 2025 14:27
 Operator : YP/AJ
 Sample : BSF0404S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0404S2

Integration File: Calibration.e
 Quant Time: Apr 05 00:24:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
 Quant Title :
 QLast Update : Wed Mar 26 12:17:59 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	309634	13.948 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.724	855533	33.599 ng/ml
2) t 2,2,4-Trimethylpentane	7.421	1144598	32.252 ng/ml
3) t n-Heptane	7.755	336509	10.355 ng/ml
4) t Benzene	7.894	443162	10.499 ng/ml
6) t Toluene	10.621	1275357	32.116 ng/ml
7) t Ethylbenzene	13.057	379743	10.608 ng/ml
8) t m-Xylene	13.191	830941	21.180 ng/ml
9) t O-Xylene	13.919	781440	21.131 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	577389	20.995 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040425\
Data File : FB031628.D
Signal(s) : FID2B.CH
Acq On : 4 Apr 2025 14:27
Operator : YP/AJ
Sample : BSF0404S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0404S2

Integration File: Calibration.e
Quant Time: Apr 05 00:24:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032625.M
Quant Title :
QLast Update : Wed Mar 26 12:17:59 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

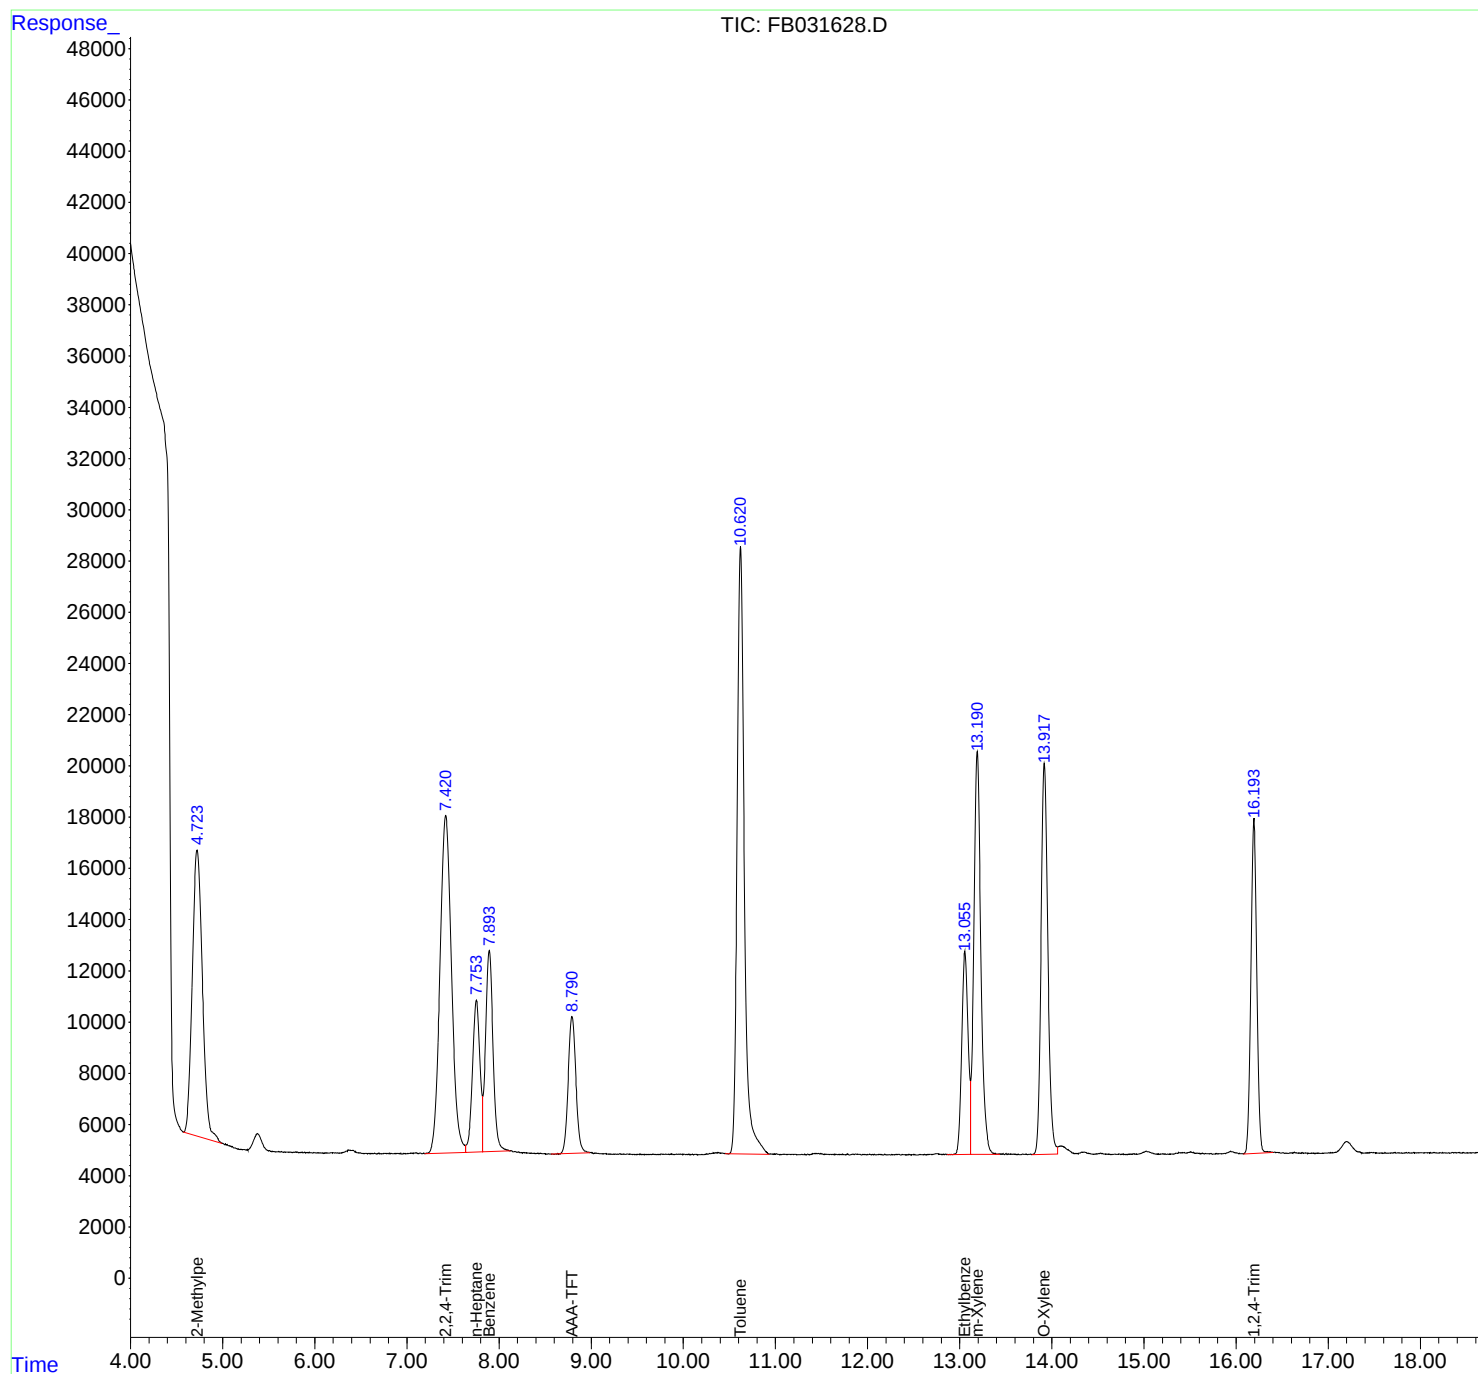


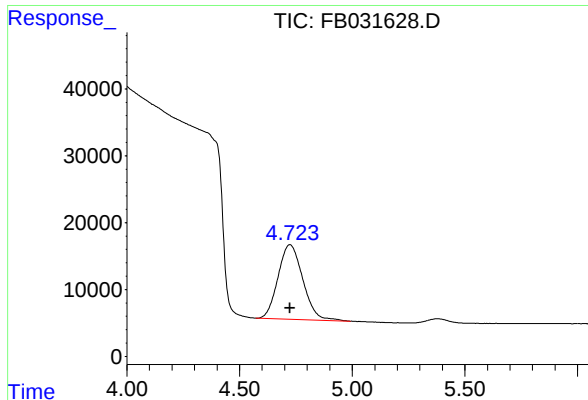

#1 2-Methylpentane


R.T.: 4.724 min
Delta R.T.: 0.000 min
Response: 855533
Conc: 33.60 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S2

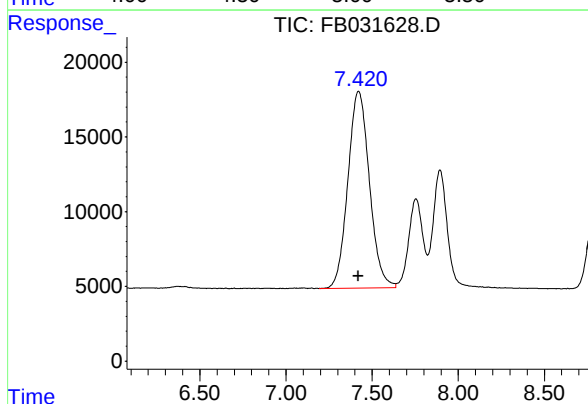


#2 2,2,4-Trimethylpentane

R.T.: 7.421 min
Delta R.T.: 0.000 min
Response: 1144598
Conc: 32.25 ng/ml

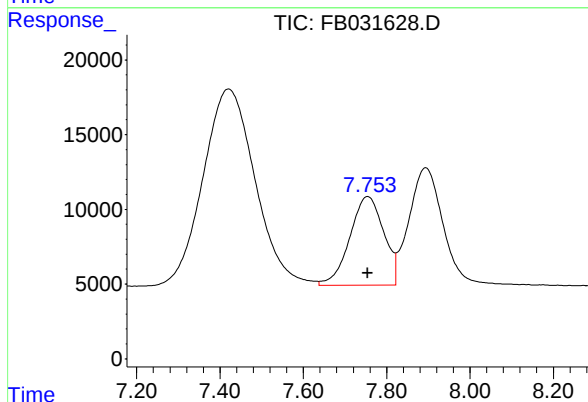


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 336509
Conc: 10.36 ng/ml

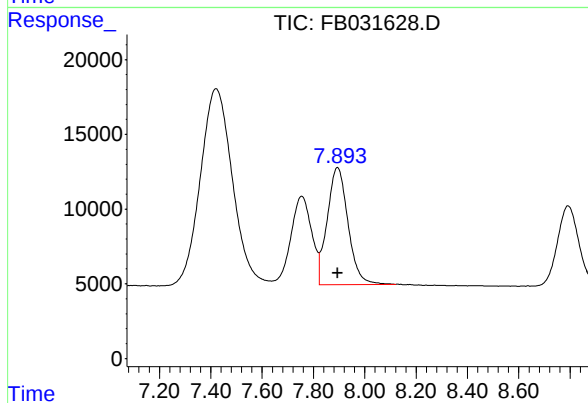

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 443162
Conc: 10.50 ng/ml

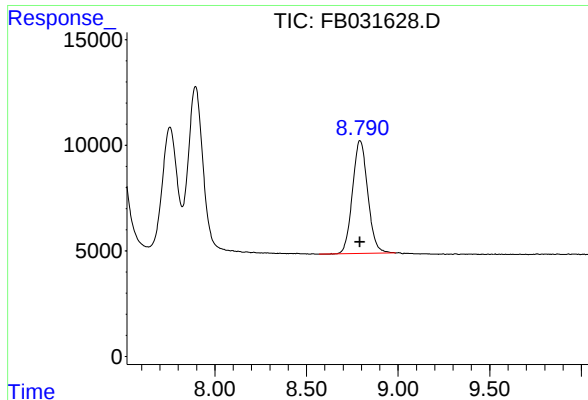

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 309634
Conc: 13.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S2

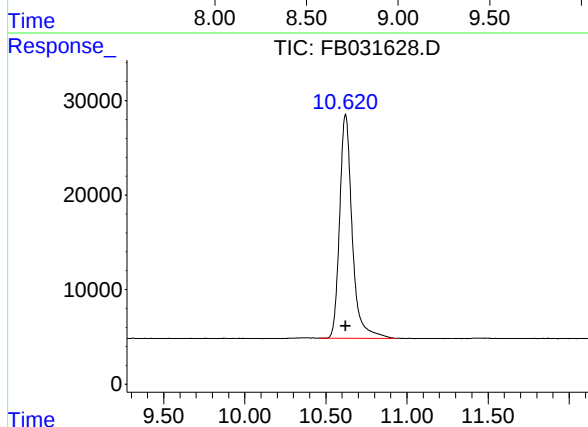


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 1275357
Conc: 32.12 ng/ml

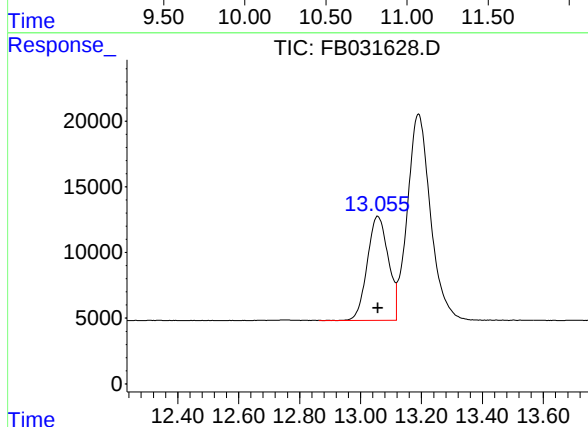


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 379743
Conc: 10.61 ng/ml

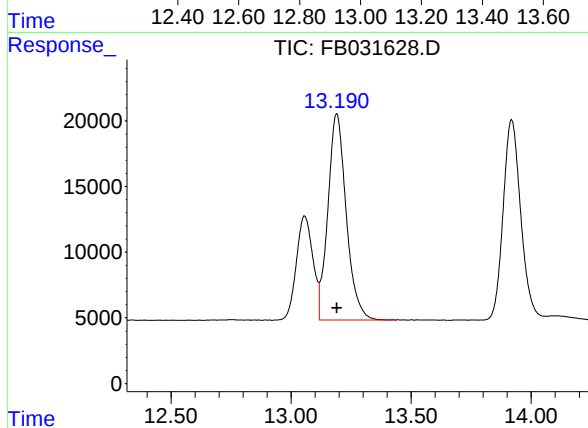

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 830941
Conc: 21.18 ng/ml

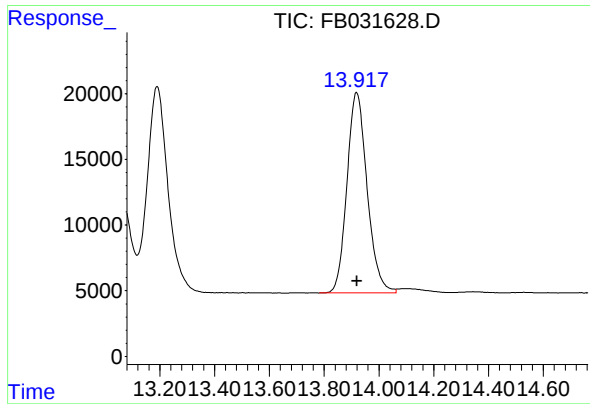

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: -0.001 min
Response: 781440
Conc: 21.13 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S2

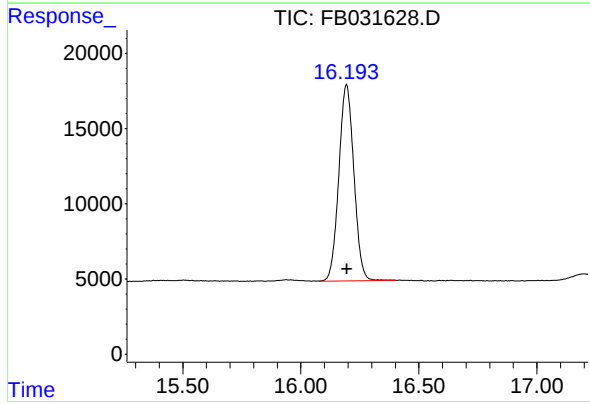

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: -0.002 min
Response: 577389
Conc: 20.99 ng/ml