

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020535.D
 Signal(s) : FID2B.CH
 Acq On : 5 Apr 2019 10:53
 Operator : MJ/SJ
 Sample : BSF0405W1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0405W1

Integration File: Calibration.e
 Quant Time: Apr 06 01:16:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	382732	20.751 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	1138082	32.329 ng/ml
2) t 2,2,4-Trimethylpentane	7.621	951331	31.909 ng/ml
3) t n-Heptane	7.952	412267	10.502 ng/ml
4) t Benzene	8.088	439235	10.694 ng/ml
6) t Toluene	10.839	957797	31.698 ng/ml
7) t Ethylbenzene	13.289	261489	10.222 ng/ml
8) t m-Xylene	13.422	539969	20.431 ng/ml
9) t O-Xylene	14.152	547502	20.224 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	533041	20.402 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020535.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2019 10:53
Operator : MJ/SJ
Sample : BSF0405W1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0405W1

Integration File: Calibration.e
Quant Time: Apr 06 01:16:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

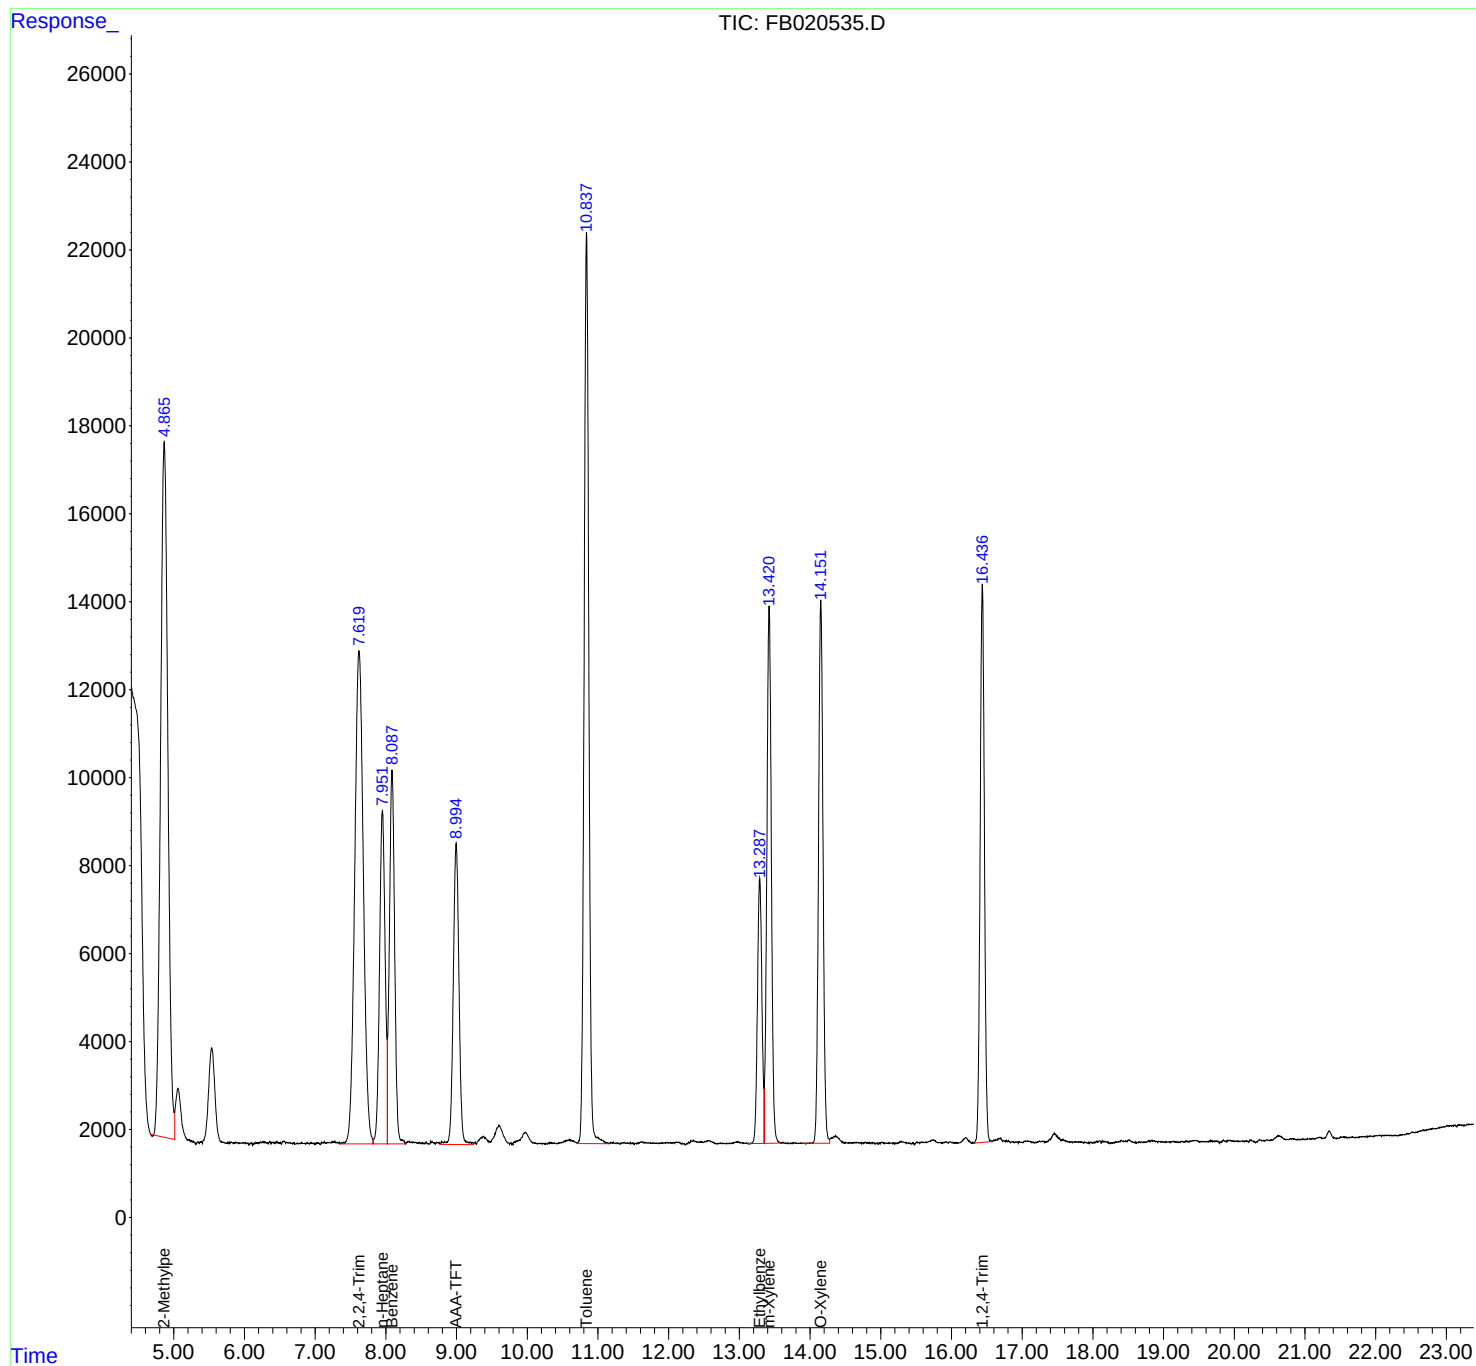


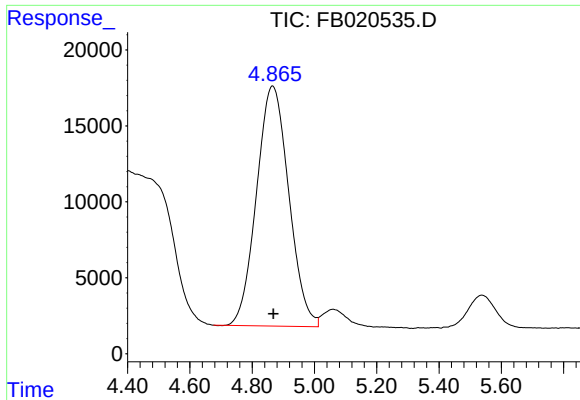

#1 2-Methylpentane


R.T.: 4.866 min
 Delta R.T.: -0.003 min
 Response: 1138082
 Conc: 32.33 ng/ml

Instrument :
 FID_B
 ClientSampleId :
 BSF0405W1

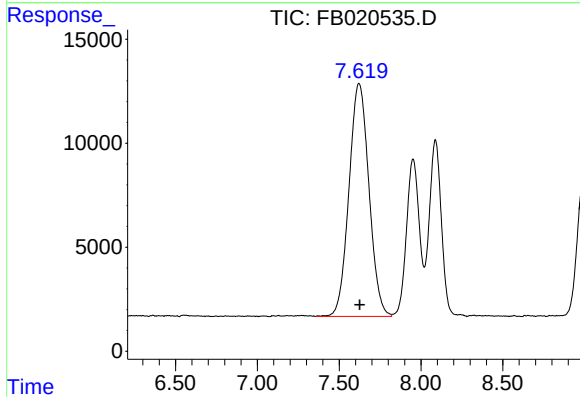


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
 Delta R.T.: -0.005 min
 Response: 951331
 Conc: 31.91 ng/ml

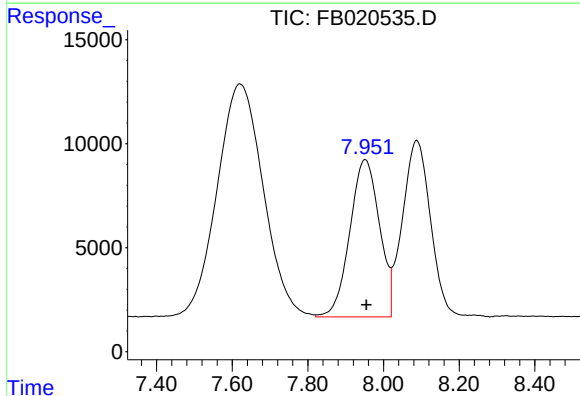


#3 n-Heptane

R.T.: 7.952 min
 Delta R.T.: -0.003 min
 Response: 412267
 Conc: 10.50 ng/ml

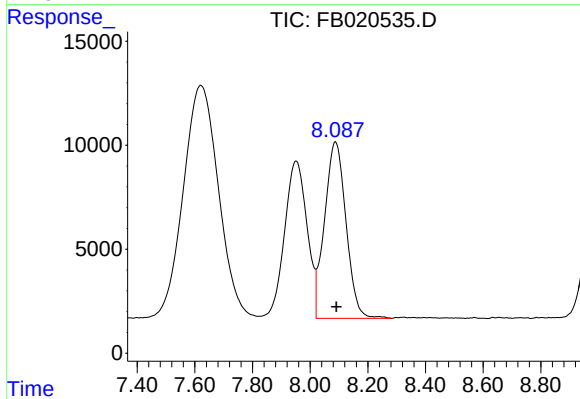

#4 Benzene


R.T.: 8.088 min
 Delta R.T.: -0.003 min
 Response: 439235
 Conc: 10.69 ng/ml

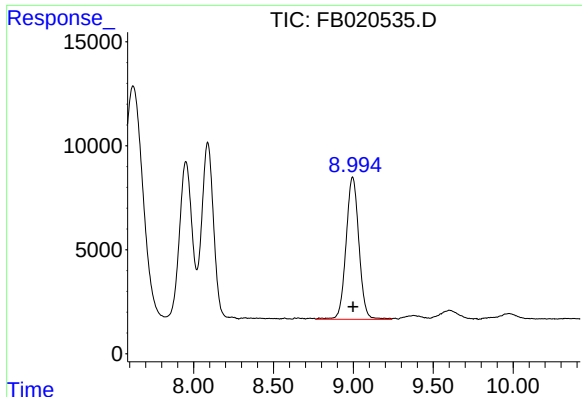

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 382732
Conc: 20.75 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0405W1

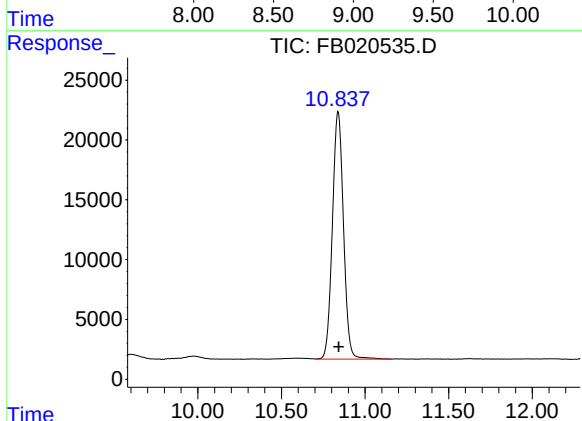


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 957797
Conc: 31.70 ng/ml

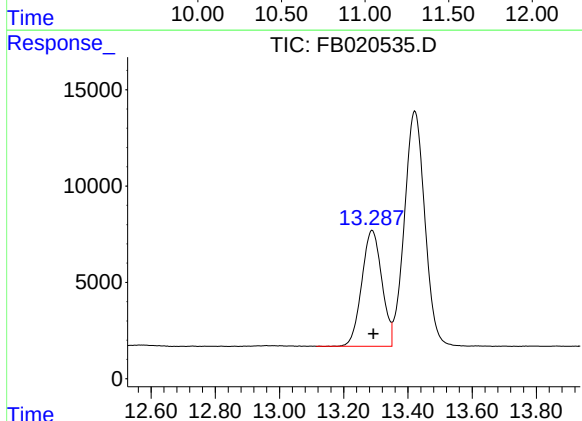


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 261489
Conc: 10.22 ng/ml

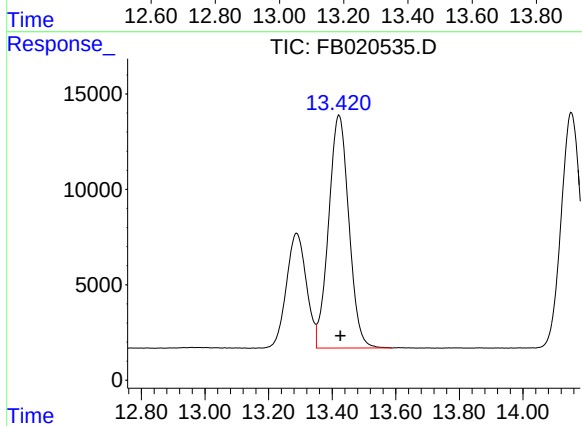

#8 m-Xylene


R.T.: 13.422 min
Delta R.T.: -0.004 min
Response: 539969
Conc: 20.43 ng/ml

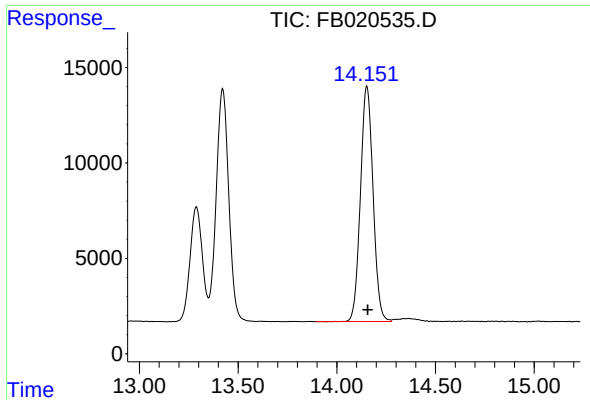

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: -0.004 min
Response: 547502
Conc: 20.22 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0405W1

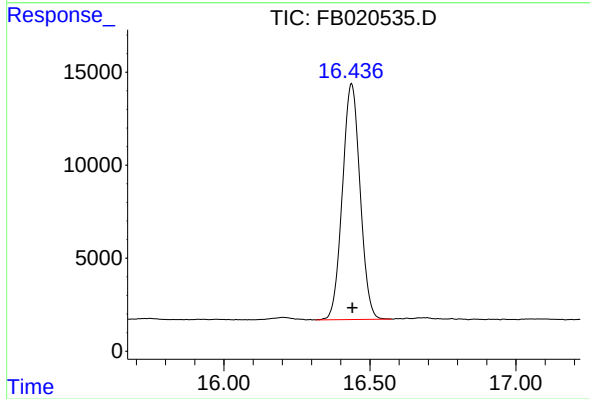

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.003 min
Response: 533041
Conc: 20.40 ng/ml