

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020544.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2019 17:31
Operator : MJ/SJ
Sample : K2240-01
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-01-(0-2)

Integration File: Calibration.e
Quant Time: Apr 06 01:18:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.997	389394	21.112 ng/ml
Target Compounds			
6) t Toluene	10.842	8266	0.274 ng/ml
8) t m-Xylene	13.425	6047	0.229 ng/ml
9) t O-Xylene	14.154	3932	0.145 ng/ml
10) t 1,2,4-Trimethylbenzene	16.444	6620	0.253 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020544.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2019 17:31
Operator : MJ/SJ
Sample : K2240-01
Misc : 5.05g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-01-(0-2)

Integration File: Calibration.e
Quant Time: Apr 06 01:18:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

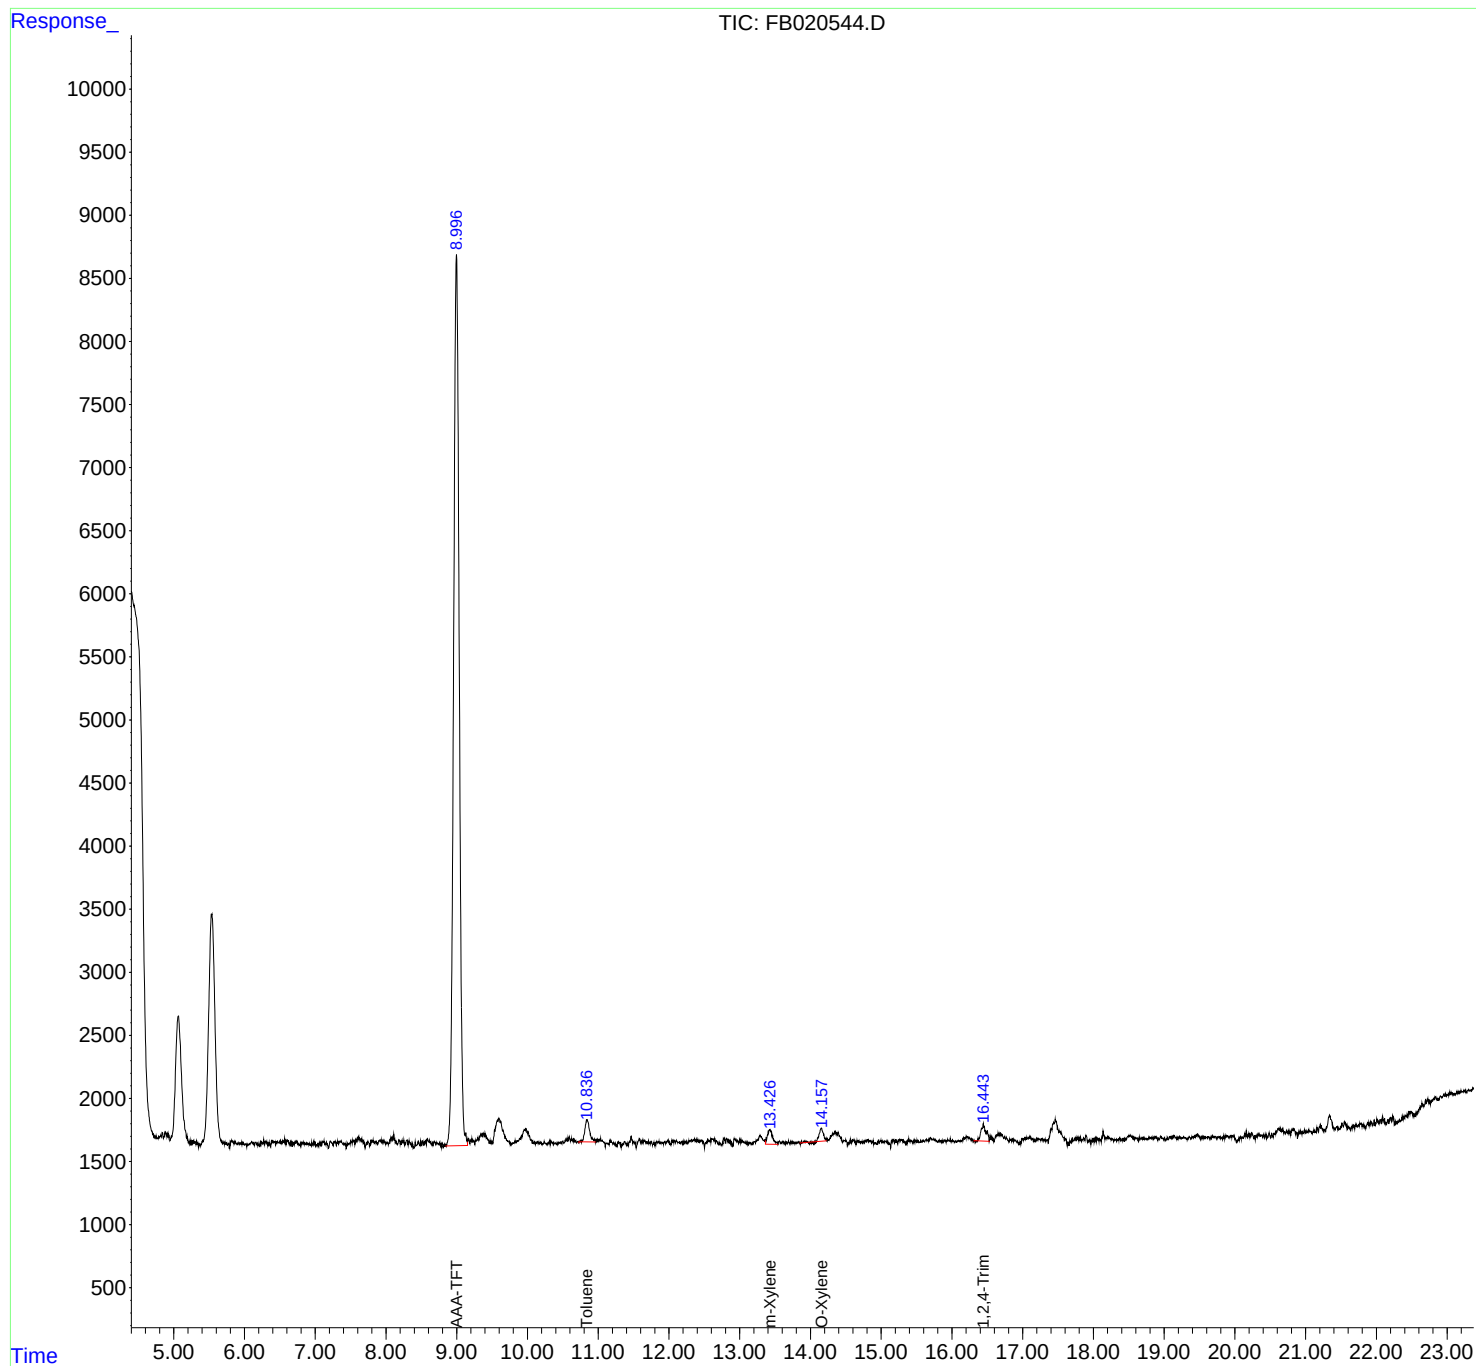


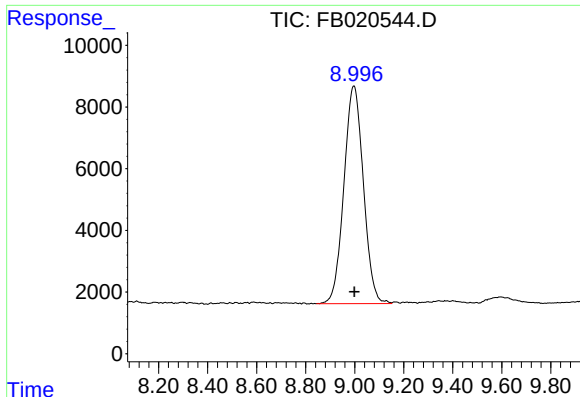

#5 AAA-TFT


R.T.: 8.997 min
Delta R.T.: -0.002 min
Response: 389394
Conc: 21.11 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-01-(0-2)

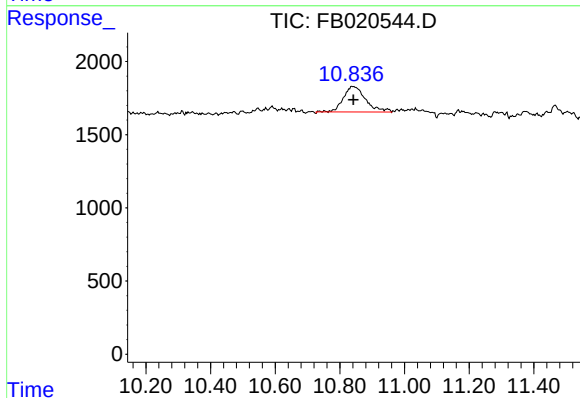


#6 Toluene

R.T.: 10.842 min
Delta R.T.: 0.000 min
Response: 8266
Conc: 0.27 ng/ml

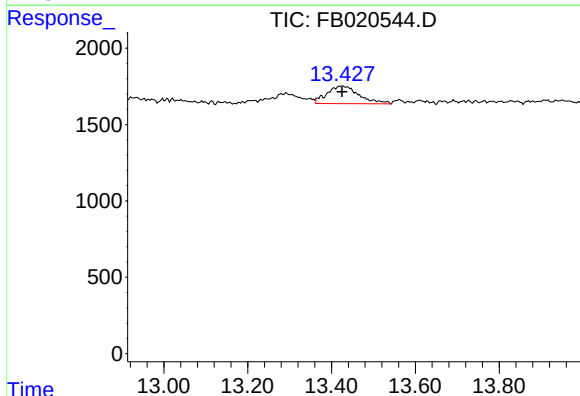


#8 m-Xylene

R.T.: 13.425 min
Delta R.T.: 0.000 min
Response: 6047
Conc: 0.23 ng/ml

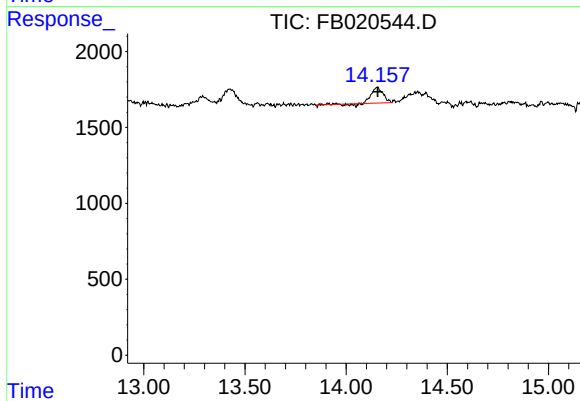

#9 O-Xylene

R.T.: 14.154 min
Delta R.T.: -0.003 min
Response: 3932
Conc: 0.15 ng/ml

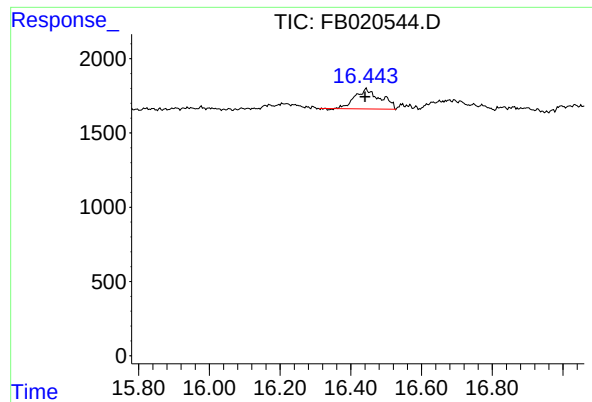

#10 1,2,4-Trimethylbenzene

R.T.: 16.444 min
Delta R.T.: 0.004 min
Response: 6620
Conc: 0.25 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-01-(0-2)