

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020565.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 4:32
 Operator : MJ/SJ
 Sample : K2193-01
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: SAMPLE.e
 Quant Time: Apr 08 05:29:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	287721	15.599 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.859	478	0.014 ng/ml
2) t 2,2,4-Trimethylpentane	7.625	829	0.028 ng/ml
3) t n-Heptane	7.965	971	0.025 ng/ml
4) t Benzene	8.089	243	0.006 ng/ml
6) t Toluene	10.841	449	0.015 ng/ml
7) t Ethylbenzene	13.256	70056	2.739 ng/ml
9) t O-Xylene	14.170	25050	0.925 ng/ml
10) t 1,2,4-Trimethylbenzene	16.460	39256	1.503 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020565.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 4:32
Operator : MJ/SJ
Sample : K2193-01
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: SAMPLE.e
Quant Time: Apr 08 05:29:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

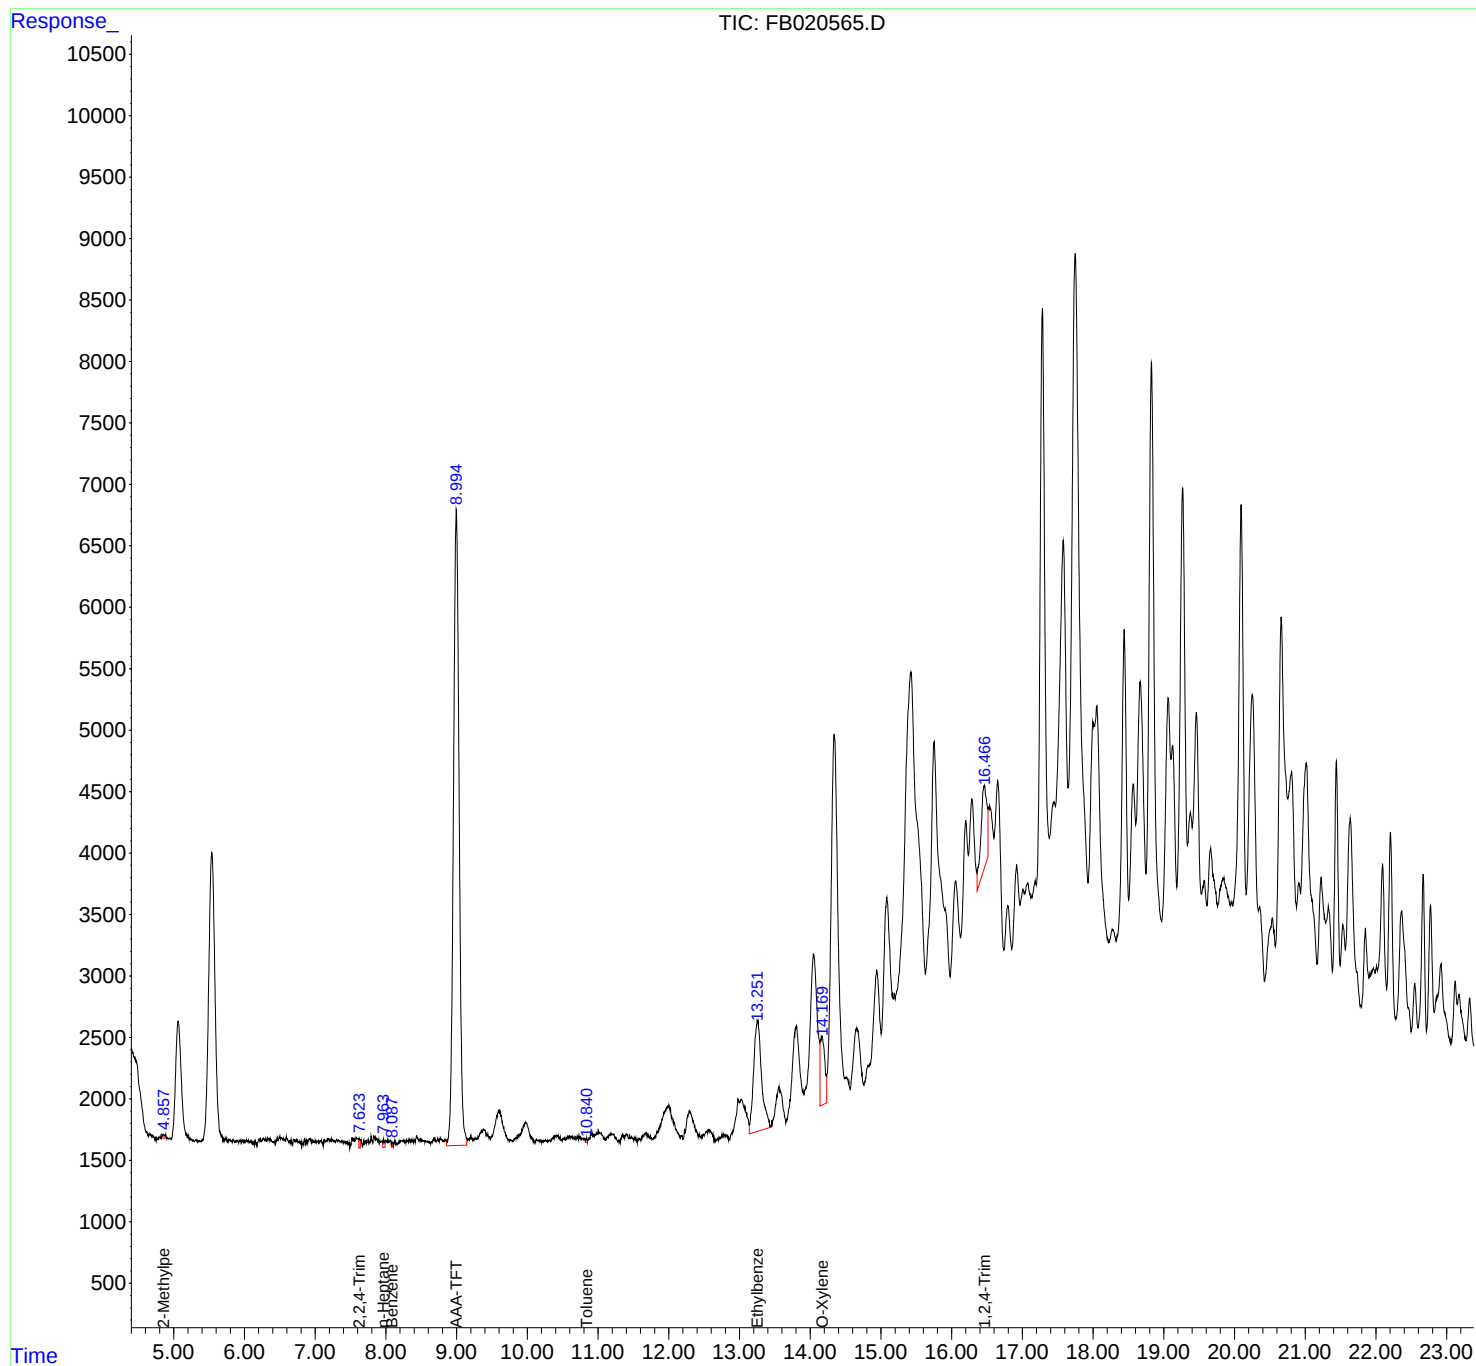


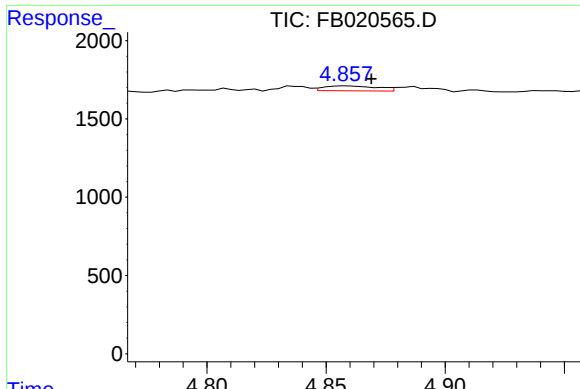

#1 2-Methylpentane


R.T.: 4.859 min
Delta R.T.: -0.010 min
Response: 478
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :

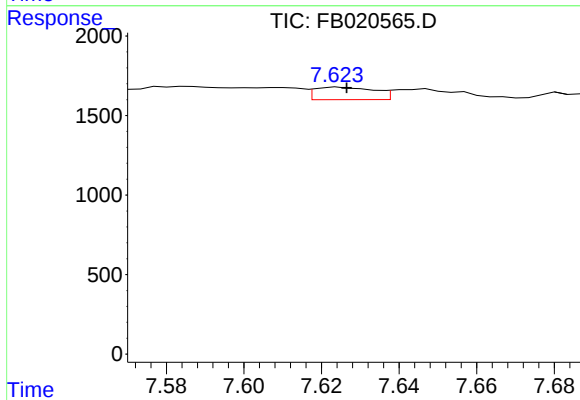


#2 2,2,4-Trimethylpentane

R.T.: 7.625 min
Delta R.T.: -0.001 min
Response: 829
Conc: 0.03 ng/ml

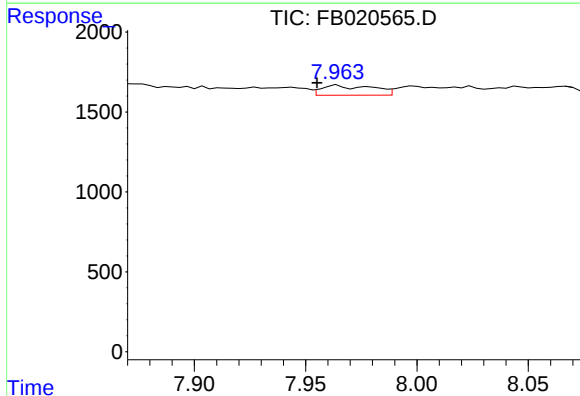


#3 n-Heptane

R.T.: 7.965 min
Delta R.T.: 0.009 min
Response: 971
Conc: 0.02 ng/ml

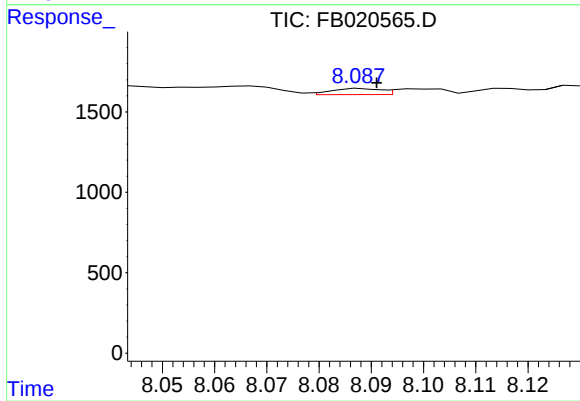

#4 Benzene


R.T.: 8.089 min
Delta R.T.: -0.002 min
Response: 243
Conc: 0.01 ng/ml

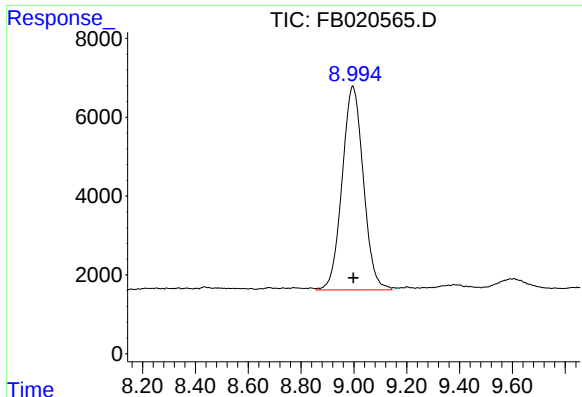

#5 AAA-TFT


R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 287721
Conc: 15.60 ng/ml

Instrument :
FID_B
ClientSampleId :

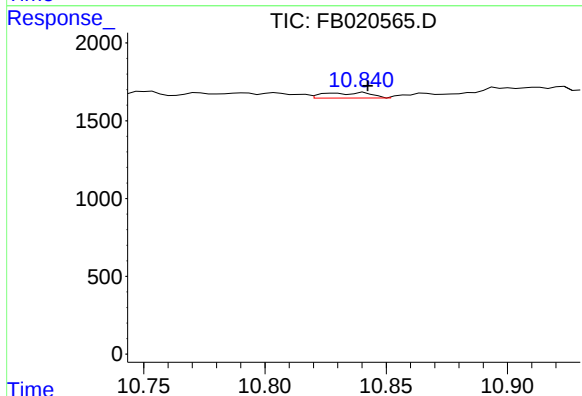


#6 Toluene

R.T.: 10.841 min
Delta R.T.: -0.002 min
Response: 449
Conc: 0.01 ng/ml

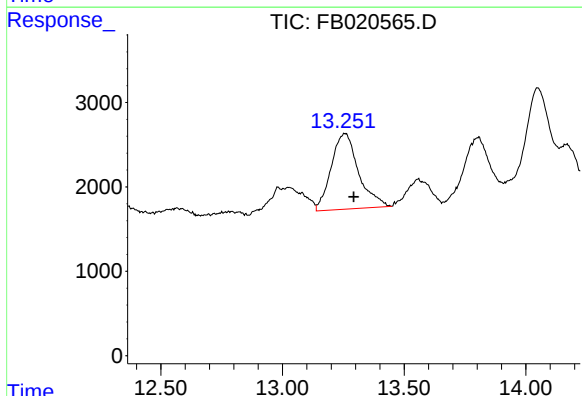


#7 Ethylbenzene

R.T.: 13.256 min
Delta R.T.: -0.037 min
Response: 70056
Conc: 2.74 ng/ml

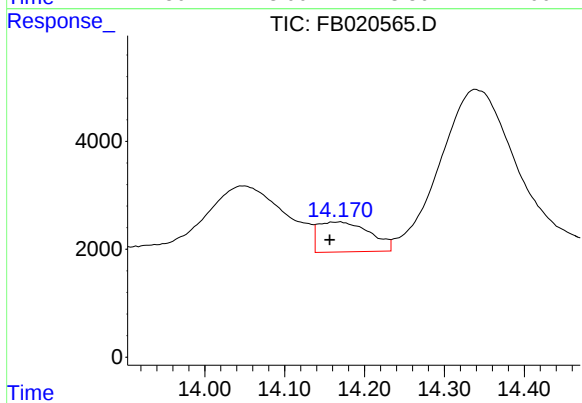

#9 O-Xylene

R.T.: 14.170 min
Delta R.T.: 0.013 min
Response: 25050
Conc: 0.93 ng/ml

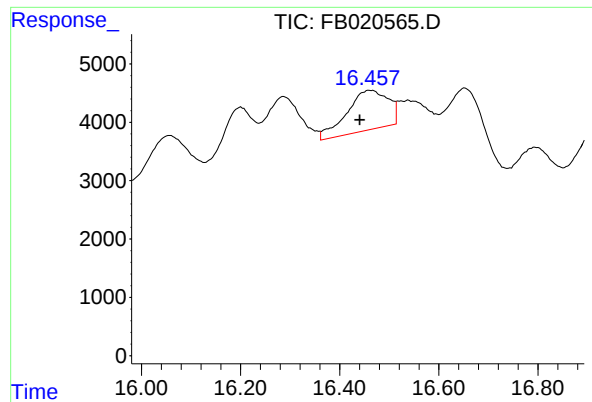

#10 1,2,4-Trimethylbenzene

R.T.: 16.460 min
Delta R.T.: 0.020 min
Response: 39256
Conc: 1.50 ng/ml

Instrument :
FID_B
ClientSampleId :