

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020569.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 6:32
 Operator : MJ/SJ
 Sample : K2257-33MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RO-20MSD

Integration File: SAMPLE.e
 Quant Time: Apr 08 05:30:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	319459	17.320 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.865	965249	27.419 ng/ml
2) t 2,2,4-Trimethylpentane	7.620	821381	27.550 ng/ml
3) t n-Heptane	7.952	351644	8.958 ng/ml
4) t Benzene	8.088	381362	9.285 ng/ml
6) t Toluene	10.839	830204	27.476 ng/ml
7) t Ethylbenzene	13.289	239632	9.367 ng/ml
8) t m-Xylene	13.421	482097	18.241 ng/ml
9) t O-Xylene	14.152	499737	18.460 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	459606	17.591 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020569.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 6:32
Operator : MJ/SJ
Sample : K2257-33MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RO-20MSD

Integration File: SAMPLE.e
Quant Time: Apr 08 05:30:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

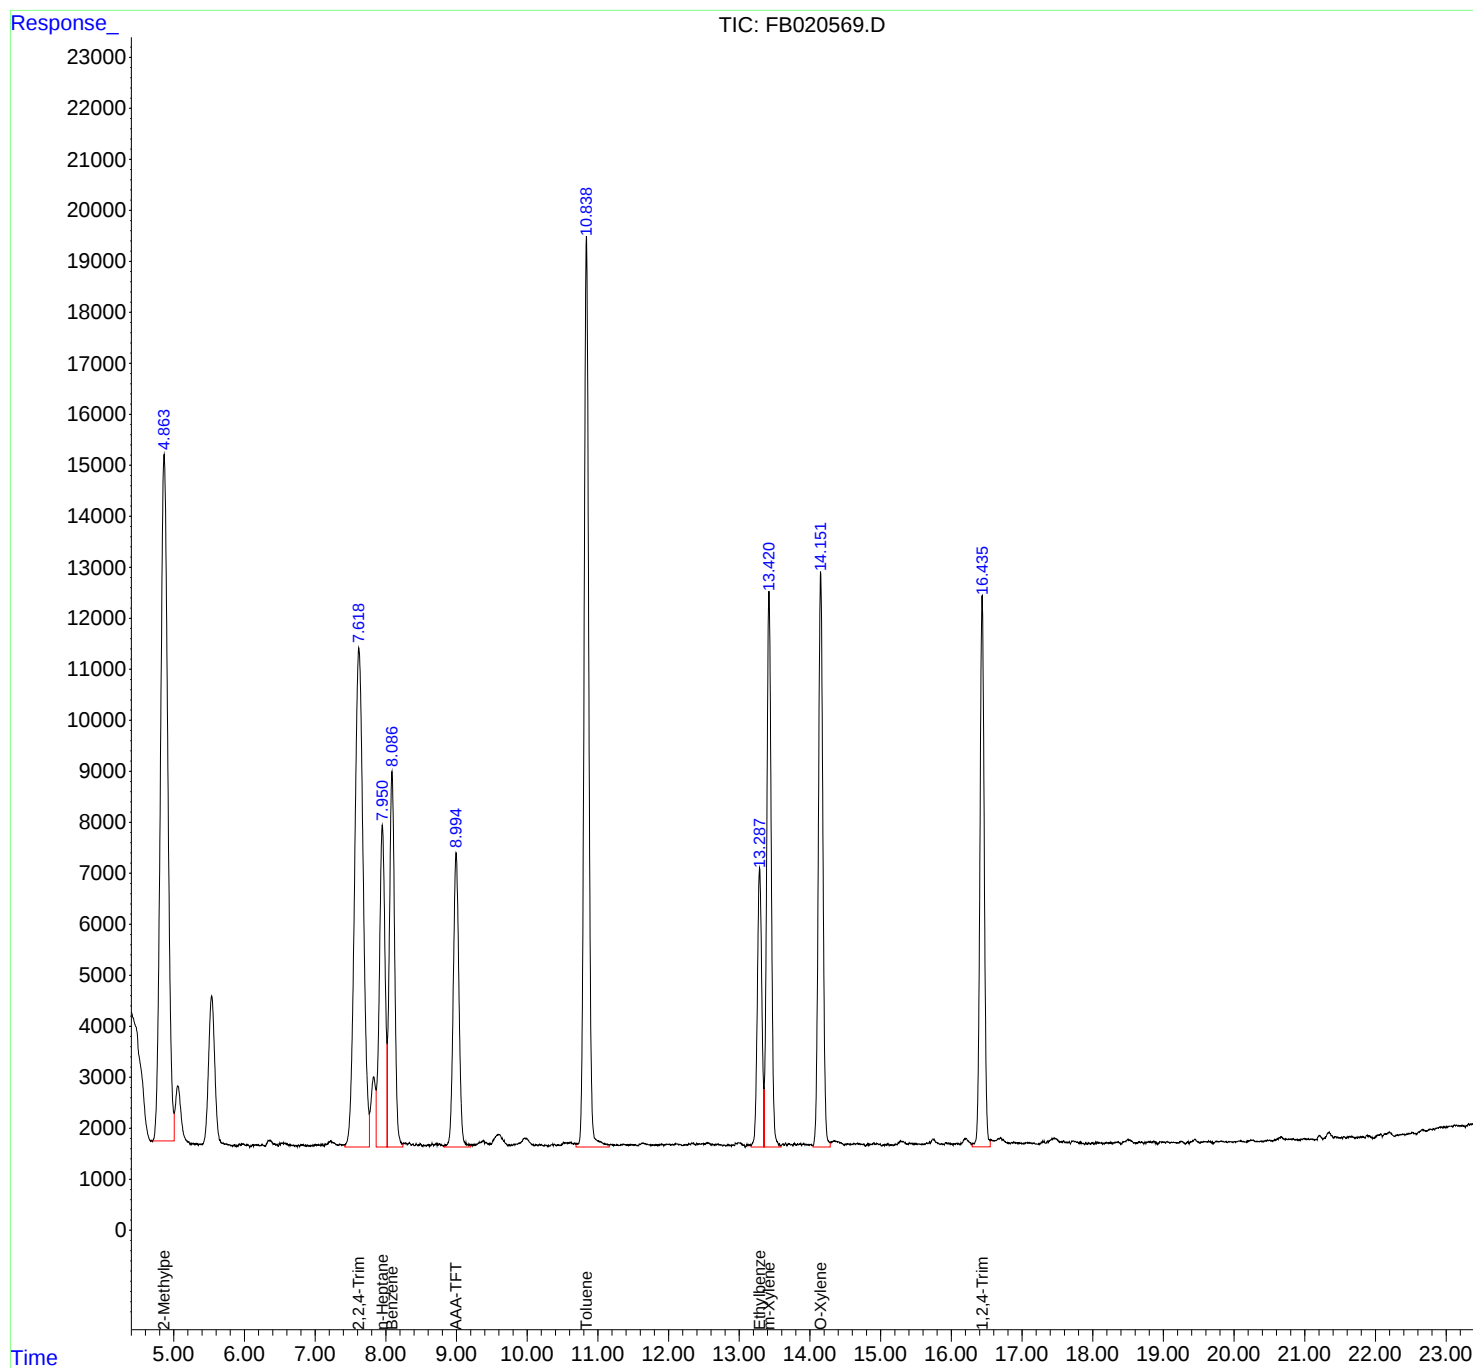


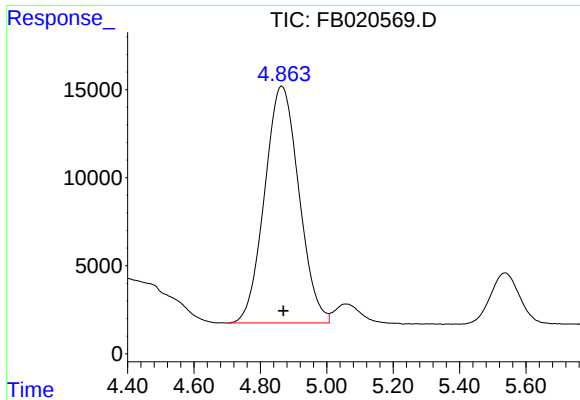

#1 2-Methylpentane


R.T.: 4.865 min
Delta R.T.: -0.004 min
Response: 965249
Conc: 27.42 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MSD

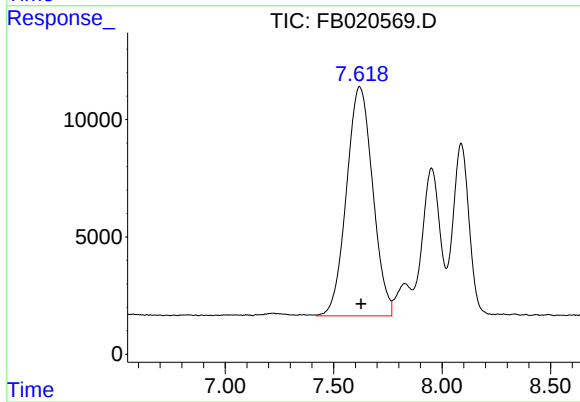


#2 2,2,4-Trimethylpentane

R.T.: 7.620 min
Delta R.T.: -0.007 min
Response: 821381
Conc: 27.55 ng/ml

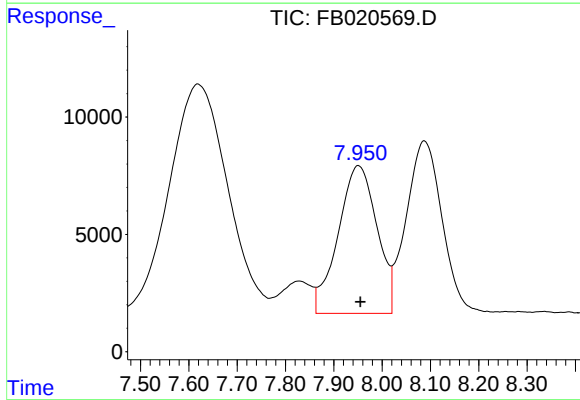


#3 n-Heptane

R.T.: 7.952 min
Delta R.T.: -0.003 min
Response: 351644
Conc: 8.96 ng/ml

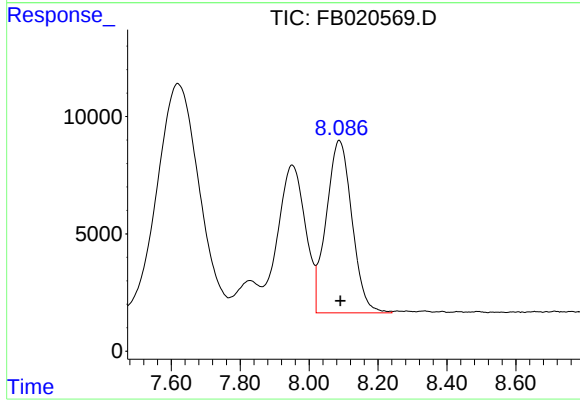

#4 Benzene


R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 381362
Conc: 9.28 ng/ml

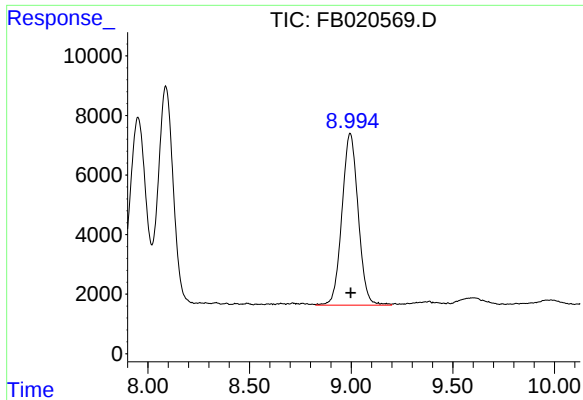

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 319459
Conc: 17.32 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MSD

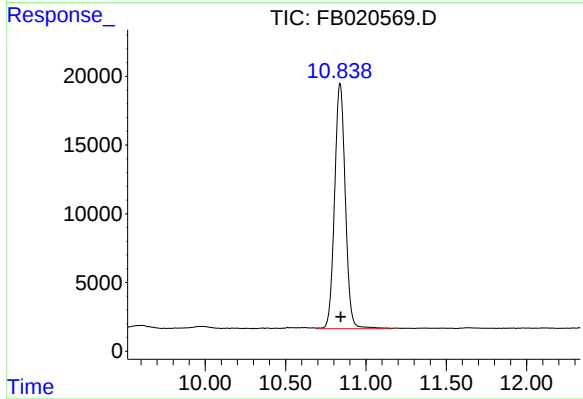


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 830204
Conc: 27.48 ng/ml

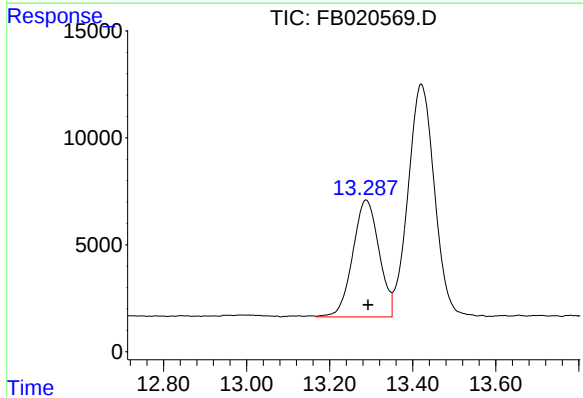


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.004 min
Response: 239632
Conc: 9.37 ng/ml

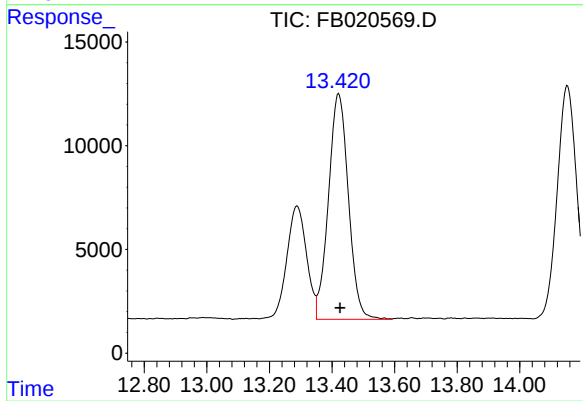

#8 m-Xylene


R.T.: 13.421 min
Delta R.T.: -0.004 min
Response: 482097
Conc: 18.24 ng/ml

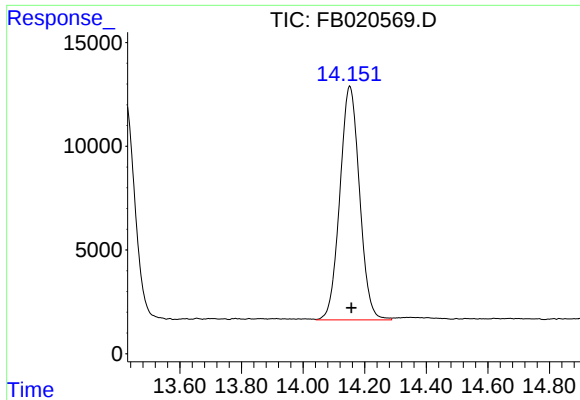

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: -0.004 min
Response: 499737
Conc: 18.46 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MSD

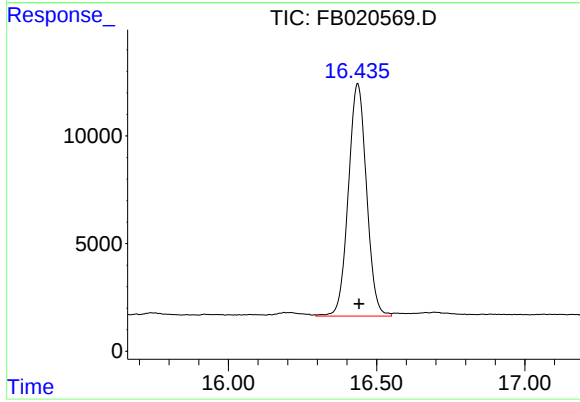

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.004 min
Response: 459606
Conc: 17.59 ng/ml