

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020571.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 7:32
 Operator : MJ/SJ
 Sample : K2294-02
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-14-S2

Integration File: SAMPLE.e
 Quant Time: Apr 08 05:30:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.996	292113	15.837 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.879	1458	0.041 ng/ml
2) t 2,2,4-Trimethylpentane	7.621	2211	0.074 ng/ml
3) t n-Heptane	7.954	2887	0.074 ng/ml
4) t Benzene	8.090	4436	0.108 ng/ml
6) t Toluene	10.844	4657	0.154 ng/ml
7) t Ethylbenzene	13.295	1564	0.061 ng/ml
8) t m-Xylene	13.403	2972	0.112 ng/ml
9) t O-Xylene	14.144	1857	0.069 ng/ml
10) t 1,2,4-Trimethylbenzene	16.434	561	0.021 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020571.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 7:32
Operator : MJ/SJ
Sample : K2294-02
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-14-S2

Integration File: SAMPLE.e
Quant Time: Apr 08 05:30:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

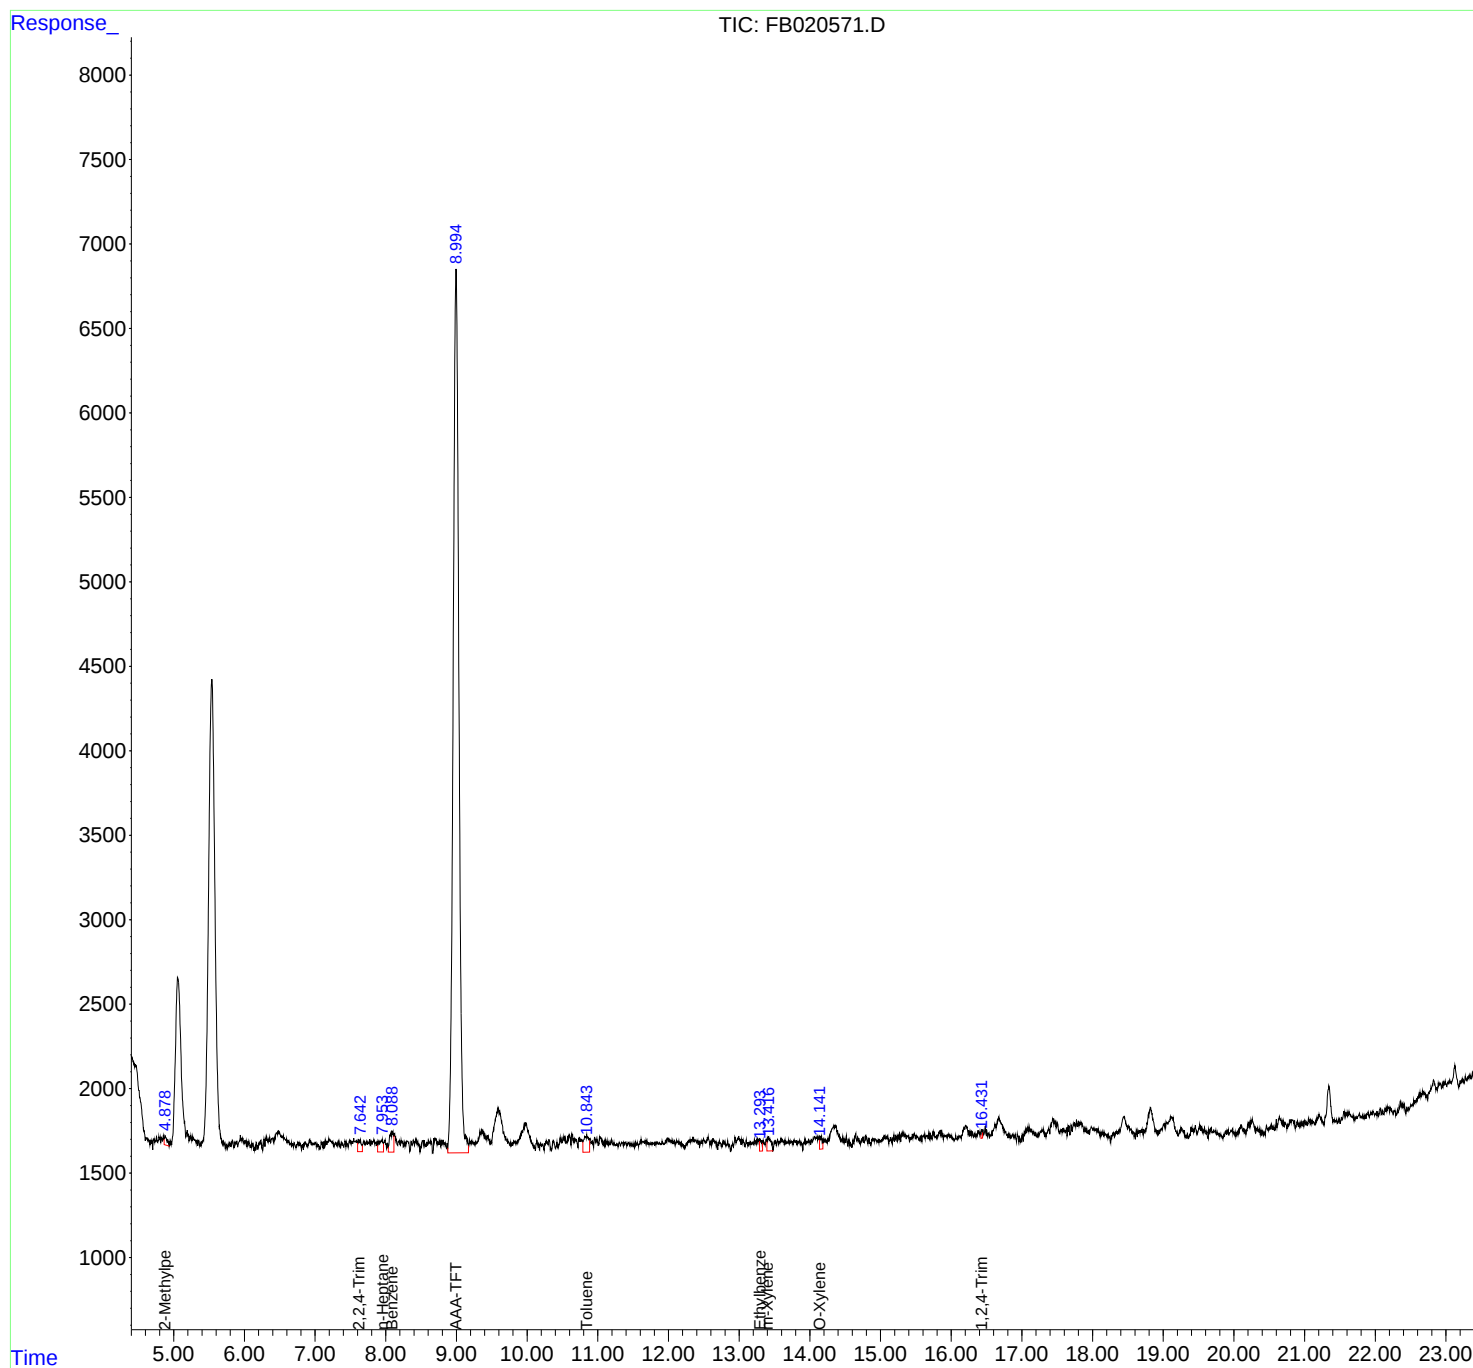


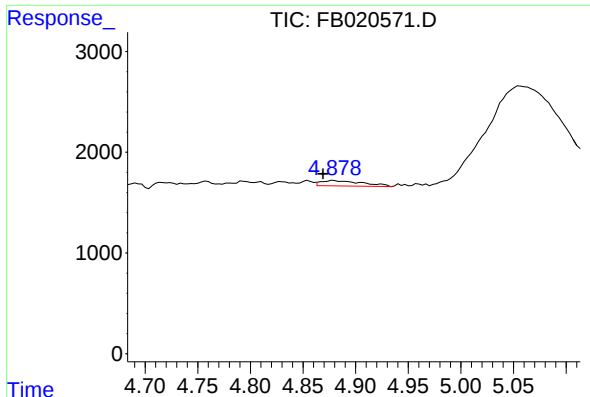

#1 2-Methylpentane


R.T.: 4.879 min
Delta R.T.: 0.010 min
Response: 1458
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-S2

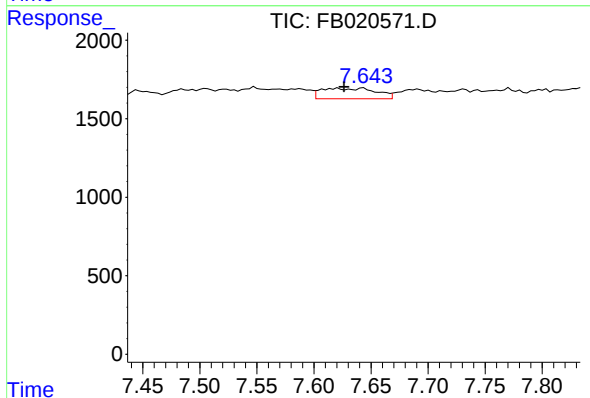


#2 2,2,4-Trimethylpentane

R.T.: 7.621 min
Delta R.T.: -0.006 min
Response: 2211
Conc: 0.07 ng/ml

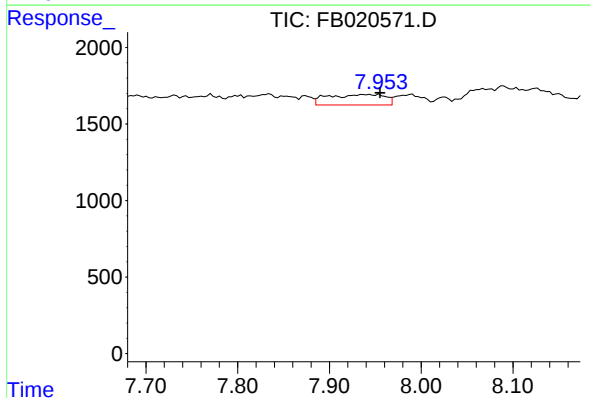


#3 n-Heptane

R.T.: 7.954 min
Delta R.T.: -0.001 min
Response: 2887
Conc: 0.07 ng/ml

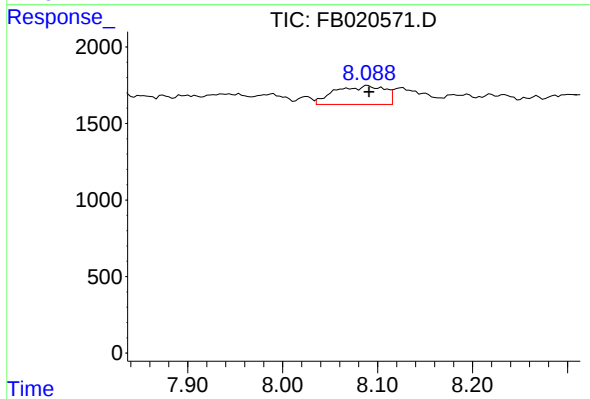

#4 Benzene


R.T.: 8.090 min
Delta R.T.: -0.001 min
Response: 4436
Conc: 0.11 ng/ml

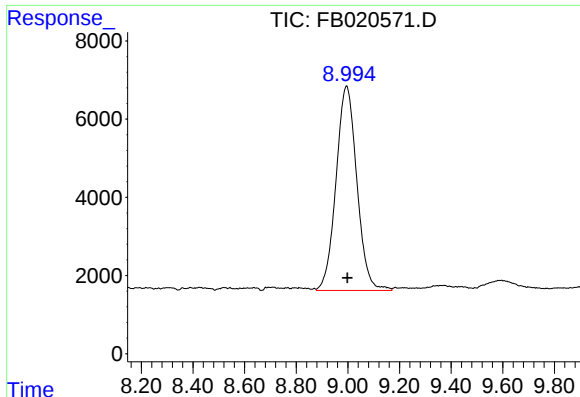

#5 AAA-TFT


R.T.: 8.996 min
Delta R.T.: -0.003 min
Response: 292113
Conc: 15.84 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-S2

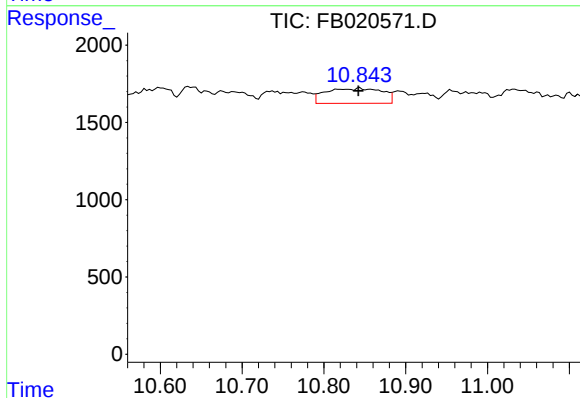


#6 Toluene

R.T.: 10.844 min
Delta R.T.: 0.002 min
Response: 4657
Conc: 0.15 ng/ml

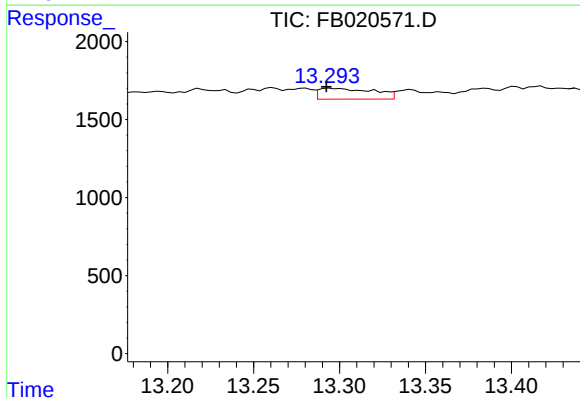


#7 Ethylbenzene

R.T.: 13.295 min
Delta R.T.: 0.003 min
Response: 1564
Conc: 0.06 ng/ml

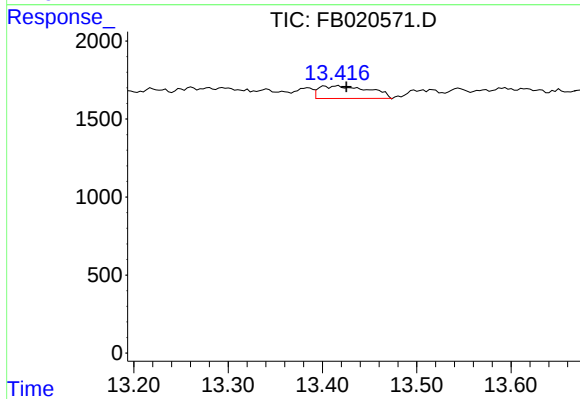

#8 m-Xylene


R.T.: 13.403 min
Delta R.T.: -0.023 min
Response: 2972
Conc: 0.11 ng/ml

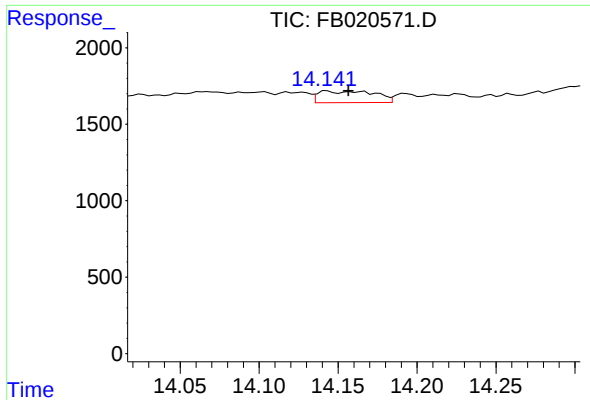

#9 O-Xylene

R.T.: 14.144 min
Delta R.T.: -0.013 min
Response: 1857
Conc: 0.07 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-S2

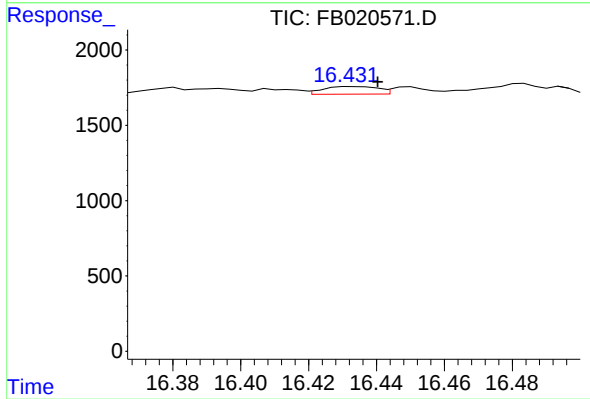

#10 1,2,4-Trimethylbenzene

R.T.: 16.434 min
Delta R.T.: -0.007 min
Response: 561
Conc: 0.02 ng/ml