

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020572.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 8:02
 Operator : MJ/SJ
 Sample : K2294-05
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-14-D1

Integration File: SAMPLE.e
 Quant Time: Apr 08 05:30:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	285419	15.475 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.854	2225	0.063 ng/ml
2) t 2,2,4-Trimethylpentane	7.614	2465	0.083 ng/ml
3) t n-Heptane	7.950	1321	0.034 ng/ml
4) t Benzene	8.099	892	0.022 ng/ml
6) t Toluene	10.827	2146	0.071 ng/ml
7) t Ethylbenzene	13.284	6090	0.238 ng/ml
8) t m-Xylene	13.439	948	0.036 ng/ml
9) t O-Xylene	14.167	779	0.029 ng/ml
10) t 1,2,4-Trimethylbenzene	16.419	1002	0.038 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020572.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 8:02
Operator : MJ/SJ
Sample : K2294-05
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-14-D1

Integration File: SAMPLE.e
Quant Time: Apr 08 05:30:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

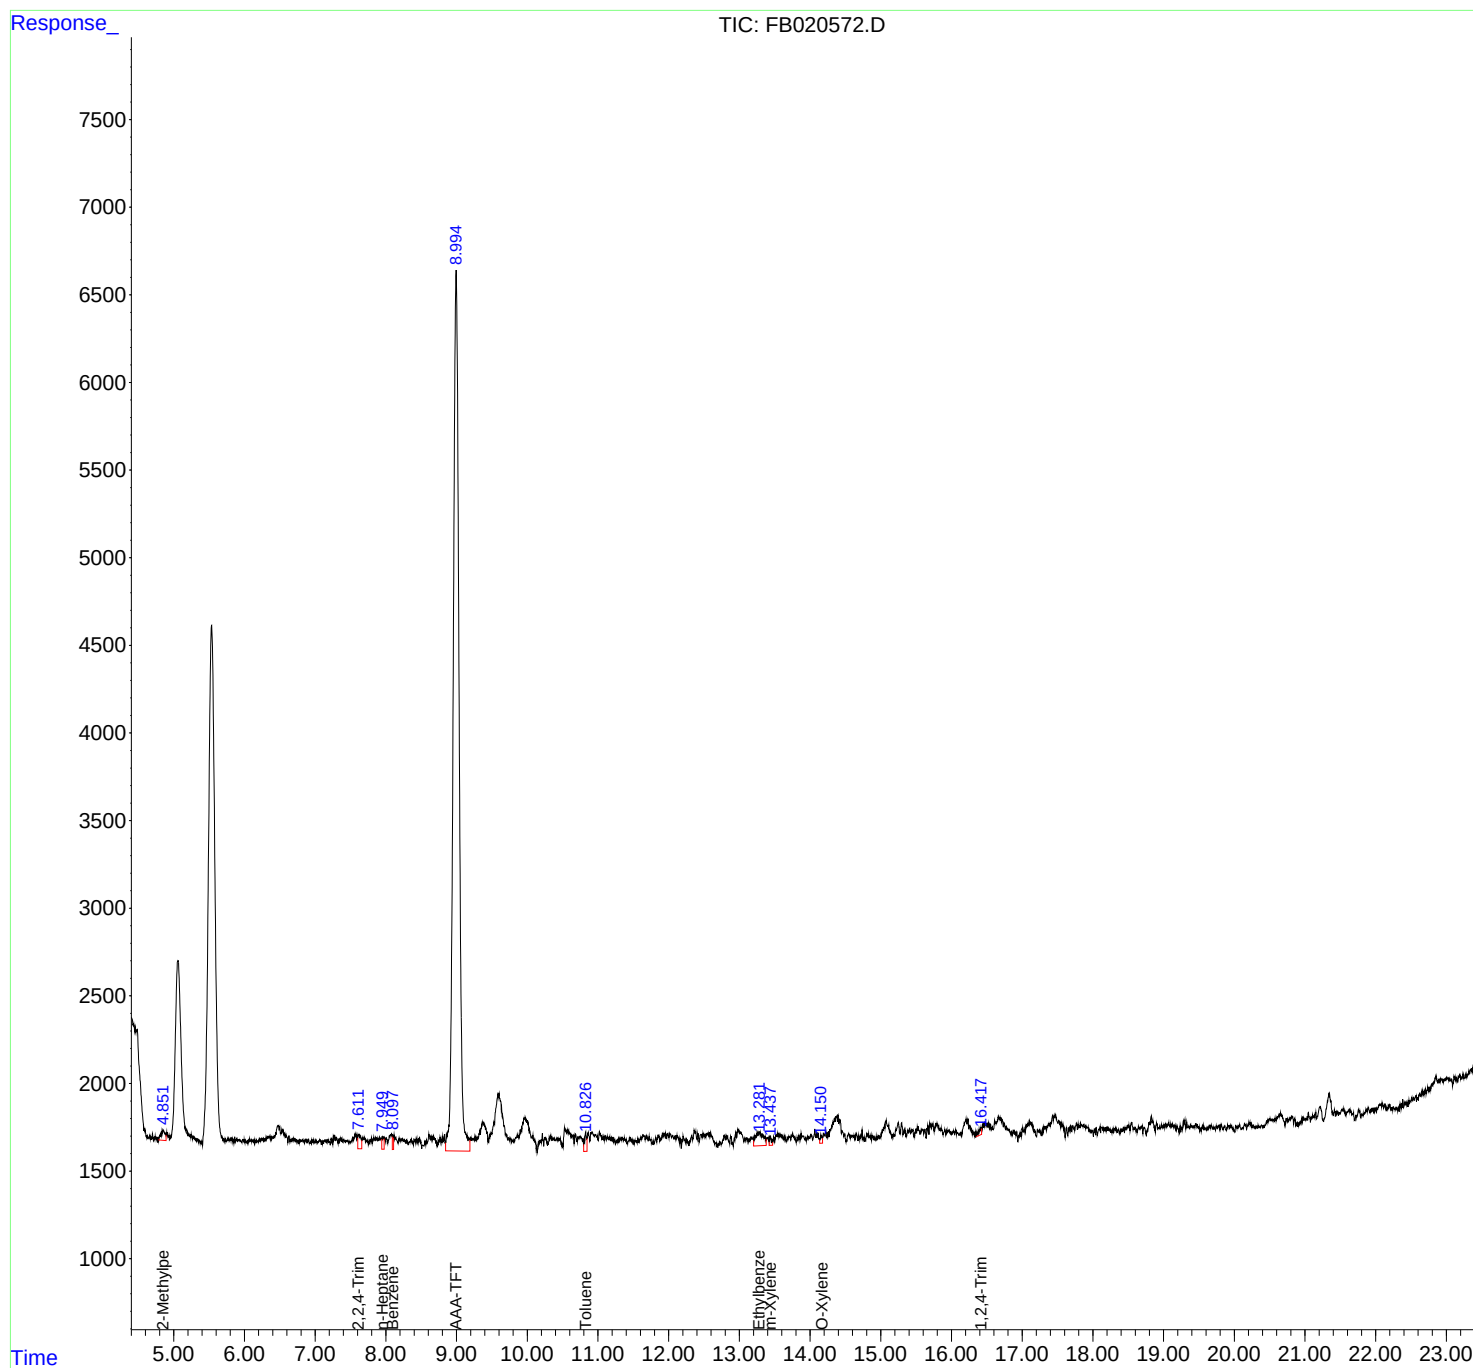


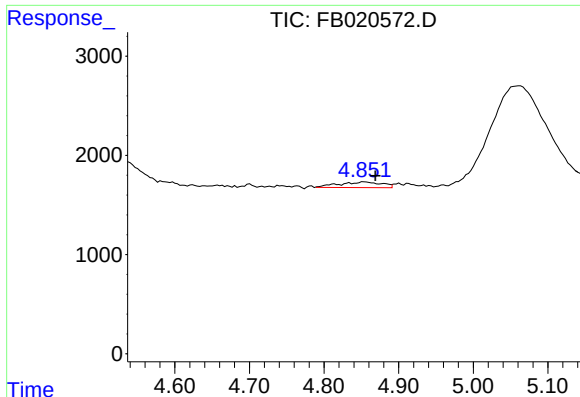

#1 2-Methylpentane


R.T.: 4.854 min
Delta R.T.: -0.015 min
Response: 2225
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D1

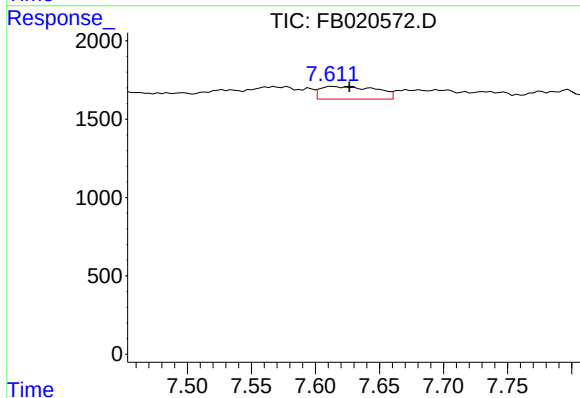


#2 2,2,4-Trimethylpentane

R.T.: 7.614 min
Delta R.T.: -0.013 min
Response: 2465
Conc: 0.08 ng/ml

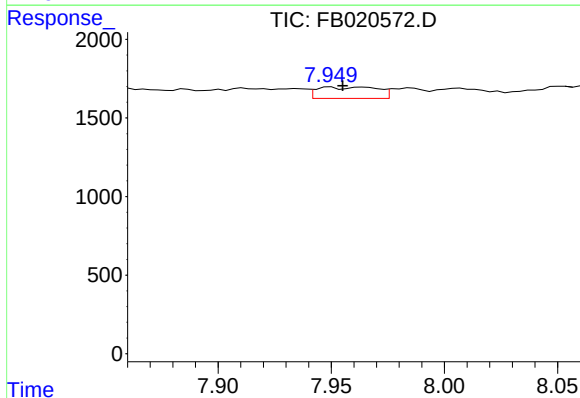


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 1321
Conc: 0.03 ng/ml

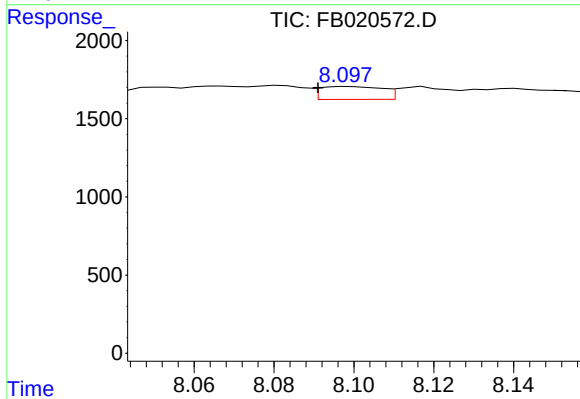

#4 Benzene


R.T.: 8.099 min
Delta R.T.: 0.008 min
Response: 892
Conc: 0.02 ng/ml

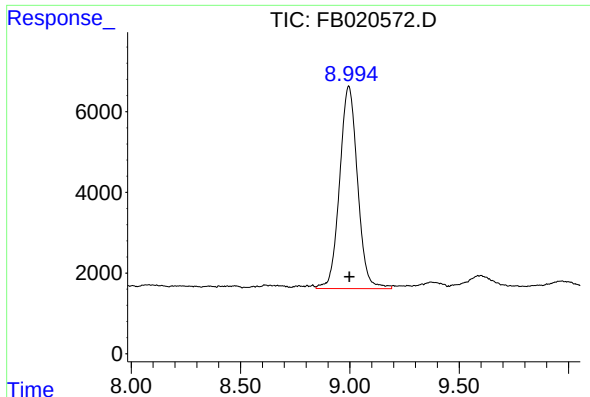

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: -0.003 min
Response: 285419
Conc: 15.47 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D1

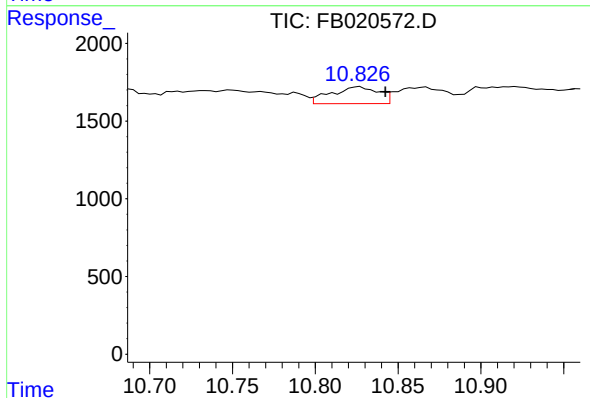


#6 Toluene

R.T.: 10.827 min
Delta R.T.: -0.016 min
Response: 2146
Conc: 0.07 ng/ml

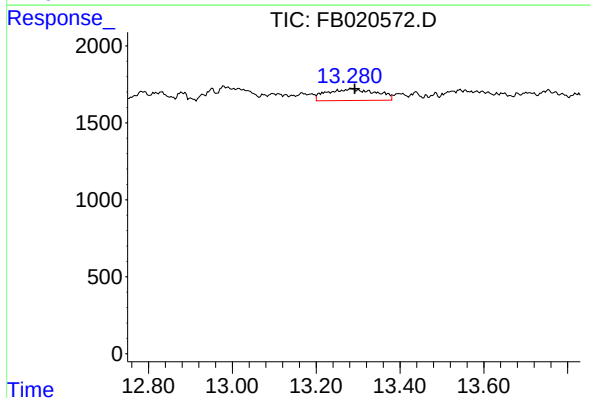


#7 Ethylbenzene

R.T.: 13.284 min
Delta R.T.: -0.008 min
Response: 6090
Conc: 0.24 ng/ml

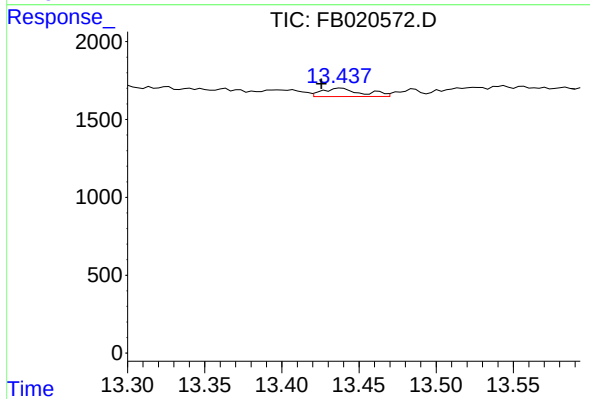

#8 m-Xylene


R.T.: 13.439 min
Delta R.T.: 0.013 min
Response: 948
Conc: 0.04 ng/ml

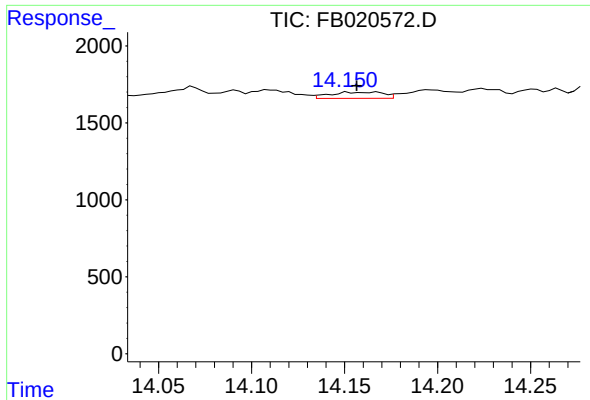

#9 O-Xylene

R.T.: 14.167 min
Delta R.T.: 0.011 min
Response: 779
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D1

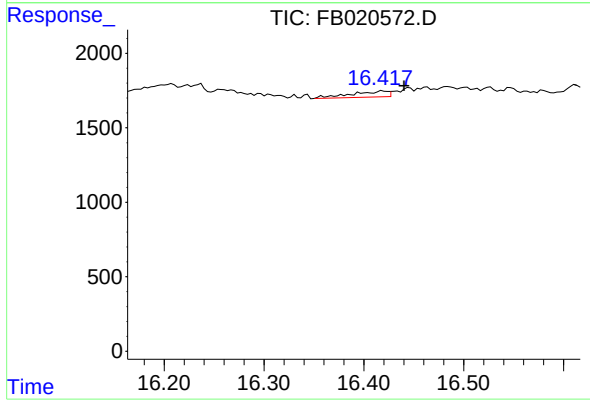

#10 1,2,4-Trimethylbenzene

R.T.: 16.419 min
Delta R.T.: -0.021 min
Response: 1002
Conc: 0.04 ng/ml