

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020573.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 8:32
 Operator : MJ/SJ
 Sample : K2294-06
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 TP-14-D2

Integration File: SAMPLE.e
 Quant Time: Apr 08 05:31:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	167133	9.061 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.867	2729	0.078 ng/ml
2) t 2,2,4-Trimethylpentane	7.624	2093	0.070 ng/ml
3) t n-Heptane	7.949	2137	0.054 ng/ml
4) t Benzene	8.098	1375	0.033 ng/ml
6) t Toluene	10.852	1701	0.056 ng/ml
7) t Ethylbenzene	13.310	1345	0.053 ng/ml
8) t m-Xylene	13.444	2476	0.094 ng/ml
9) t O-Xylene	14.165	1928	0.071 ng/ml
10) t 1,2,4-Trimethylbenzene	16.478	2213	0.085 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020573.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 8:32
Operator : MJ/SJ
Sample : K2294-06
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
TP-14-D2

Integration File: SAMPLE.e
Quant Time: Apr 08 05:31:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

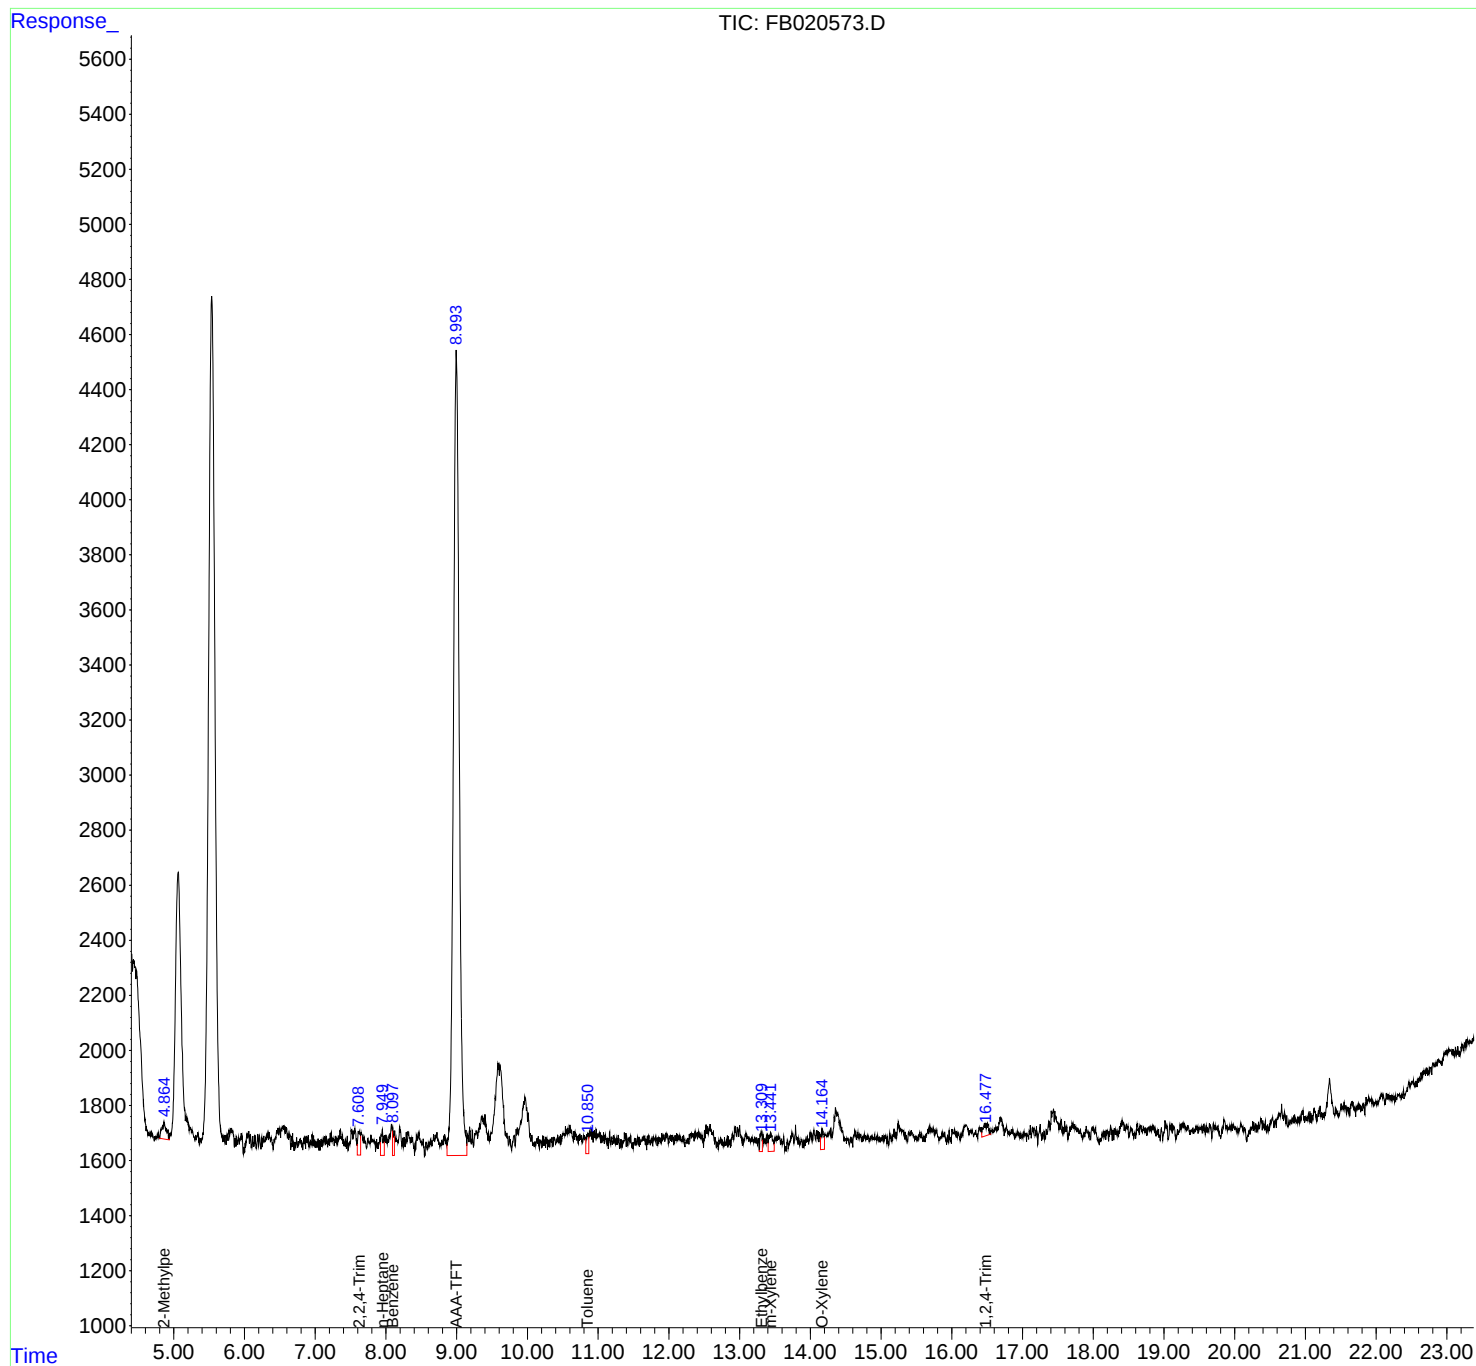


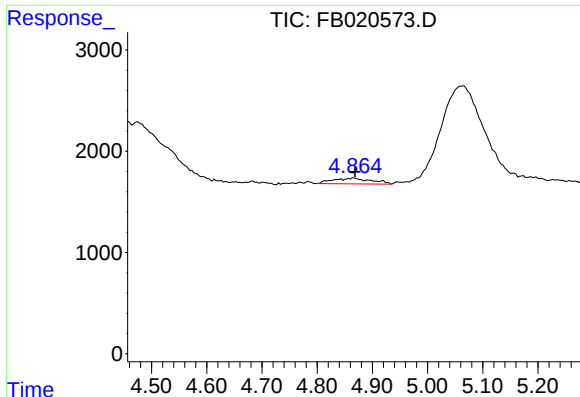

#1 2-Methylpentane


R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 2729
Conc: 0.08 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D2

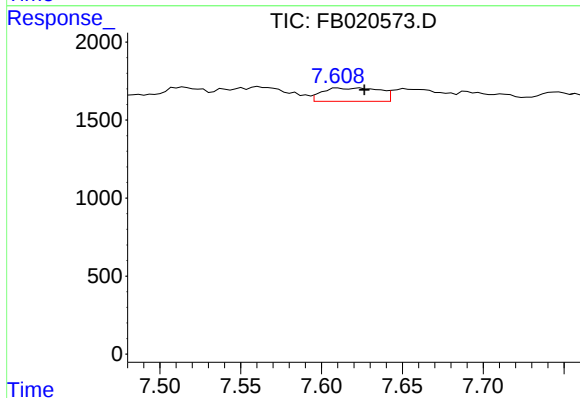


#2 2,2,4-Trimethylpentane

R.T.: 7.624 min
Delta R.T.: -0.003 min
Response: 2093
Conc: 0.07 ng/ml

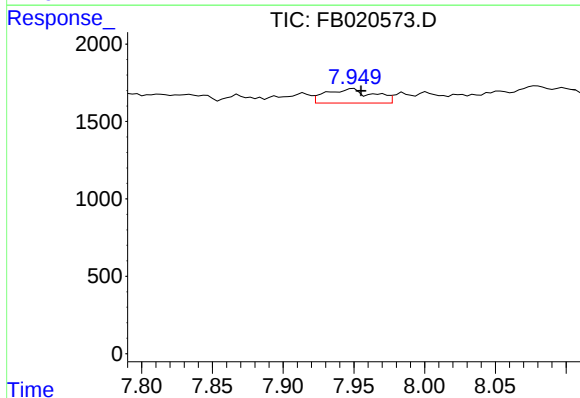


#3 n-Heptane

R.T.: 7.949 min
Delta R.T.: -0.006 min
Response: 2137
Conc: 0.05 ng/ml

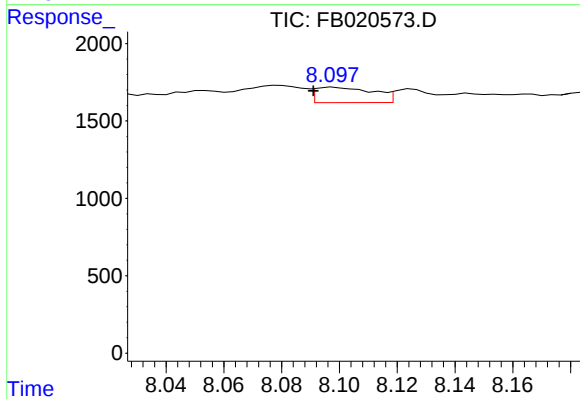

#4 Benzene


R.T.: 8.098 min
Delta R.T.: 0.007 min
Response: 1375
Conc: 0.03 ng/ml

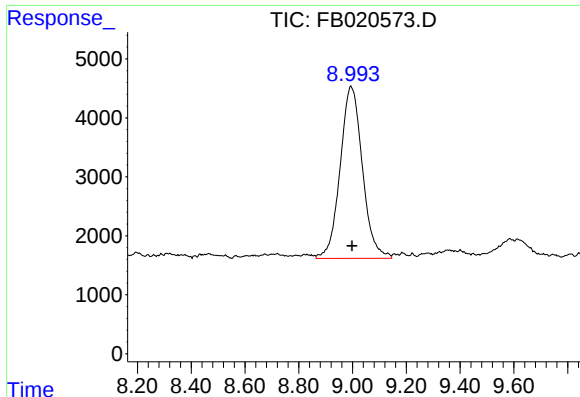

#5 AAA-TFT


R.T.: 8.994 min
Delta R.T.: -0.004 min
Response: 167133
Conc: 9.06 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D2

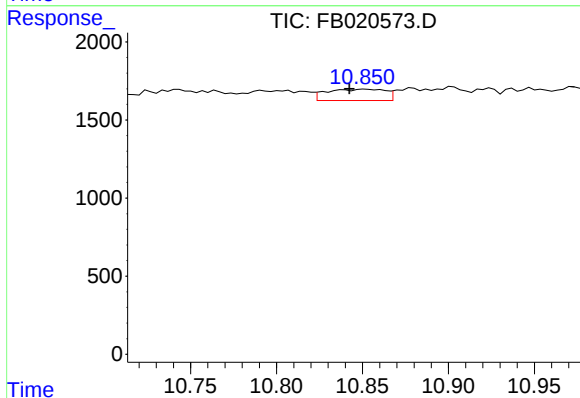


#6 Toluene

R.T.: 10.852 min
Delta R.T.: 0.010 min
Response: 1701
Conc: 0.06 ng/ml

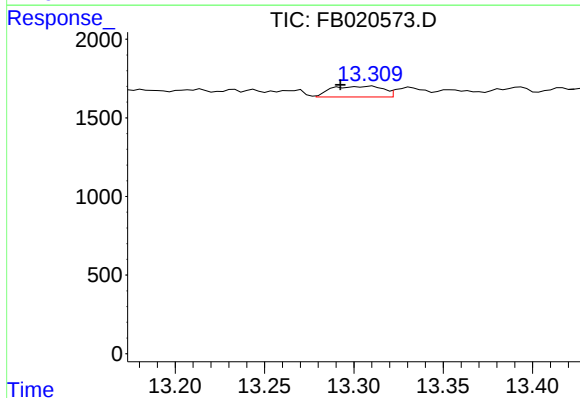


#7 Ethylbenzene

R.T.: 13.310 min
Delta R.T.: 0.017 min
Response: 1345
Conc: 0.05 ng/ml

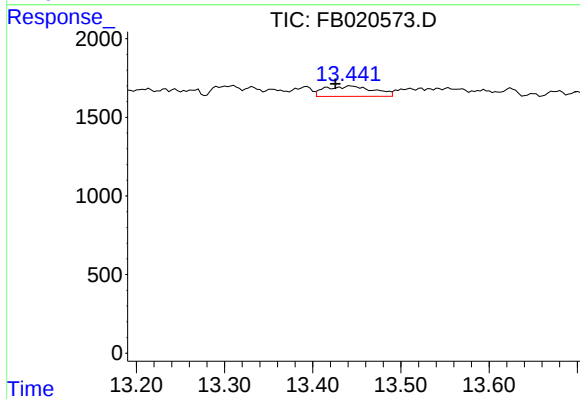

#8 m-Xylene


R.T.: 13.444 min
Delta R.T.: 0.018 min
Response: 2476
Conc: 0.09 ng/ml

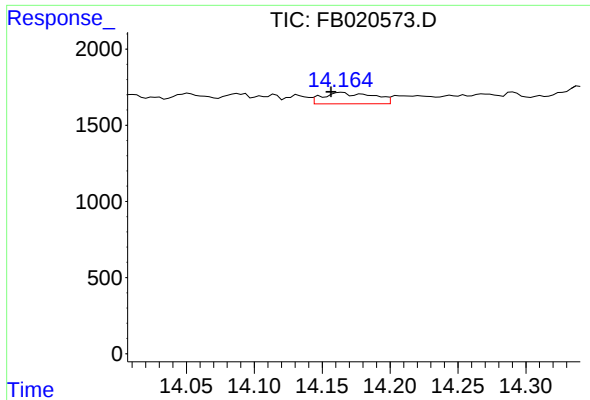

#9 O-Xylene

R.T.: 14.165 min
Delta R.T.: 0.008 min
Response: 1928
Conc: 0.07 ng/ml

Instrument :
FID_B
ClientSampleId :
TP-14-D2

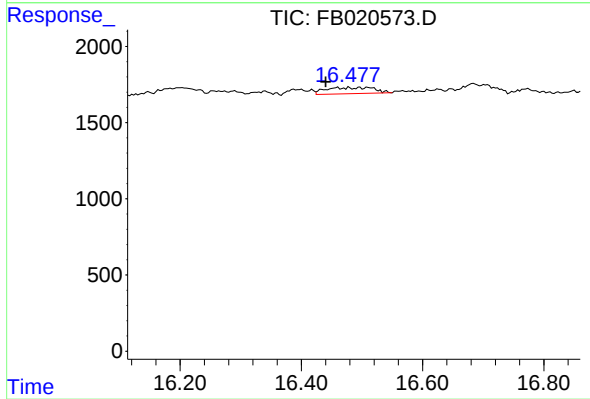

#10 1,2,4-Trimethylbenzene

R.T.: 16.478 min
Delta R.T.: 0.038 min
Response: 2213
Conc: 0.08 ng/ml