

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
 Data File : FB020568.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2019 6:02
 Operator : MJ/SJ
 Sample : K2257-33MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 RO-20MS

Integration File: Calibration.e
 Quant Time: Apr 08 05:30:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	324906	17.615 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	983946	27.950 ng/ml
2) t 2,2,4-Trimethylpentane	7.620	866394	29.060 ng/ml
3) t n-Heptane	7.950	371820	9.472 ng/ml
4) t Benzene	8.087	381902	9.298 ng/ml
6) t Toluene	10.839	821116	27.175 ng/ml
7) t Ethylbenzene	13.289	239872	9.377 ng/ml
8) t m-Xylene	13.422	484038	18.314 ng/ml
9) t O-Xylene	14.153	495377	18.299 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	463980	17.759 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040519\
Data File : FB020568.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2019 6:02
Operator : MJ/SJ
Sample : K2257-33MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
RO-20MS

Integration File: Calibration.e
Quant Time: Apr 08 05:30:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

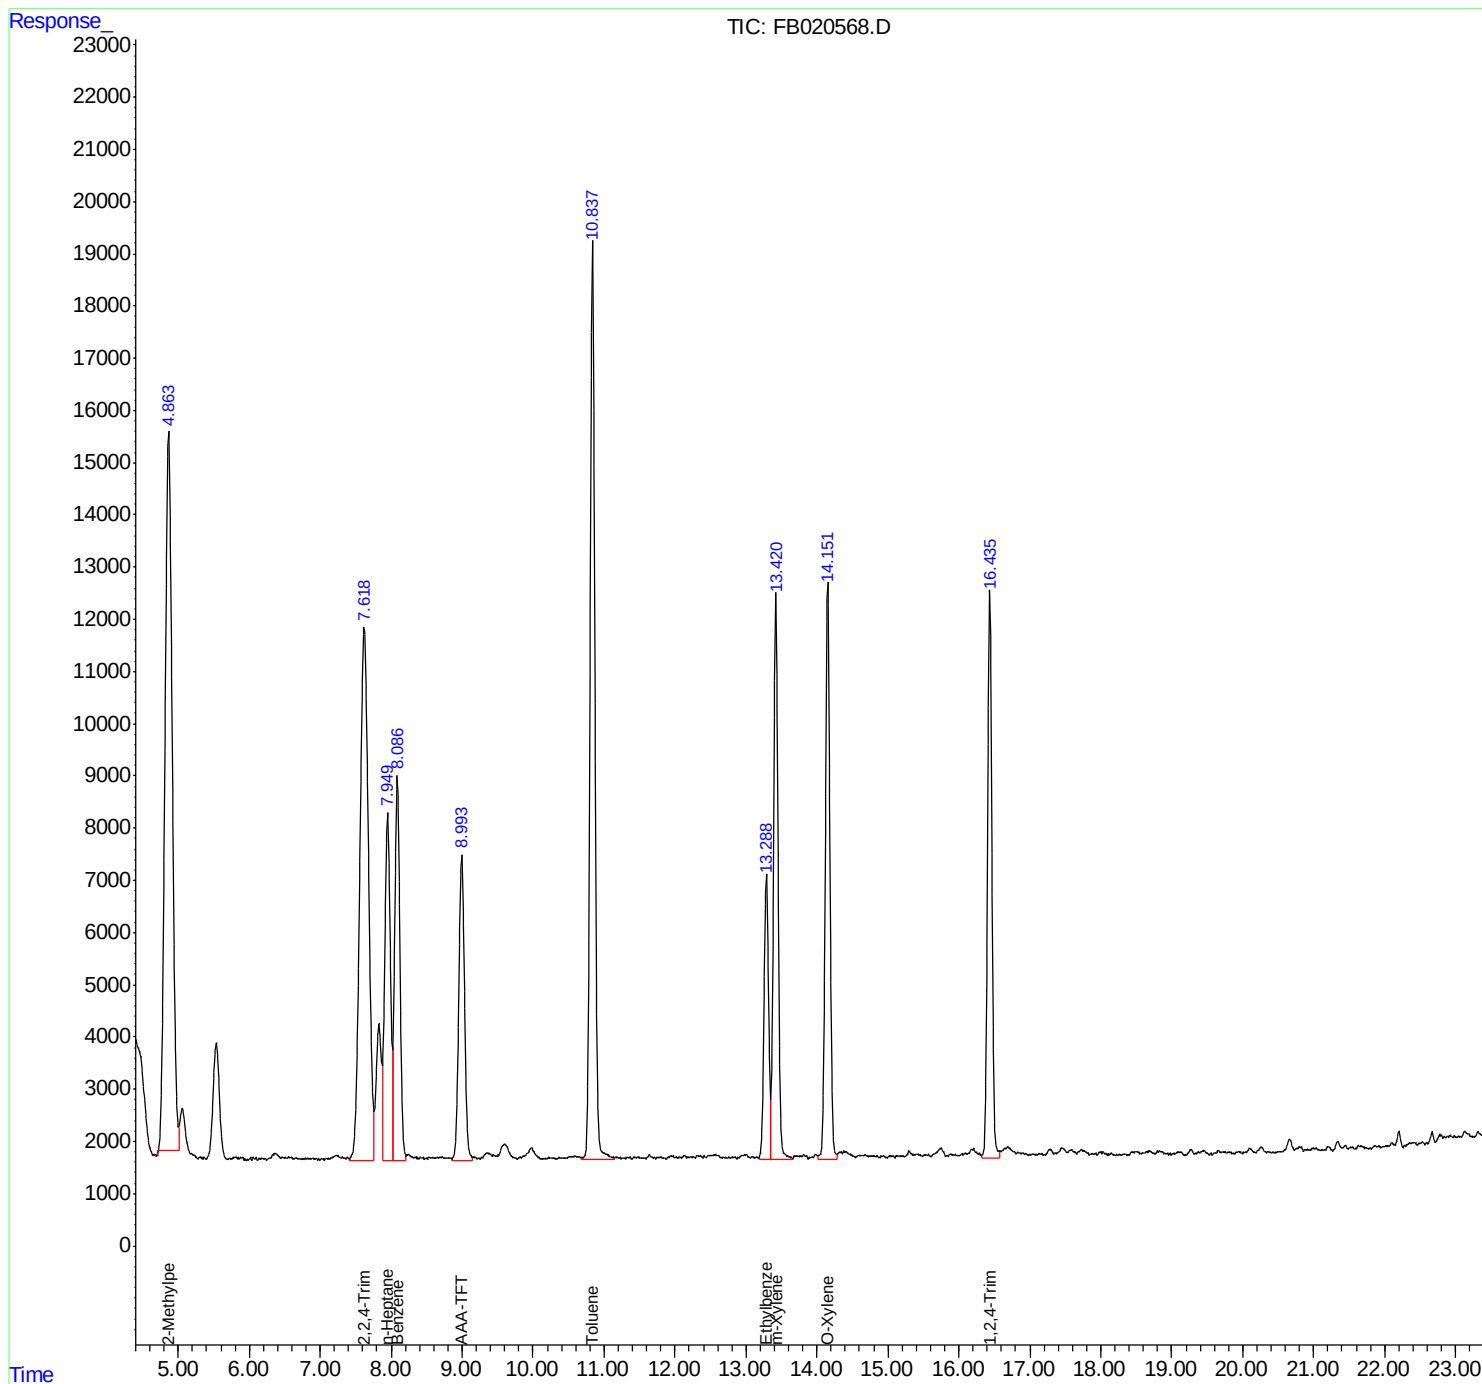


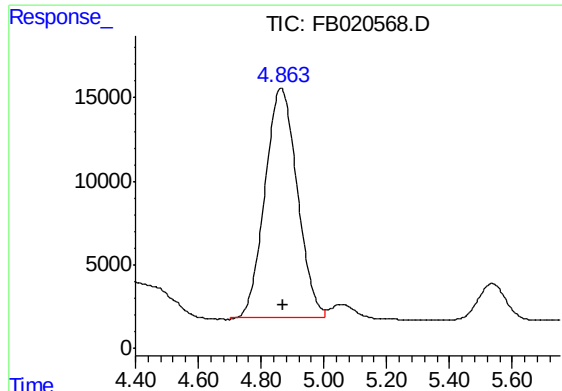

#1 2-Methylpentane


R.T.: 4.864 min
Delta R.T.: -0.005 min
Response: 983946
Conc: 27.95 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MS

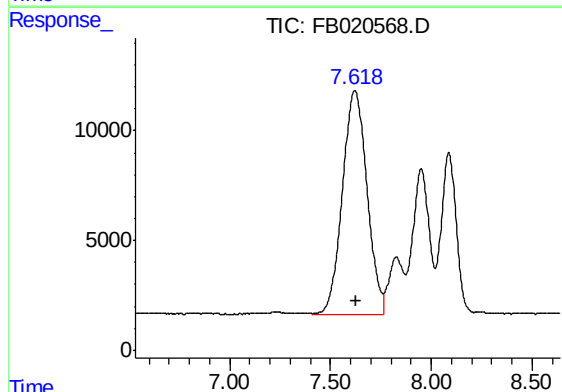


#2 2,2,4-Trimethylpentane

R.T.: 7.620 min
Delta R.T.: -0.007 min
Response: 866394
Conc: 29.06 ng/ml

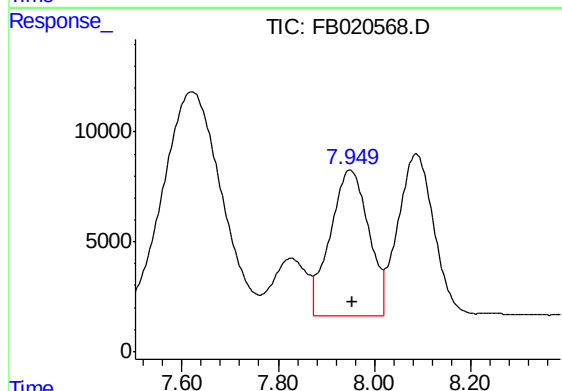


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 371820
Conc: 9.47 ng/ml

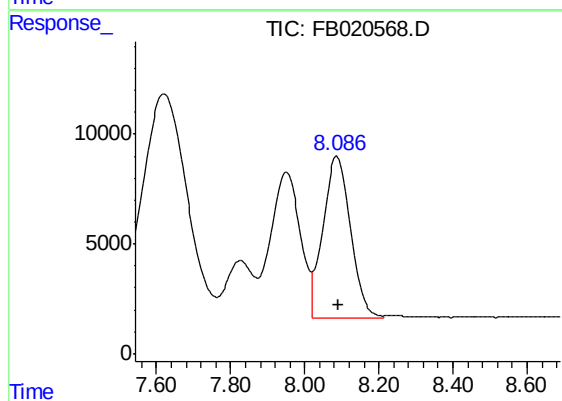

#4 Benzene


R.T.: 8.087 min
Delta R.T.: -0.004 min
Response: 381902
Conc: 9.30 ng/ml

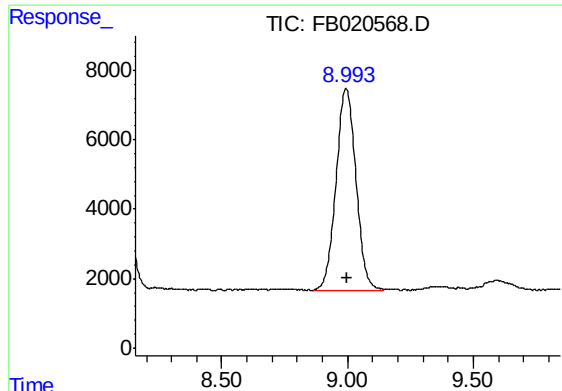

#5 AAA-TFT


R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 324906
Conc: 17.62 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MS

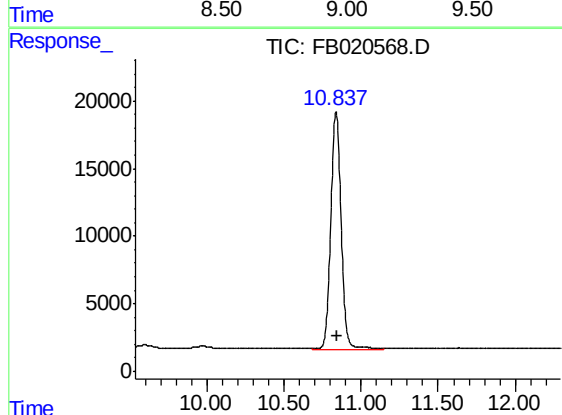


#6 Toluene

R.T.: 10.839 min
Delta R.T.: -0.004 min
Response: 821116
Conc: 27.17 ng/ml

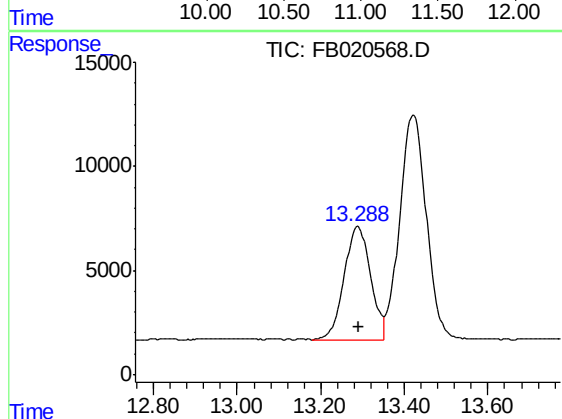


#7 Ethylbenzene

R.T.: 13.289 min
Delta R.T.: -0.003 min
Response: 239872
Conc: 9.38 ng/ml

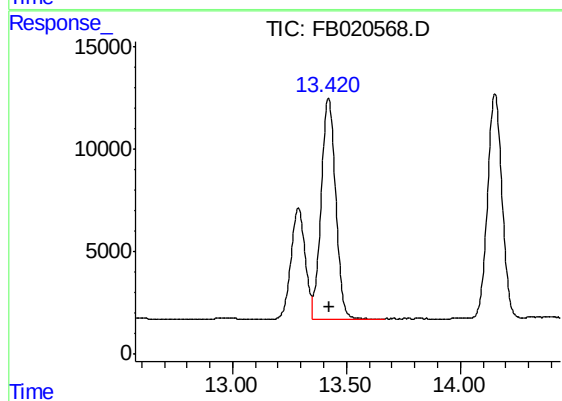

#8 m-Xylene


R.T.: 13.422 min
Delta R.T.: -0.004 min
Response: 484038
Conc: 18.31 ng/ml

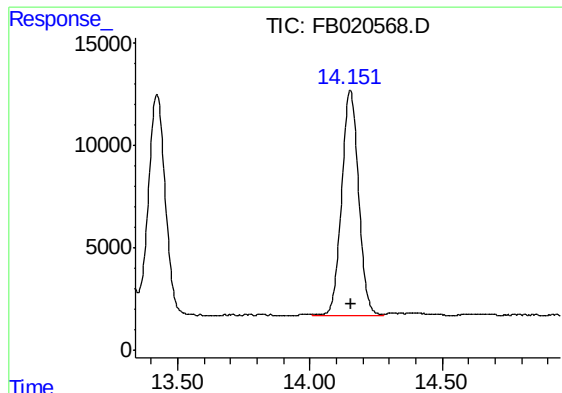

#9 O-Xylene

R.T.: 14.153 min
Delta R.T.: -0.004 min
Response: 495377
Conc: 18.30 ng/ml

Instrument :
FID_B
ClientSampleId :
RO-20MS

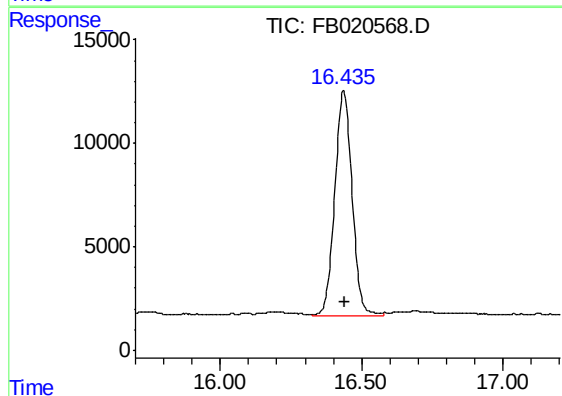

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.004 min
Response: 463980
Conc: 17.76 ng/ml