

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
Data File : FB026827.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2022 13:41
Operator : AJ/MA
Sample : N2246-04
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 06 02:14:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

1) t	2-Methylpentane	4.704	596784	31.520 ng/ml
2) t	2,2,4-Trimethylpentane	7.483	6841353	330.064 ng/ml
3) t	n-Heptane	7.778	3327930	168.137 ng/ml
7) t	Ethylbenzene	13.060	194536634	9679.515 ng/ml
9) t	O-Xylene	13.871	209920697	10522.298 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
Data File : FB026827.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2022 13:41
Operator : AJ/MA
Sample : N2246-04
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 06 02:14:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

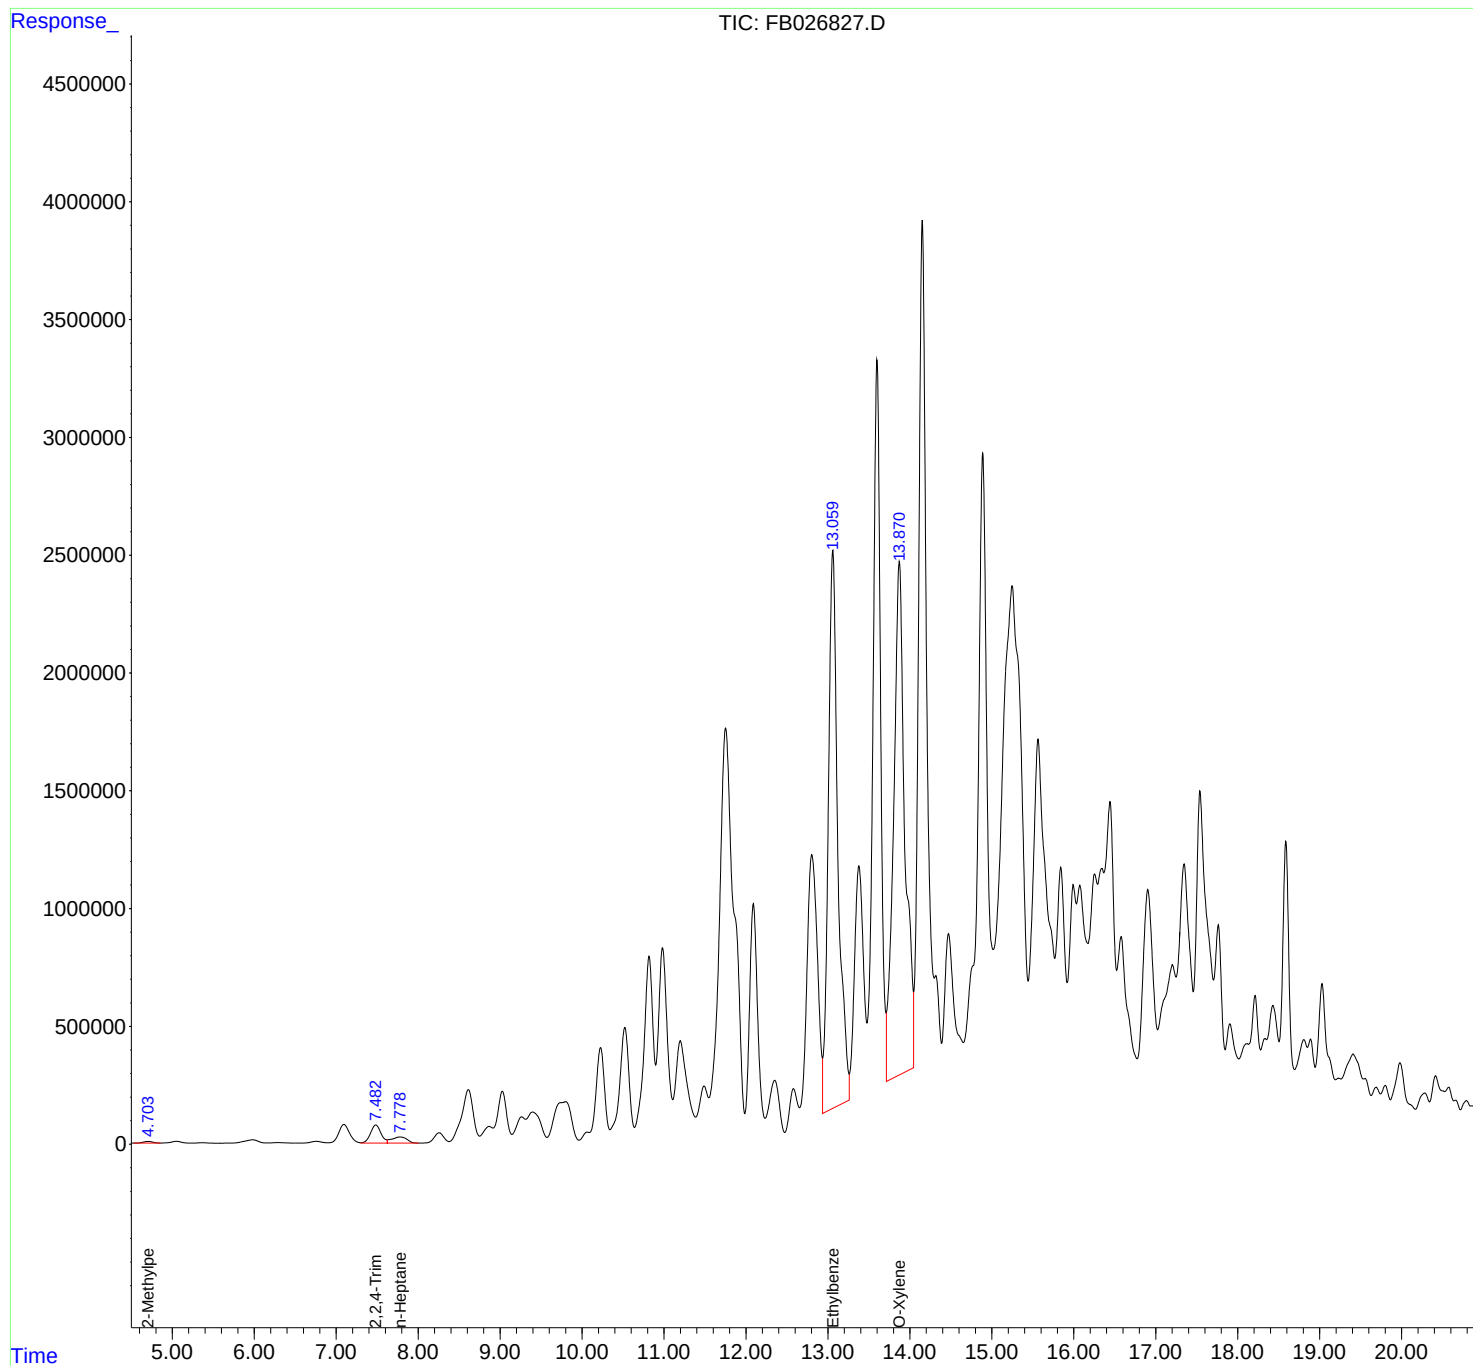


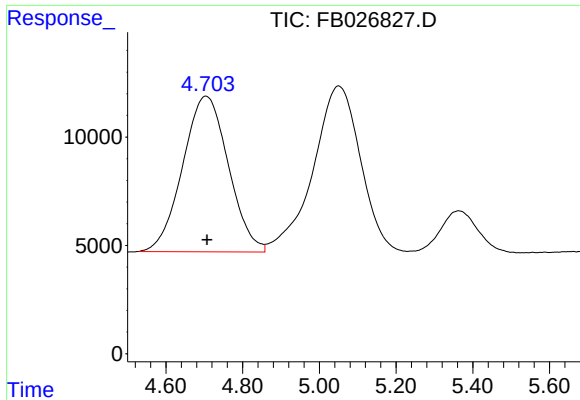

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 596784
Conc: 31.52 ng/ml

Instrument :
FID_B
ClientSampleId :

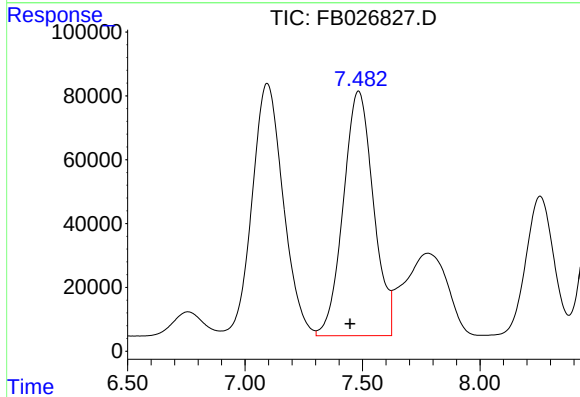


#2 2,2,4-Trimethylpentane

R.T.: 7.483 min
Delta R.T.: 0.036 min
Response: 6841353
Conc: 330.06 ng/ml

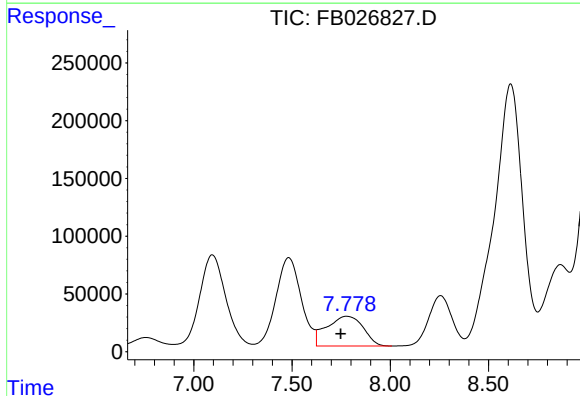


#3 n-Heptane

R.T.: 7.778 min
Delta R.T.: 0.029 min
Response: 3327930
Conc: 168.14 ng/ml

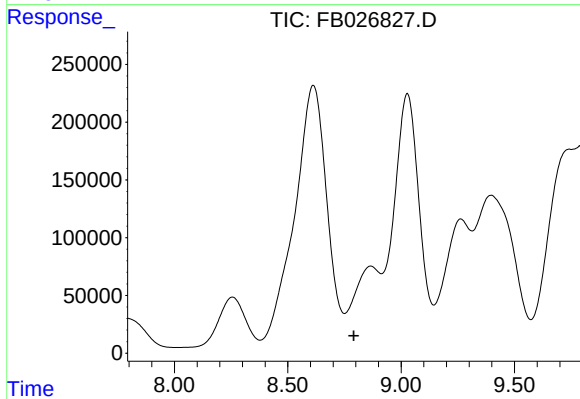

#5 AAA-TFT


R.T.: 0.000 min
Exp R.T. : 8.792 min
Response: 0
Conc: N.D.

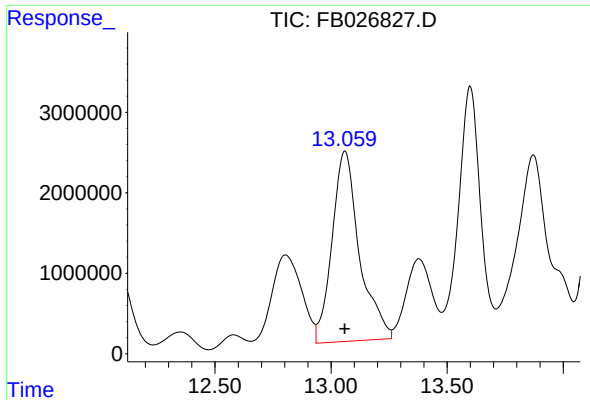

#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: 0.000 min
Response: 194536634
Conc: 9679.51 ng/m

Instrument :
FID_B
ClientSampleId :

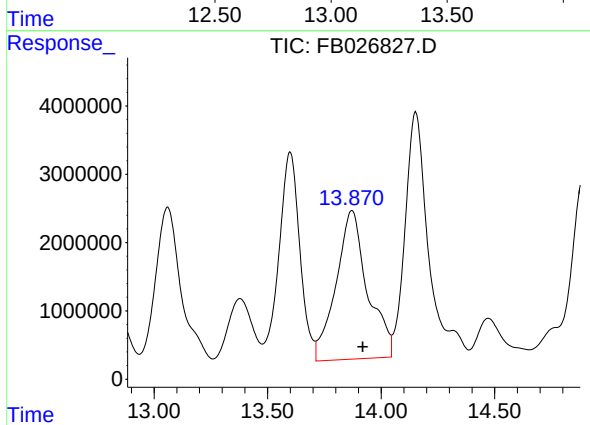

#9 O-Xylene

R.T.: 13.871 min
Delta R.T.: -0.048 min
Response: 209920697
Conc: 10522.30 ng/ml