

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
 Data File : FB026838.D
 Signal(s) : FID2B.CH
 Acq On : 5 Apr 2022 21:14
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 06 02:16:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	327974	31.255 ng/ml
Target Compounds			
3) t n-Heptane	7.757	248	0.013 ng/ml
4) t Benzene	7.908	108	0.005 ng/ml
7) t Ethylbenzene	13.071	31526	1.569 ng/ml
8) t m-Xylene	13.127	30192	1.498 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
Data File : FB026838.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2022 21:14
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 06 02:16:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

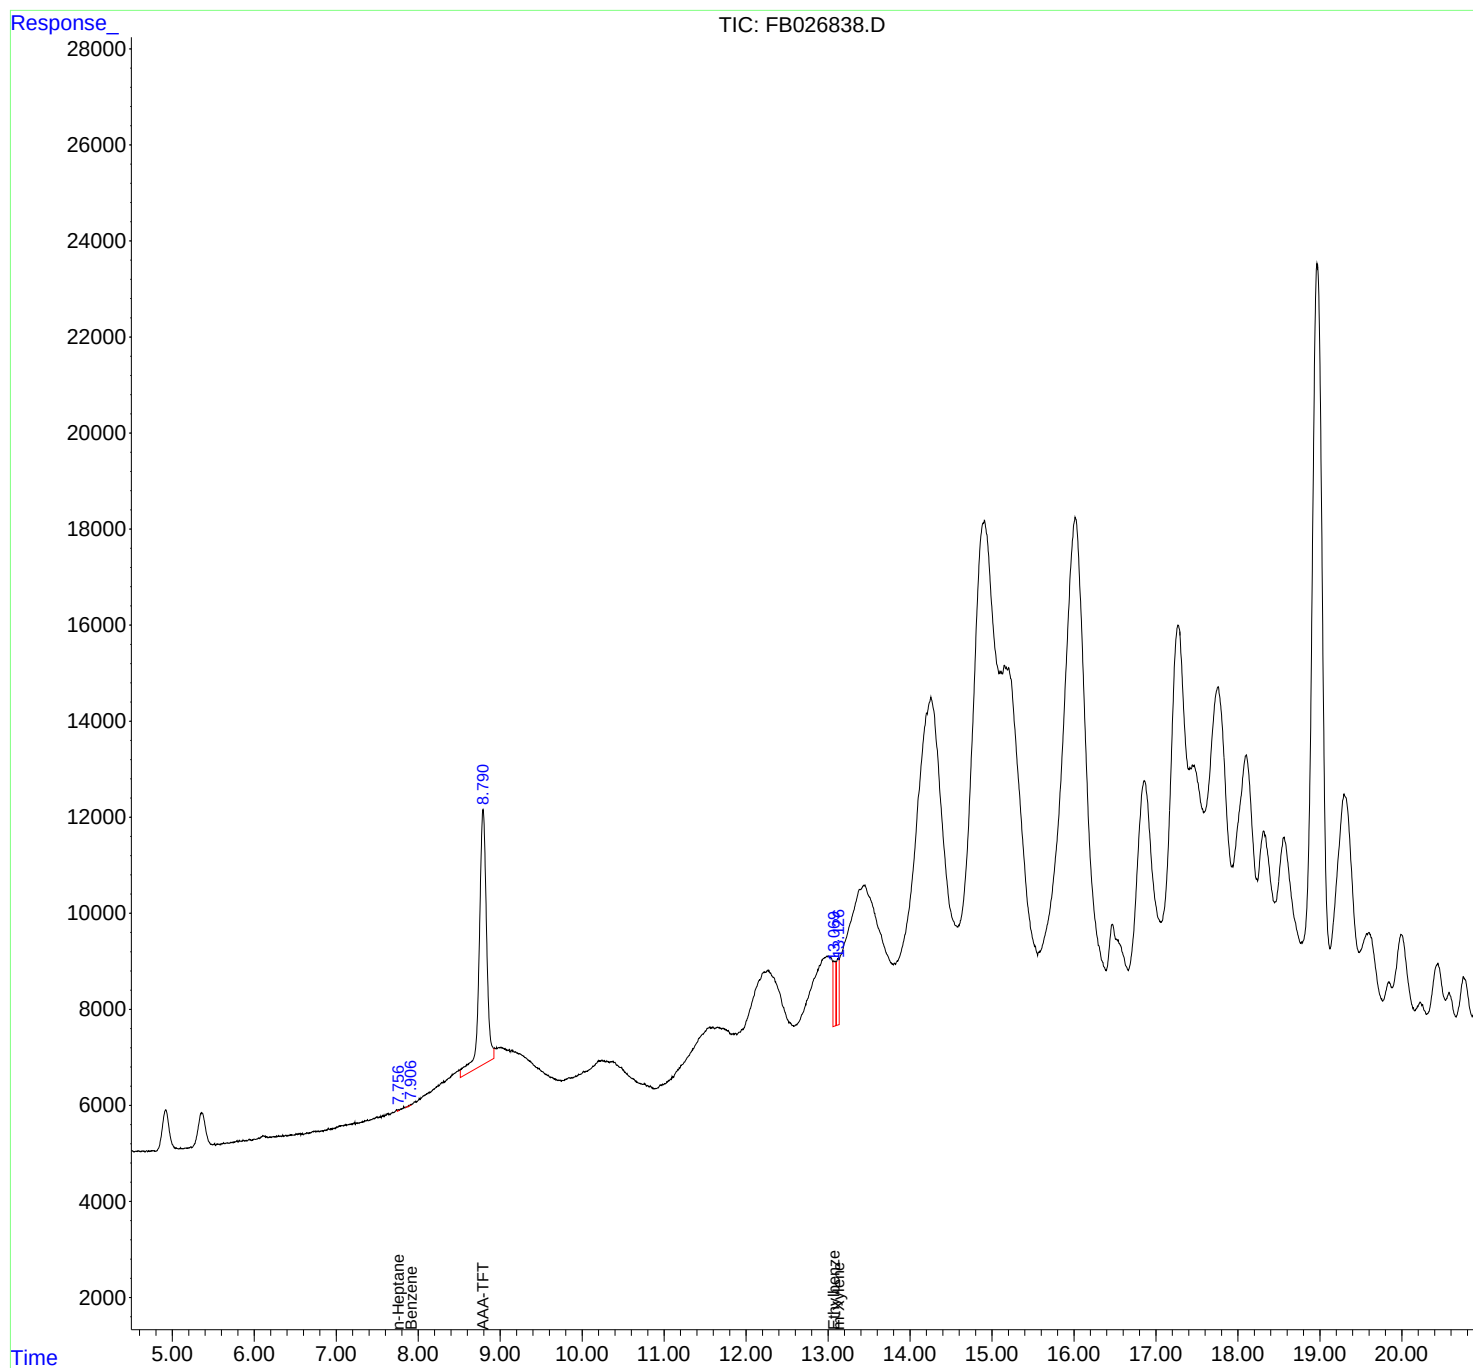


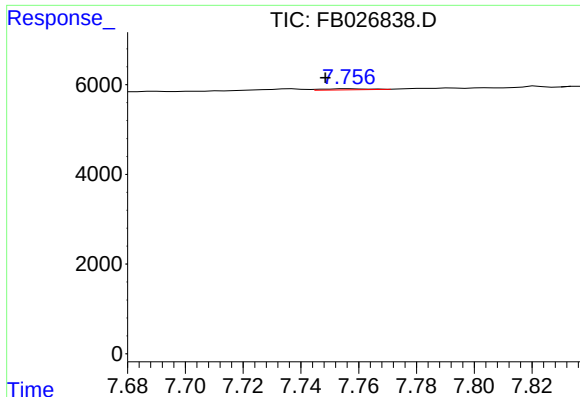

#3 n-Heptane


R.T.: 7.757 min
Delta R.T.: 0.008 min
Response: 248
Conc: 0.01 ng/ml

Instrument :
FID_B
ClientSampleId :

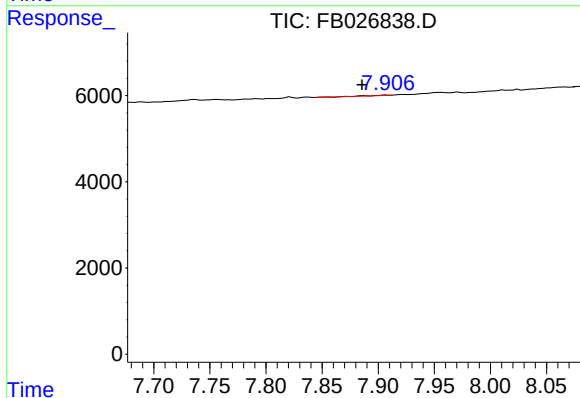


#4 Benzene

R.T.: 7.908 min
Delta R.T.: 0.022 min
Response: 108
Conc: 0.00 ng/ml

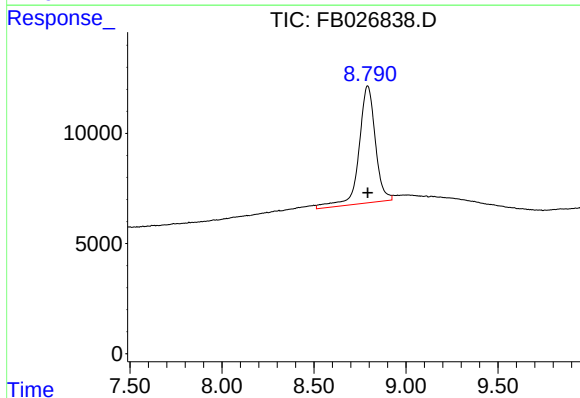


#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 327974
Conc: 31.26 ng/ml

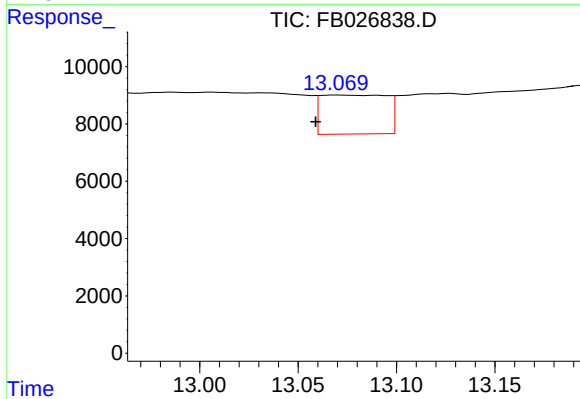

#7 Ethylbenzene

R.T.: 13.071 min
Delta R.T.: 0.012 min
Response: 31526
Conc: 1.57 ng/ml

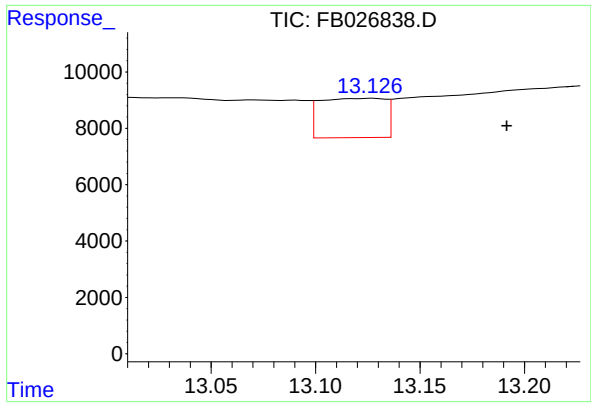

#8 m-Xylene

R.T.: 13.127 min
Delta R.T.: -0.064 min
Response: 30192
Conc: 1.50 ng/ml

Instrument :
FID_B
ClientSampleId :