

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
 Data File : FB026825.D
 Signal(s) : FID2B.CH
 Acq On : 5 Apr 2022 12:17
 Operator : AJ/MA
 Sample : BSF0405S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0405S1

Integration File: Calibration.e
 Quant Time: Apr 06 02:14:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	210483	20.059 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	353231	18.656 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	442310	21.339 ng/ml
3) t n-Heptane	7.746	109405	5.527 ng/ml
4) t Benzene	7.883	169780	7.358 ng/ml
6) t Toluene	10.617	497893	22.742 ng/ml
7) t Ethylbenzene	13.054	162695	8.095 ng/ml
8) t m-Xylene	13.186	329423	16.346 ng/ml
9) t O-Xylene	13.913	336959	16.890 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	370795	18.610 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040522\
Data File : FB026825.D
Signal(s) : FID2B.CH
Acq On : 5 Apr 2022 12:17
Operator : AJ/MA
Sample : BSF0405S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0405S1

Integration File: Calibration.e
Quant Time: Apr 06 02:14:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

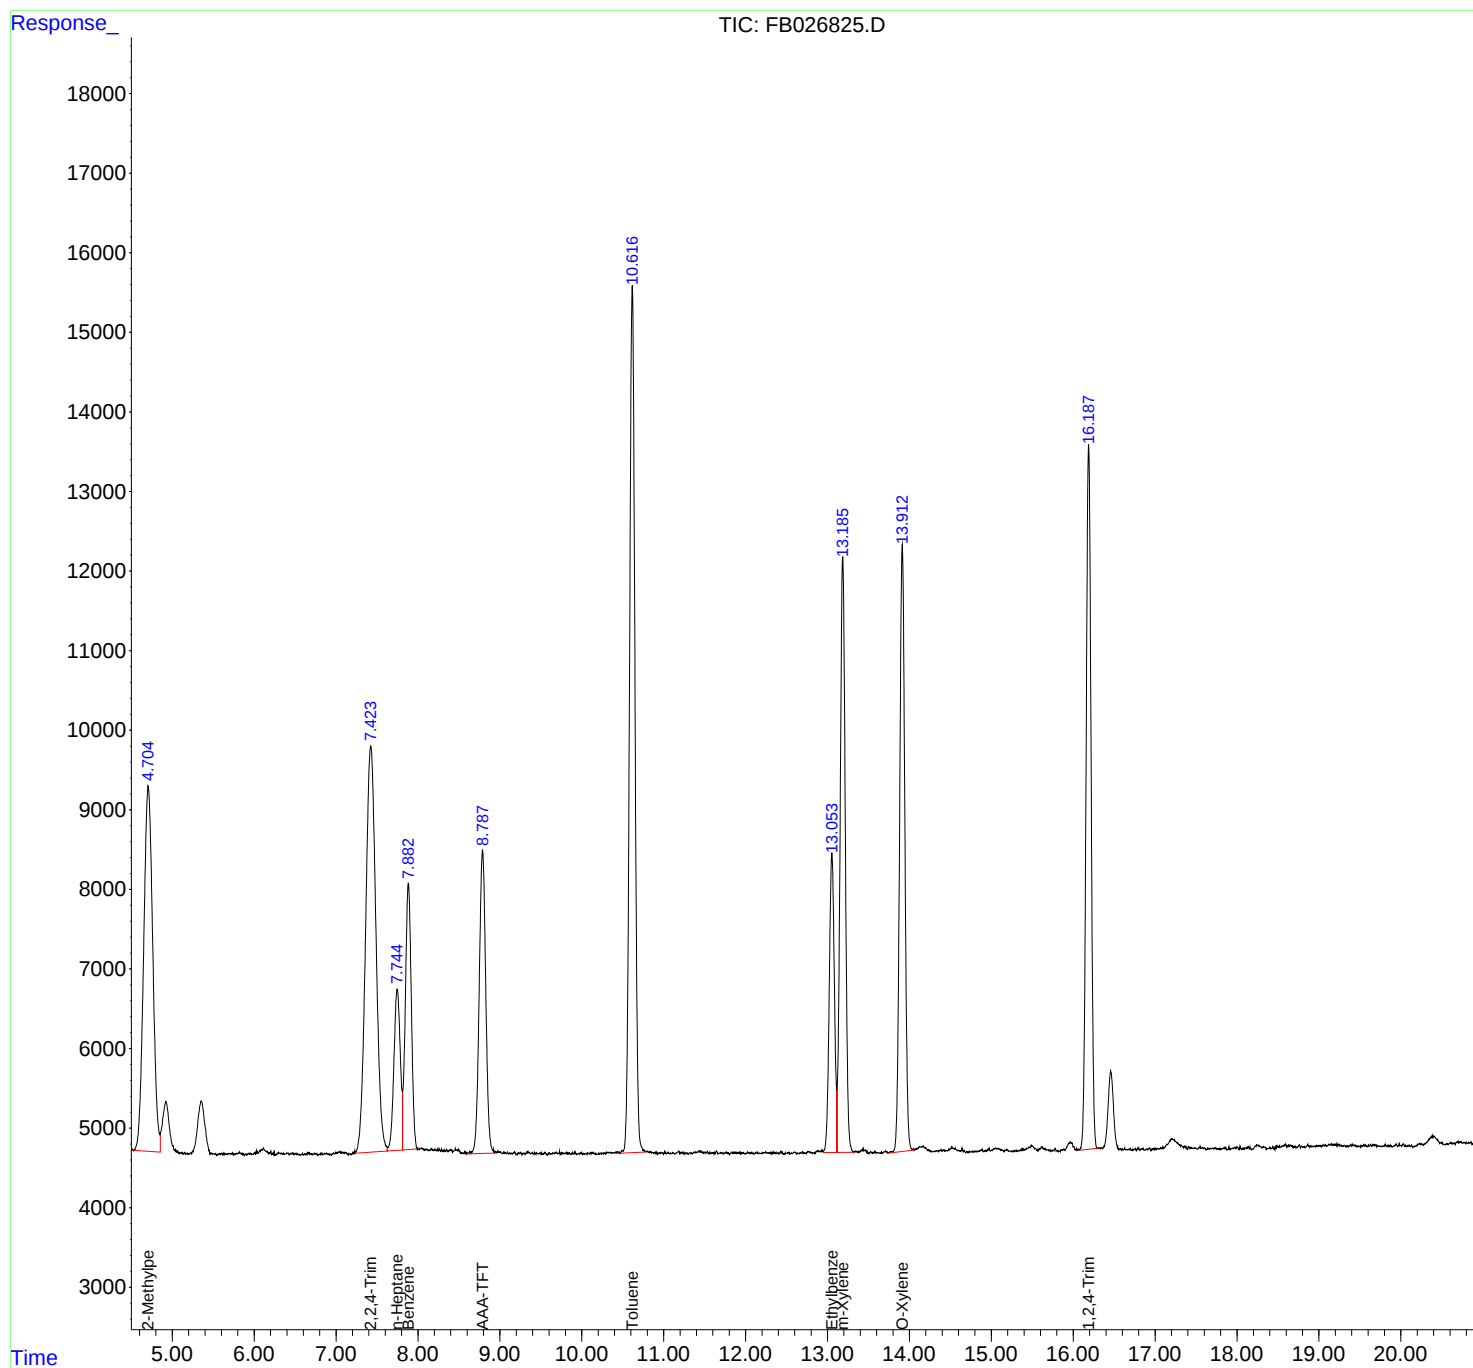


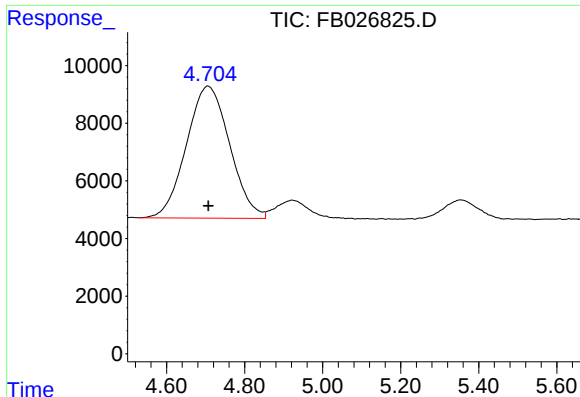

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: 0.000 min
Response: 353231
Conc: 18.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0405S1

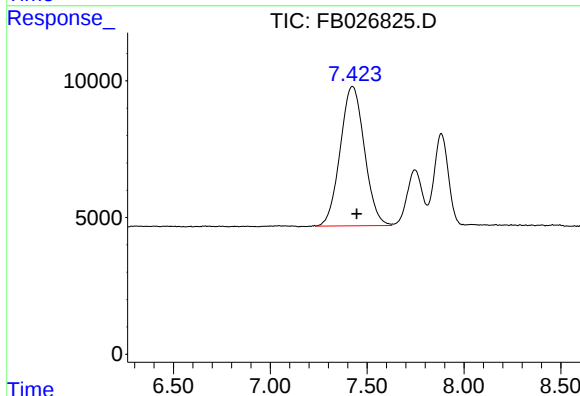


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.022 min
Response: 442310
Conc: 21.34 ng/ml

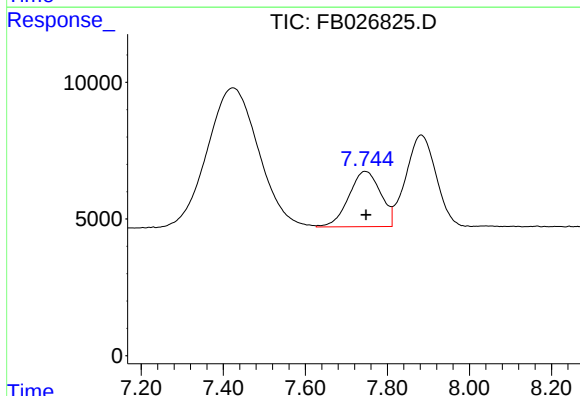


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 109405
Conc: 5.53 ng/ml

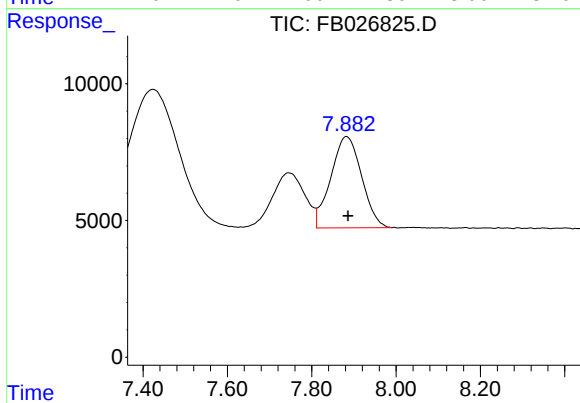

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 169780
Conc: 7.36 ng/ml

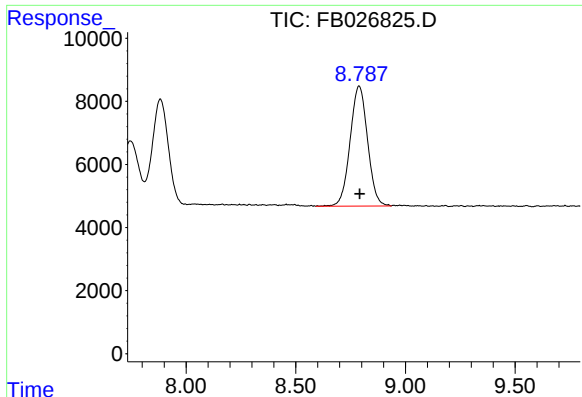

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 210483
Conc: 20.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0405S1

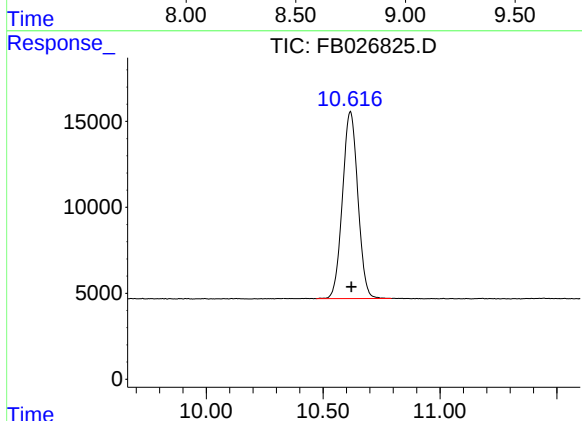


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 497893
Conc: 22.74 ng/ml

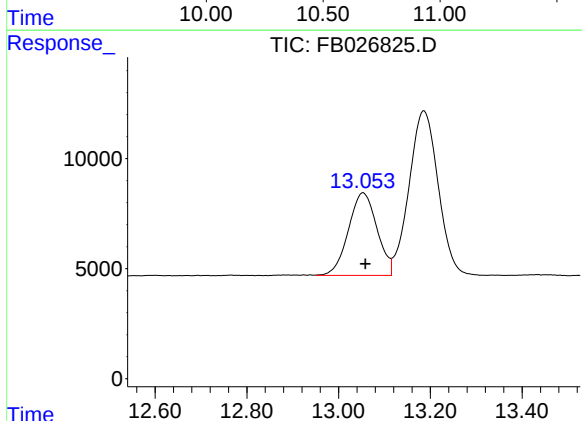


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 162695
Conc: 8.10 ng/ml

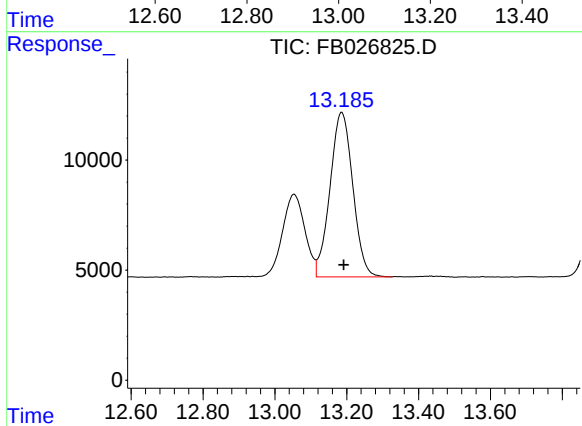

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 329423
Conc: 16.35 ng/ml

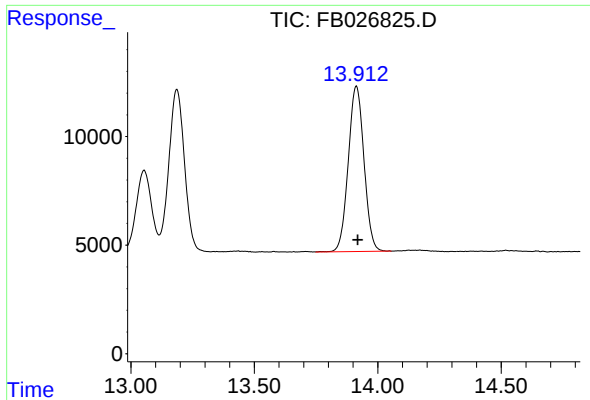

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 336959
Conc: 16.89 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0405S1

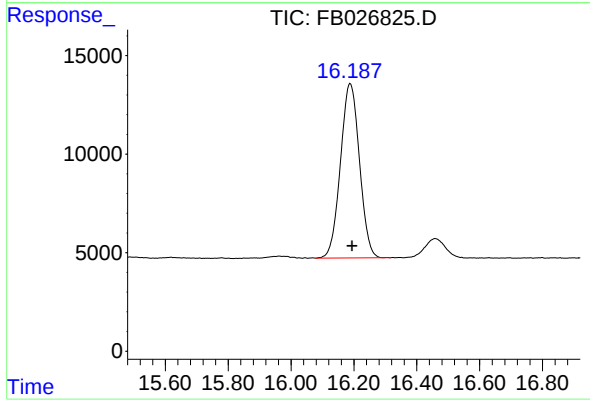

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.006 min
Response: 370795
Conc: 18.61 ng/ml