

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
 Data File : FB024089.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2020 10:31
 Operator : DD/AJ
 Sample : BSF0406S1
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 07 02:50:23 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	433022	18.959 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	932372	26.940 ng/ml
2) t	2,2,4-Trimethylpentane	7.417	1054884	28.744 ng/ml
3) t	n-Heptane	7.757	340700	9.446 ng/ml
4) t	Benzene	7.892	426193	9.609 ng/ml
6) t	Toluene	10.630	1218940	27.657 ng/ml
7) t	Ethylbenzene	13.069	385654	9.678 ng/ml
8) t	m-Xylene	13.202	751502	19.537 ng/ml
9) t	O-Xylene	13.930	719629	19.470 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	613089	19.293 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024089.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 10:31
Operator : DD/AJ
Sample : BSF0406S1
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:50:23 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

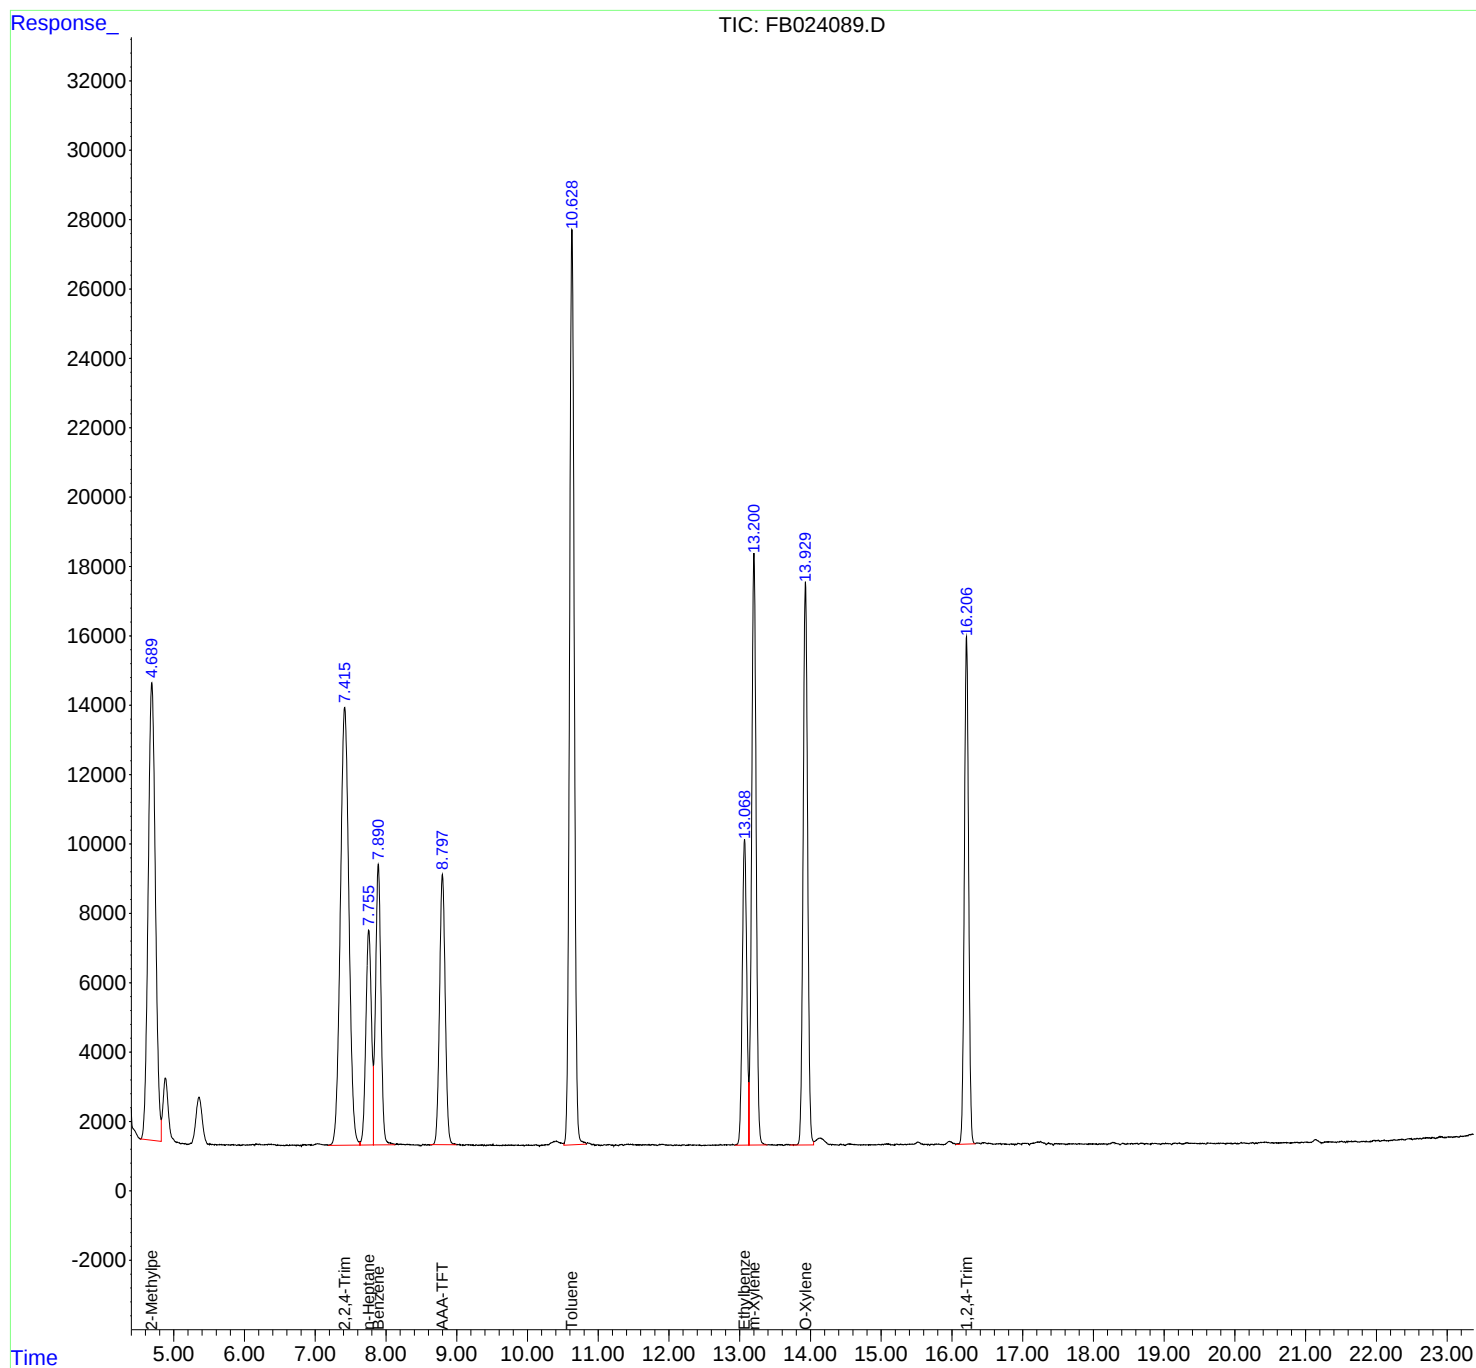

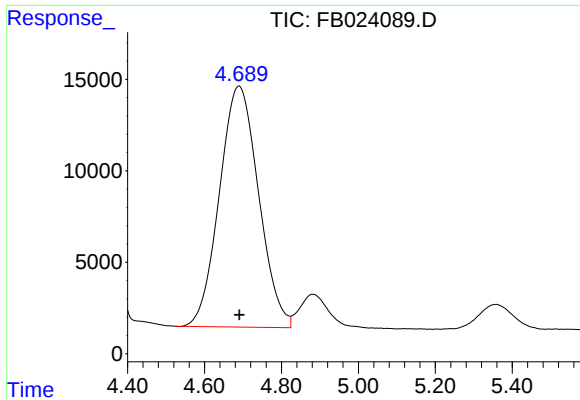


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 932372
Conc: 26.94 ng/ml

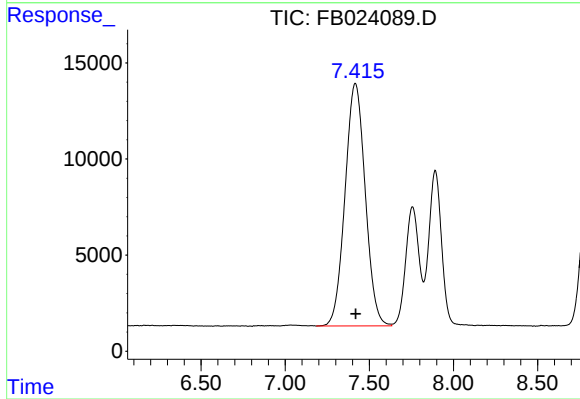


#2 2,2,4-Trimethylpentane

R.T.: 7.417 min
Delta R.T.: -0.003 min
Response: 1054884
Conc: 28.74 ng/ml

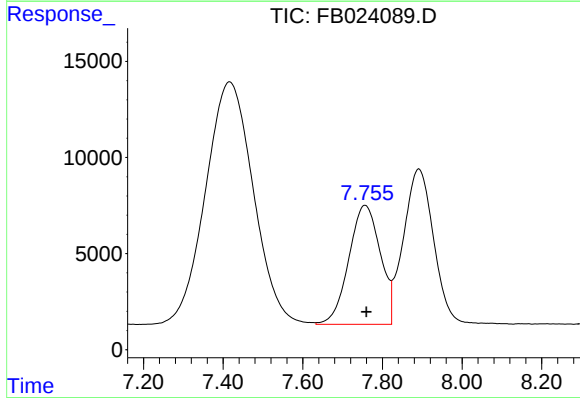


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.003 min
Response: 340700
Conc: 9.45 ng/ml

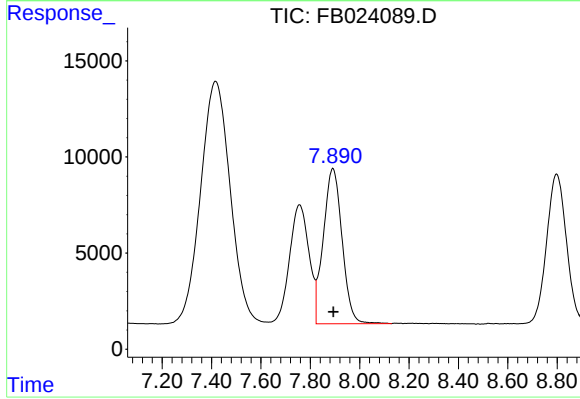


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.003 min
Response: 426193
Conc: 9.61 ng/ml

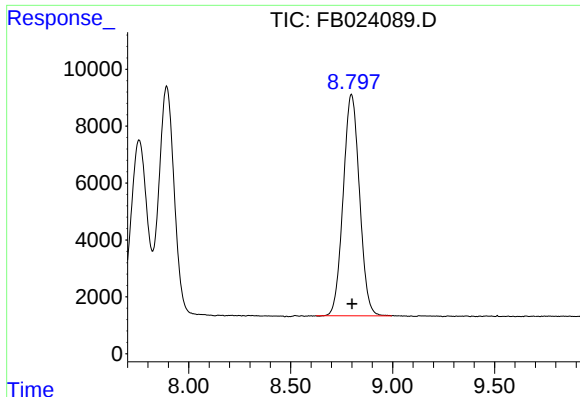


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 433022
Conc: 18.96 ng/ml

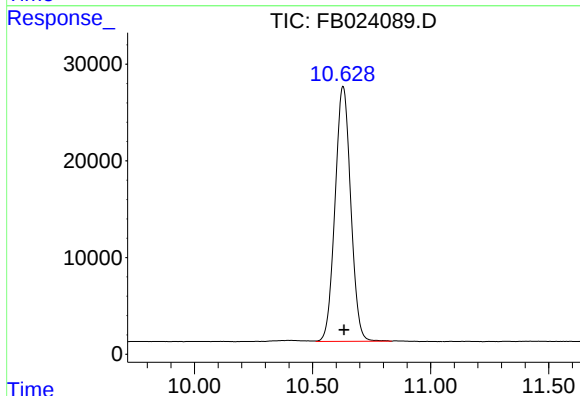


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.003 min
Response: 1218940
Conc: 27.66 ng/ml

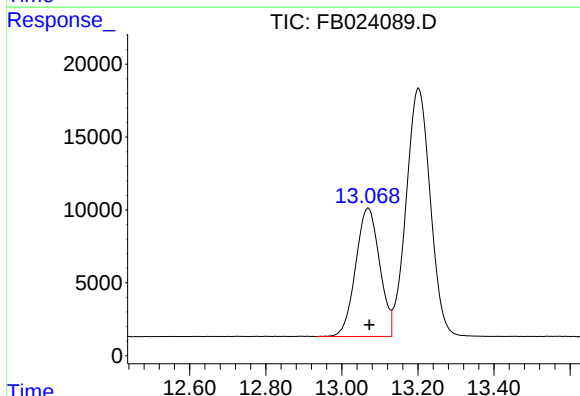


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.003 min
Response: 385654
Conc: 9.68 ng/ml

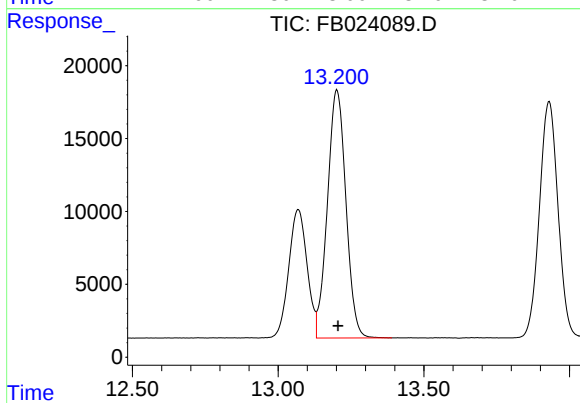


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.004 min
Response: 751502
Conc: 19.54 ng/ml

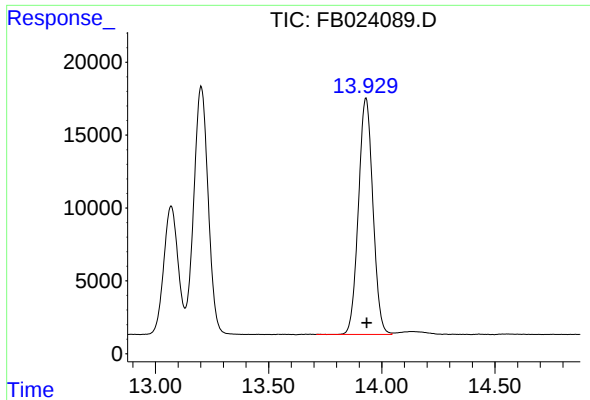

#9 O-Xylene

R.T.: 13.930 min
Delta R.T.: -0.003 min
Response: 719629
Conc: 19.47 ng/ml

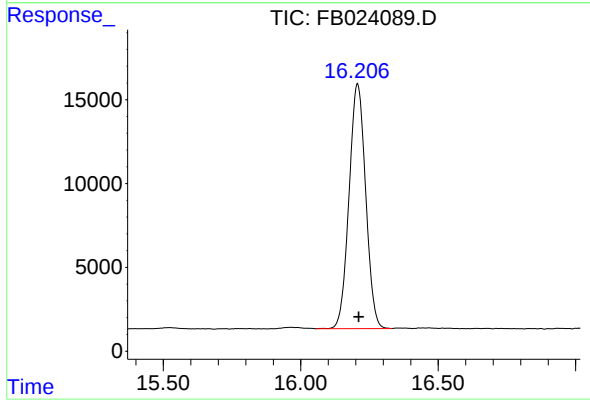

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 613089
Conc: 19.29 ng/ml