

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024090.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 11:55
Operator : DD/AJ
Sample : L2129-38
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:50:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	355622	15.570 ng/ml
Target Compounds			
6) t Toluene	10.628	3244	0.074 ng/ml
8) t m-Xylene	13.207	3623	0.094 ng/ml
9) t O-Xylene	13.953	2927	0.079 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024090.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 11:55
Operator : DD/AJ
Sample : L2129-38
Misc : 5.07g/5.00ml DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:50:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

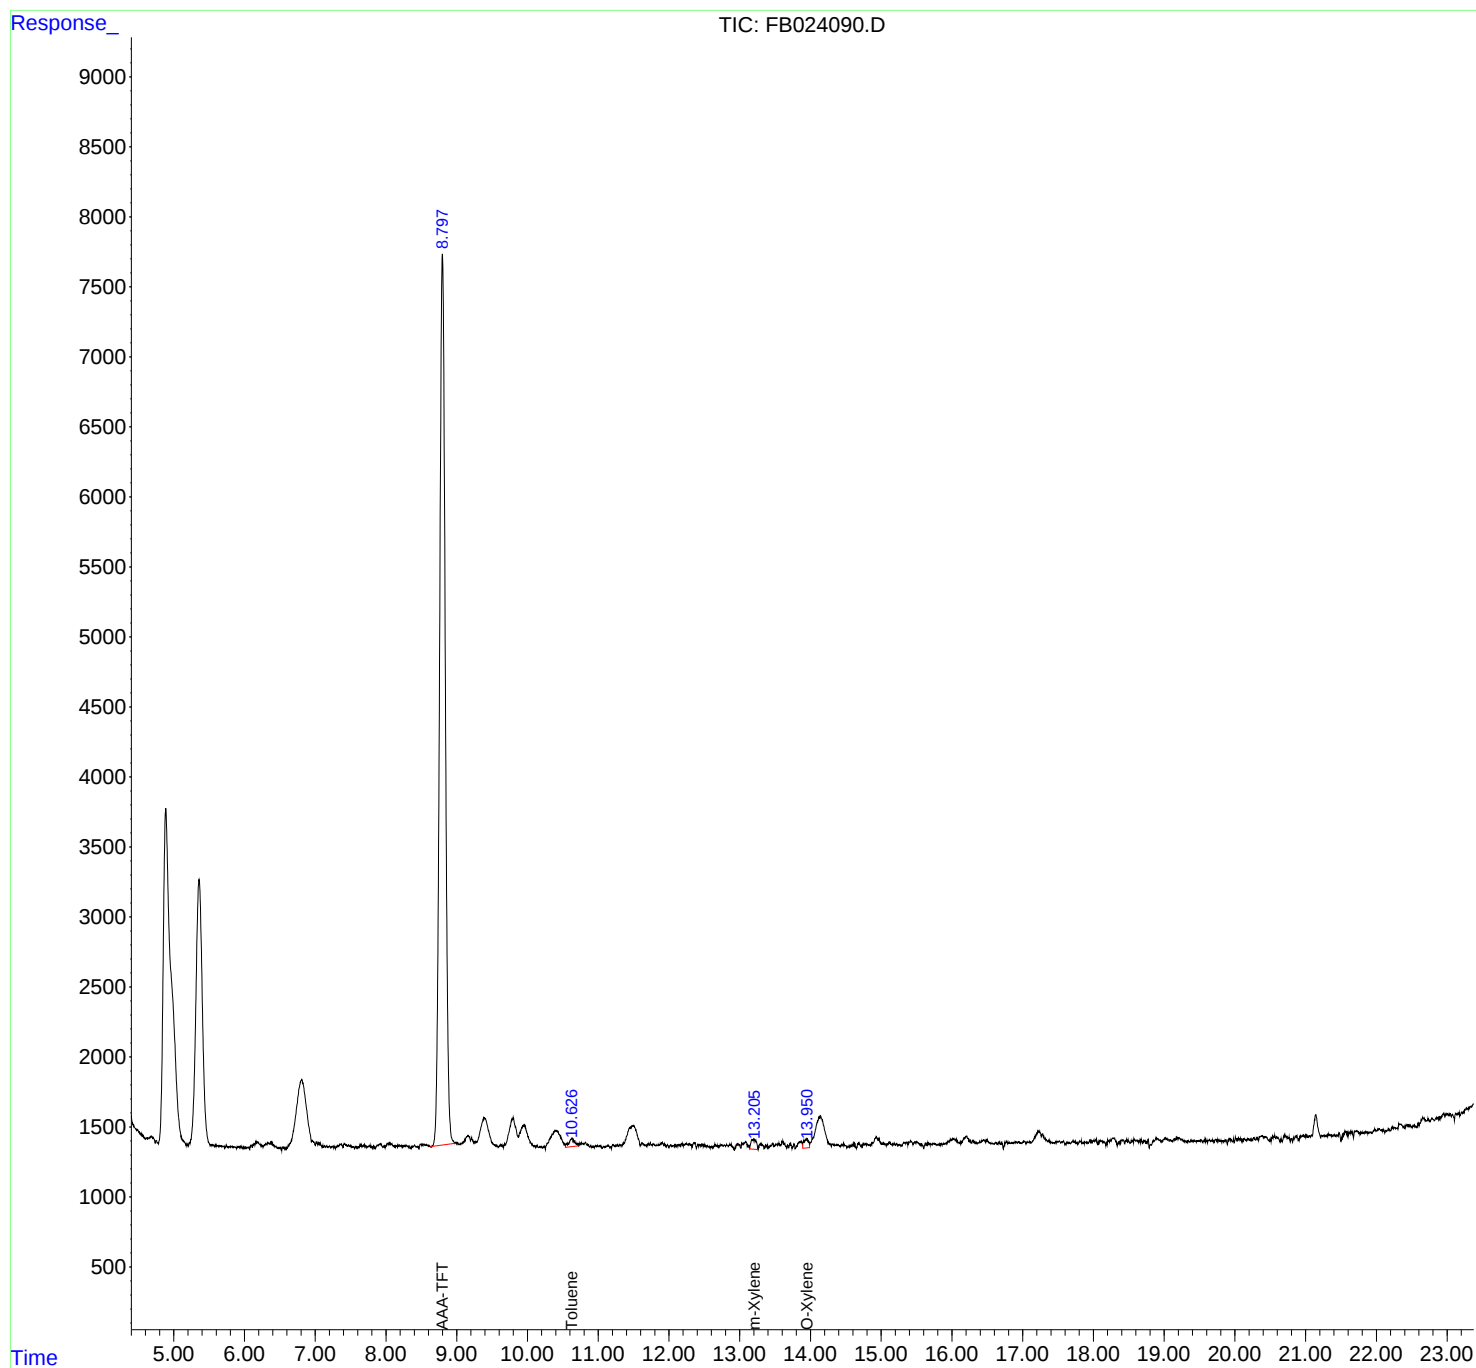

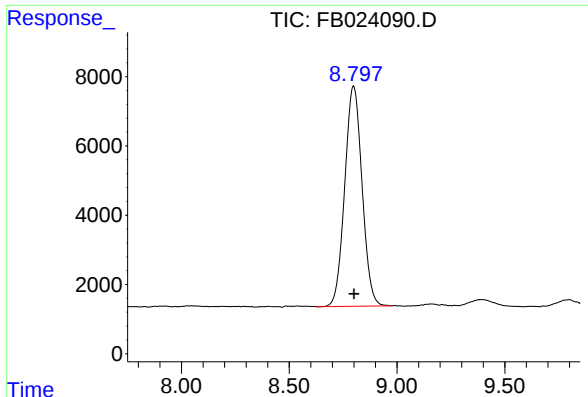


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 355622
Conc: 15.57 ng/ml

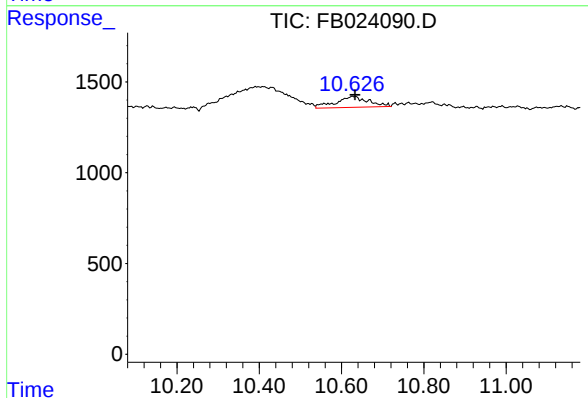


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.005 min
Response: 3244
Conc: 0.07 ng/ml

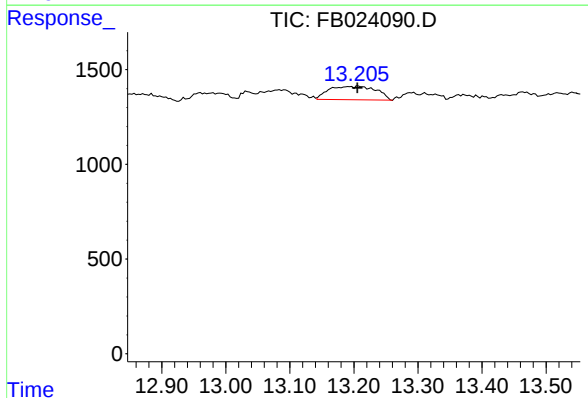

#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.002 min
Response: 3623
Conc: 0.09 ng/ml

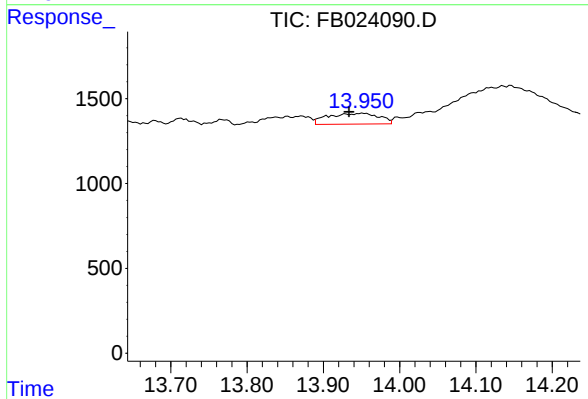

#9 O-Xylene

R.T.: 13.953 min
Delta R.T.: 0.019 min
Response: 2927
Conc: 0.08 ng/ml