

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024093.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 14:05
Operator : DD/AJ
Sample : L2129-42MS
Misc : 5.05/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:50:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.797	449571	19.683 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	909505	26.279 ng/ml
2) t	2,2,4-Trimethylpentane	7.416	1032325	28.129 ng/ml
3) t	n-Heptane	7.755	328339	9.103 ng/ml
4) t	Benzene	7.890	408100	9.201 ng/ml
6) t	Toluene	10.629	1220708	27.697 ng/ml
7) t	Ethylbenzene	13.069	365576	9.174 ng/ml
8) t	m-Xylene	13.202	717006	18.641 ng/ml
9) t	O-Xylene	13.929	692111	18.725 ng/ml
10) t	1,2,4-Trimethylbenzene	16.207	588269	18.512 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024093.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 14:05
Operator : DD/AJ
Sample : L2129-42MS
Misc : 5.05/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:50:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

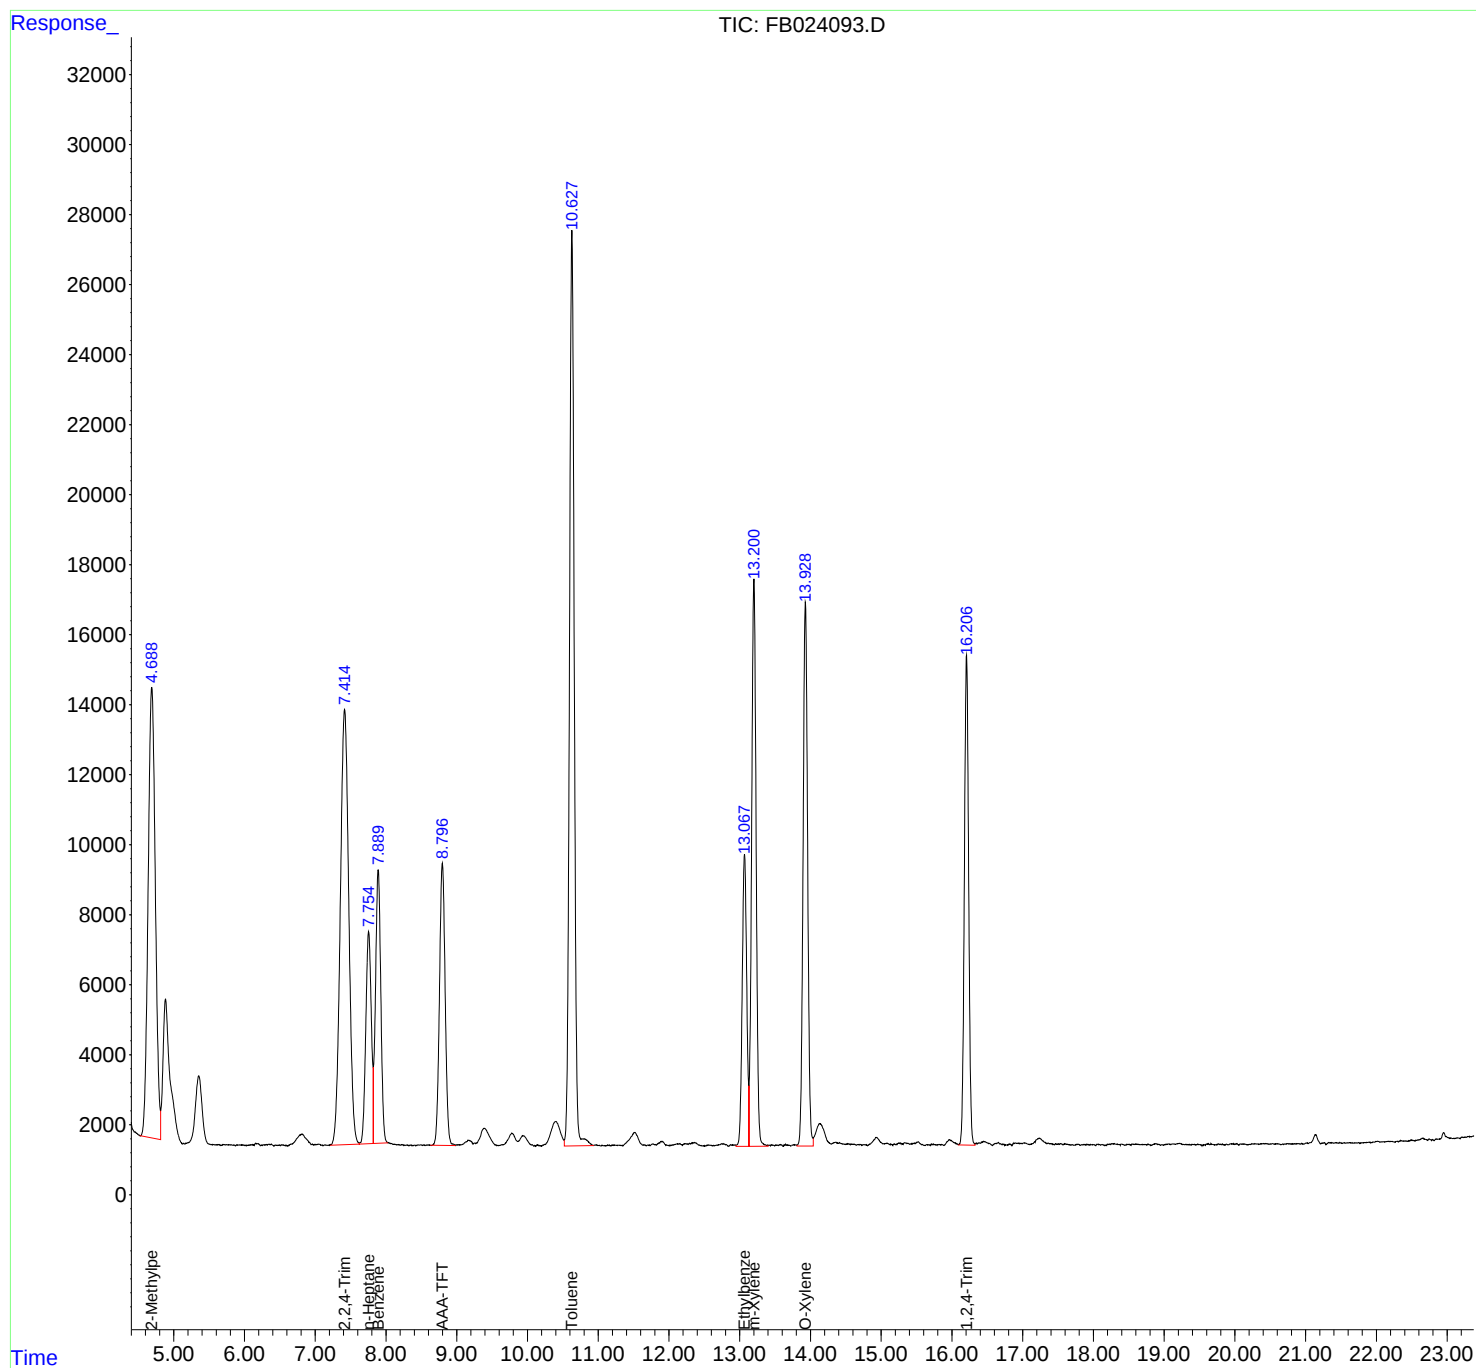

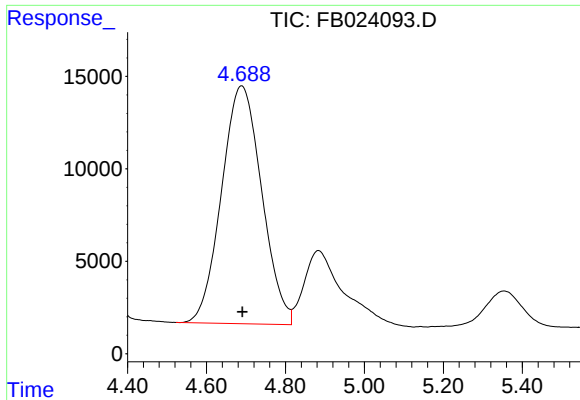


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 909505
Conc: 26.28 ng/ml

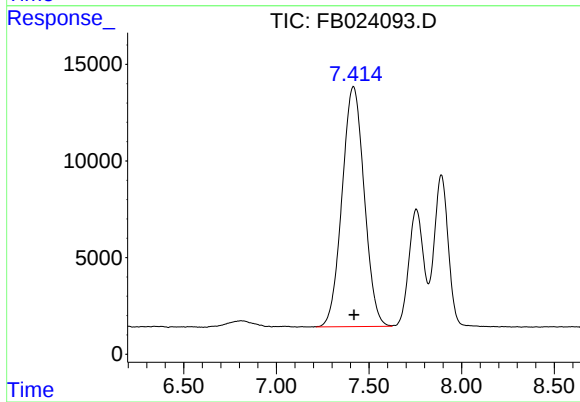


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.004 min
Response: 1032325
Conc: 28.13 ng/ml

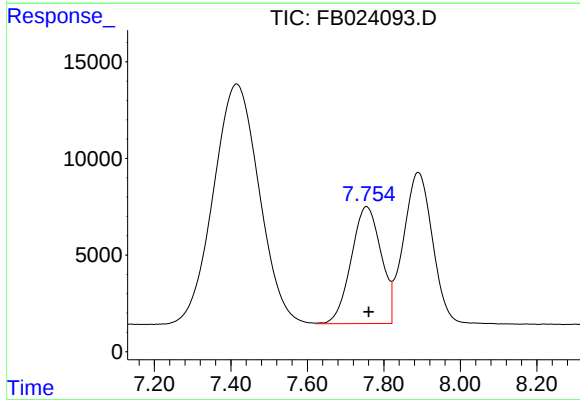


#3 n-Heptane

R.T.: 7.755 min
Delta R.T.: -0.005 min
Response: 328339
Conc: 9.10 ng/ml

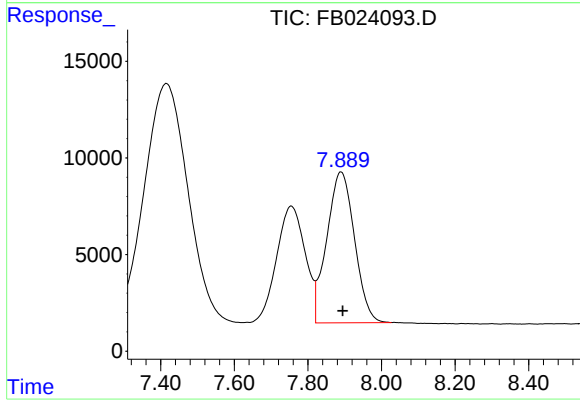


#4 Benzene

R.T.: 7.890 min
Delta R.T.: -0.004 min
Response: 408100
Conc: 9.20 ng/ml

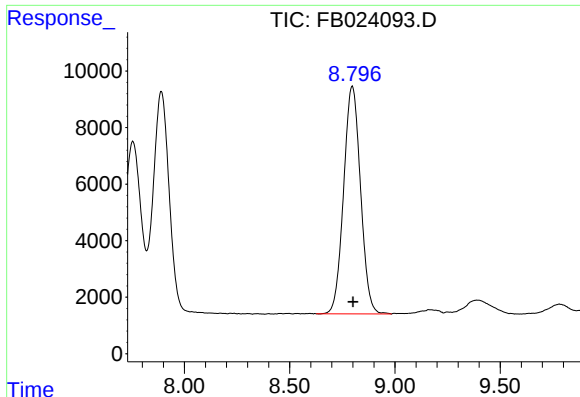


#5 AAA-TFT

R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 449571
Conc: 19.68 ng/ml

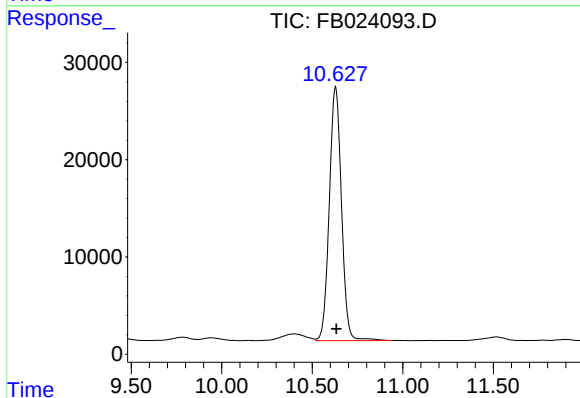


#6 Toluene

R.T.: 10.629 min
Delta R.T.: -0.004 min
Response: 1220708
Conc: 27.70 ng/ml

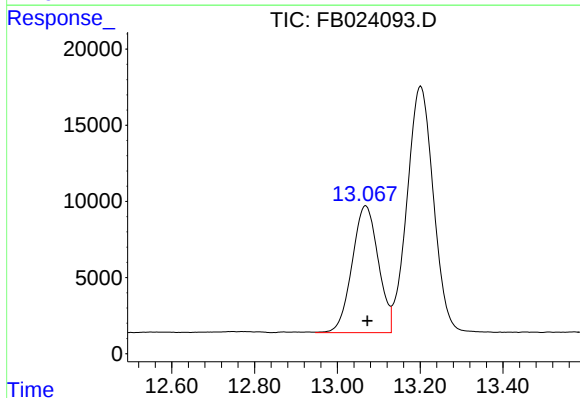


#7 Ethylbenzene

R.T.: 13.069 min
Delta R.T.: -0.004 min
Response: 365576
Conc: 9.17 ng/ml

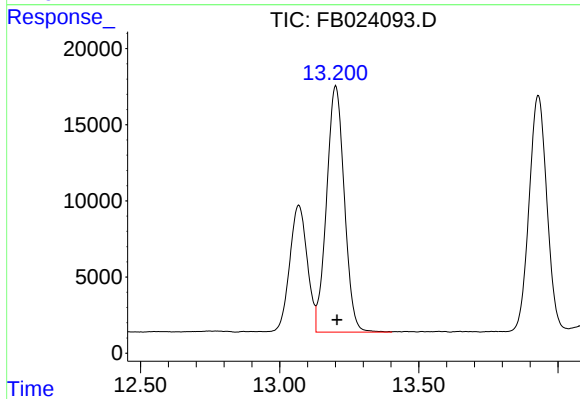


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.004 min
Response: 717006
Conc: 18.64 ng/ml

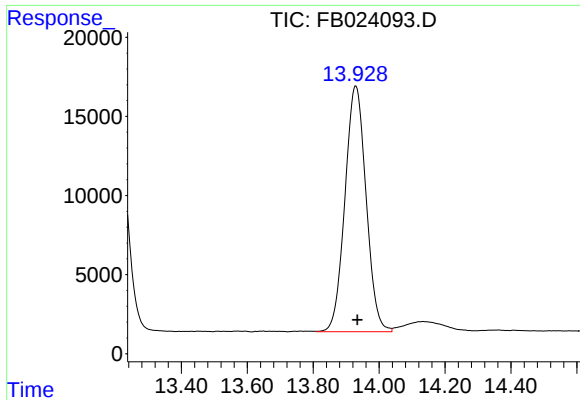

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 692111
Conc: 18.73 ng/ml

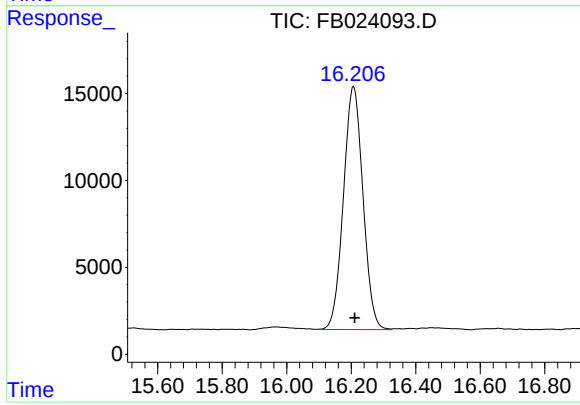

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 588269
Conc: 18.51 ng/ml