

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
 Data File : FB024094.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2020 14:35
 Operator : DD/AJ
 Sample : L2129-42MSD
 Misc : 5.04/5.00ml DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 07 02:51:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.799	459311	20.110 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	936218	27.051 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1055604	28.763 ng/ml
3) t n-Heptane	7.758	339618	9.416 ng/ml
4) t Benzene	7.892	423067	9.539 ng/ml
6) t Toluene	10.630	1236086	28.046 ng/ml
7) t Ethylbenzene	13.070	380952	9.560 ng/ml
8) t m-Xylene	13.203	738145	19.190 ng/ml
9) t O-Xylene	13.931	702908	19.017 ng/ml
10) t 1,2,4-Trimethylbenzene	16.209	594003	18.692 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040620\
Data File : FB024094.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2020 14:35
Operator : DD/AJ
Sample : L2129-42MSD
Misc : 5.04/5.00ml DI WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 07 02:51:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

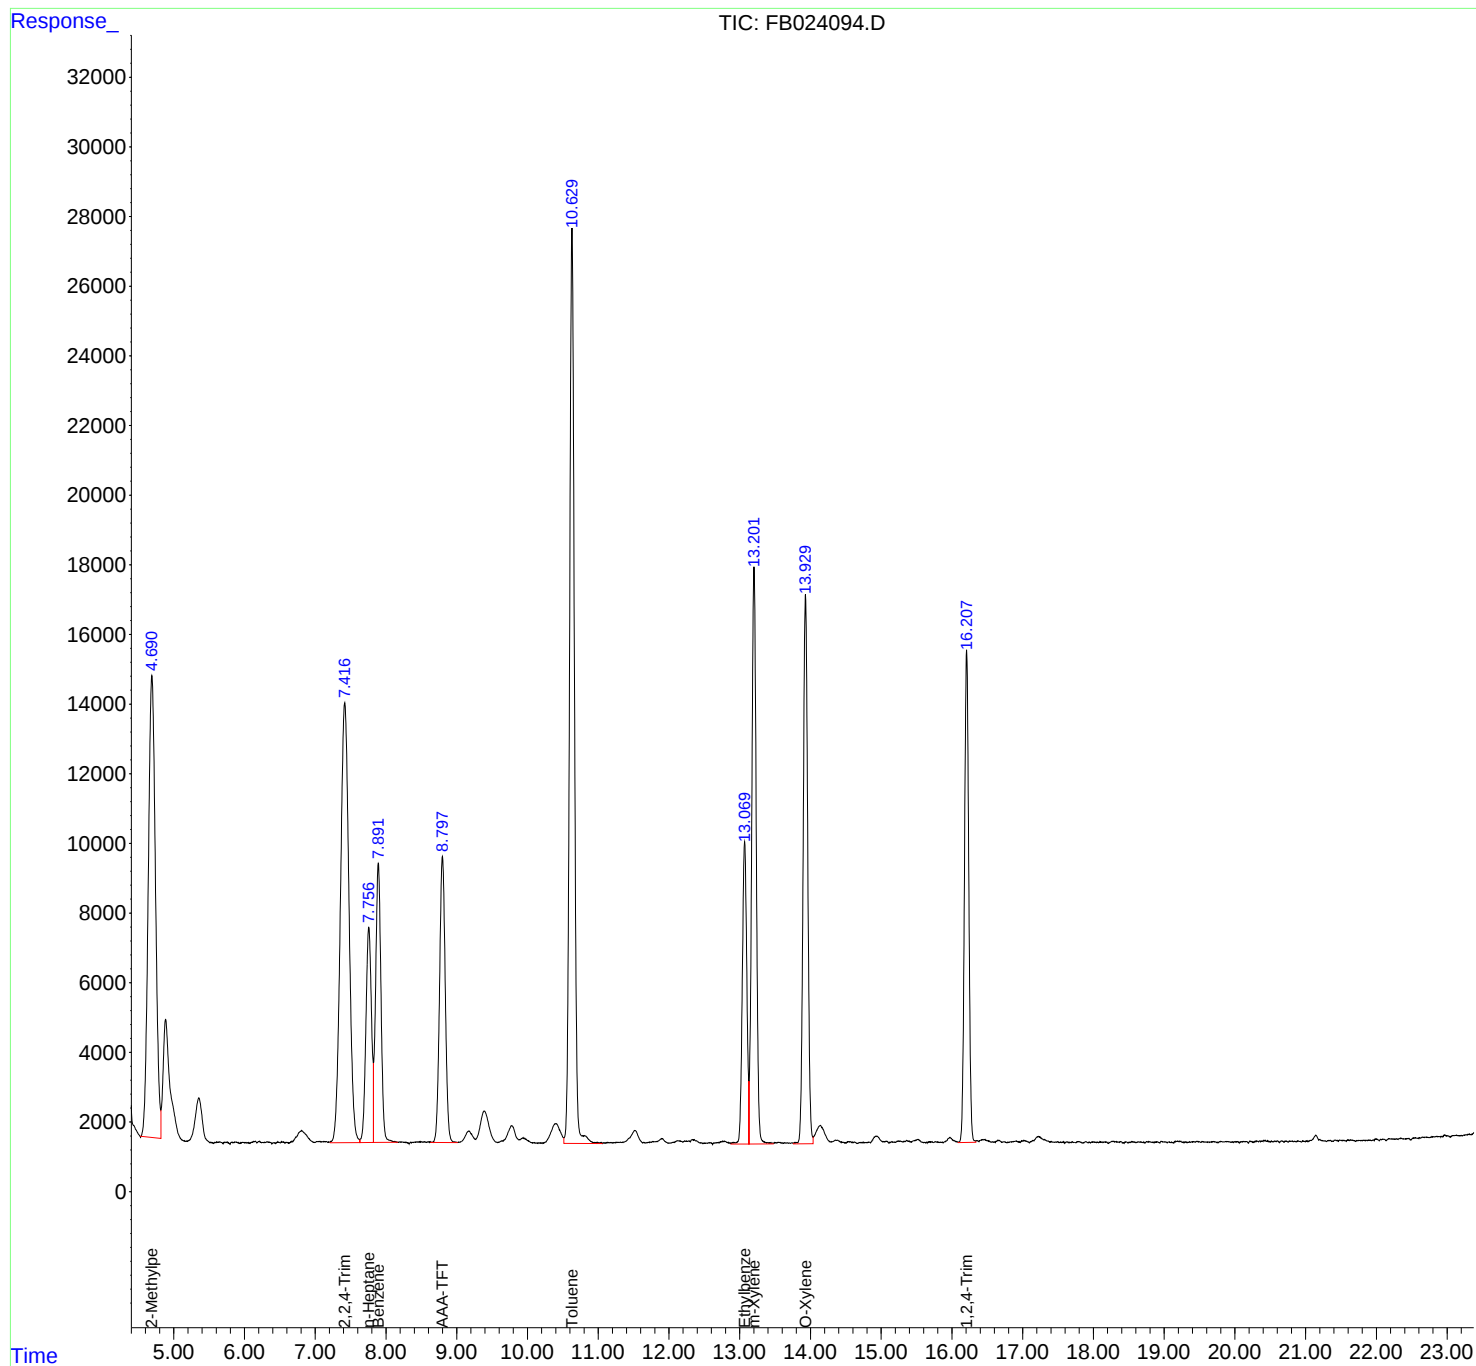

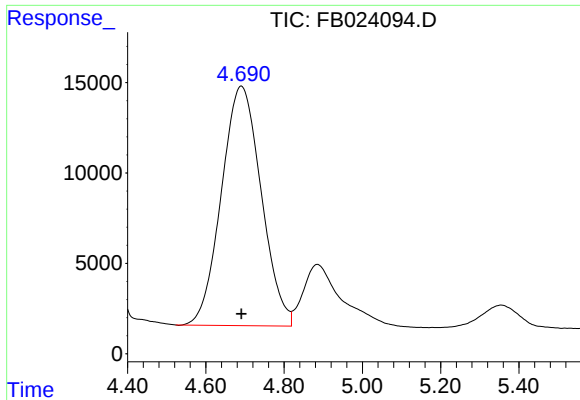


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 936218
Conc: 27.05 ng/ml

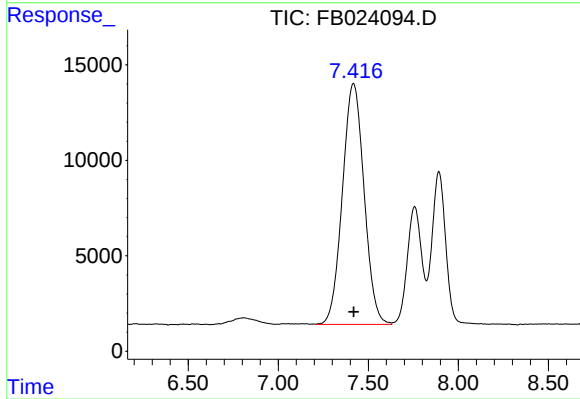


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 1055604
Conc: 28.76 ng/ml

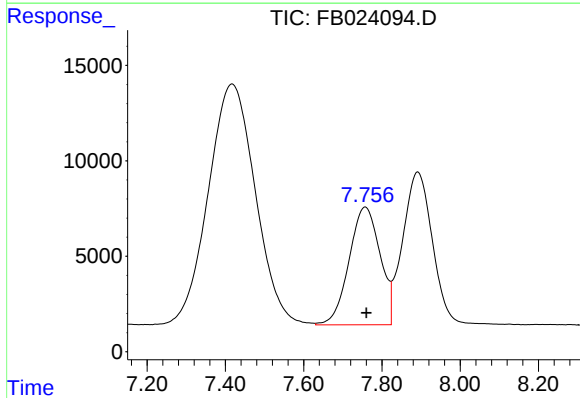


#3 n-Heptane

R.T.: 7.758 min
Delta R.T.: -0.002 min
Response: 339618
Conc: 9.42 ng/ml

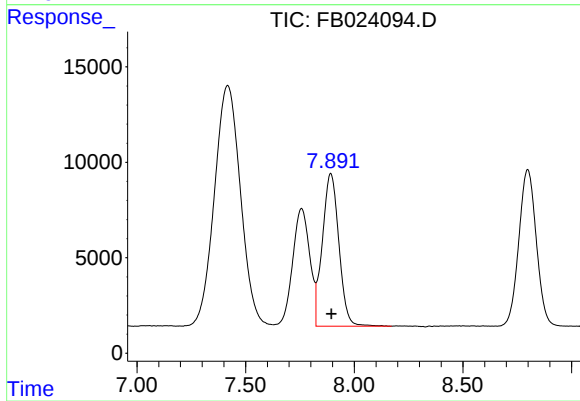


#4 Benzene

R.T.: 7.892 min
Delta R.T.: -0.002 min
Response: 423067
Conc: 9.54 ng/ml

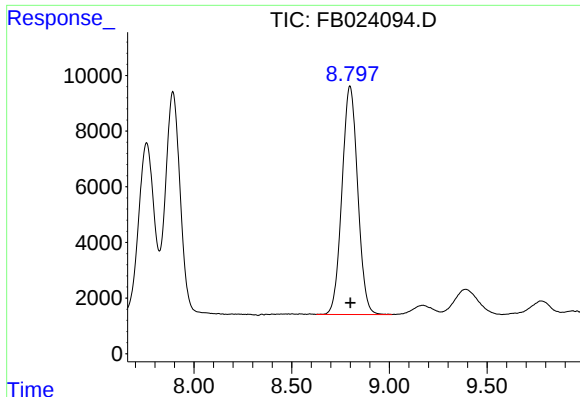


#5 AAA-TFT

R.T.: 8.799 min
Delta R.T.: -0.003 min
Response: 459311
Conc: 20.11 ng/ml

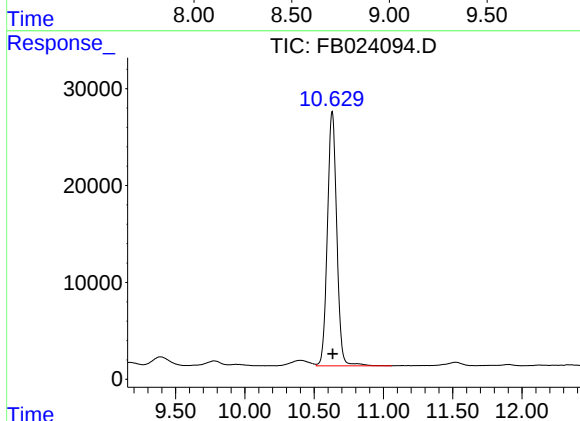


#6 Toluene

R.T.: 10.630 min
Delta R.T.: -0.003 min
Response: 1236086
Conc: 28.05 ng/ml

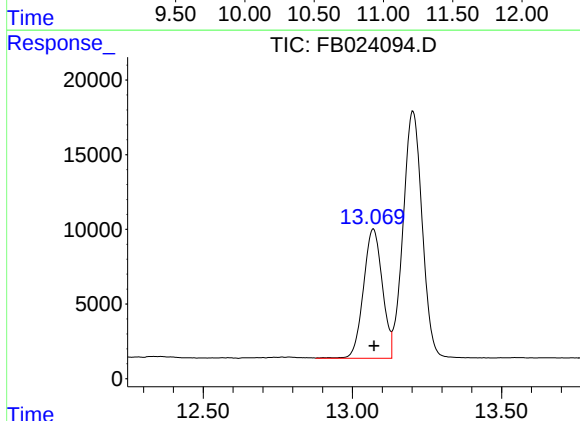


#7 Ethylbenzene

R.T.: 13.070 min
Delta R.T.: -0.003 min
Response: 380952
Conc: 9.56 ng/ml

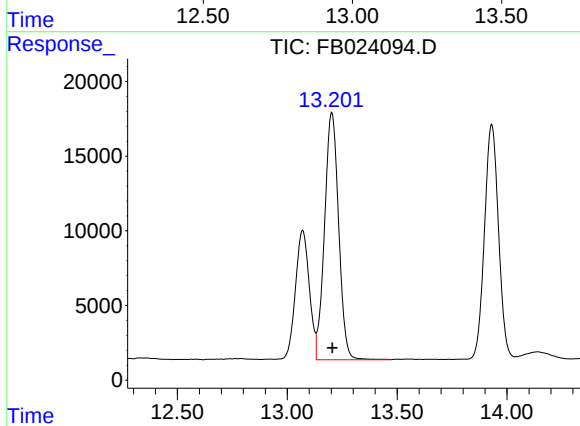


#8 m-Xylene

R.T.: 13.203 min
Delta R.T.: -0.003 min
Response: 738145
Conc: 19.19 ng/ml

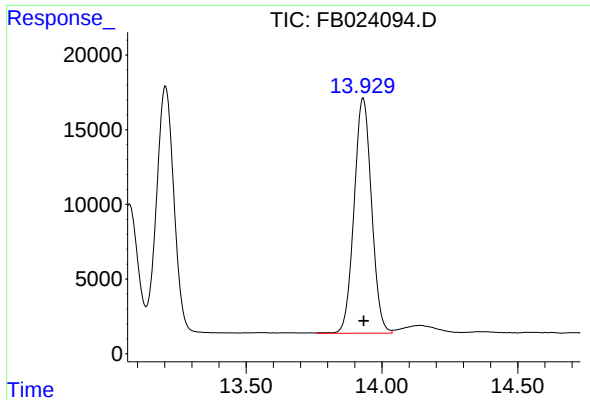

#9 O-Xylene

R.T.: 13.931 min
Delta R.T.: -0.003 min
Response: 702908
Conc: 19.02 ng/ml

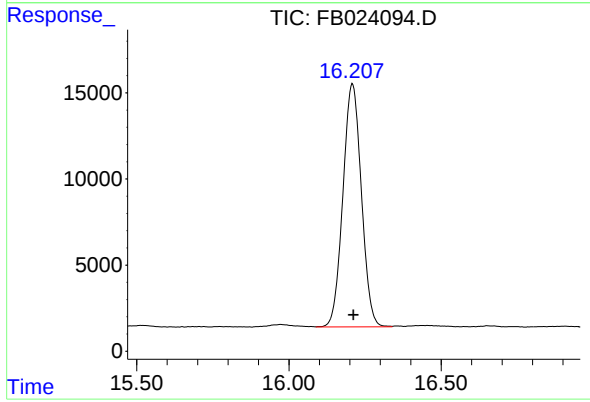

#10 1,2,4-Trimethylbenzene

R.T.: 16.209 min
Delta R.T.: -0.003 min
Response: 594003
Conc: 18.69 ng/ml