

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040622\
 Data File : FB026847.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2022 14:50
 Operator : AJ/MA
 Sample : I.BLK
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 06 16:12:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	221743	21.132 ng/ml
Target Compounds			
7) t Ethylbenzene	13.029	2889	0.144 ng/ml
9) t O-Xylene	13.966	68619	3.440 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040622\
Data File : FB026847.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2022 14:50
Operator : AJ/MA
Sample : I.BLK
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 06 16:12:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

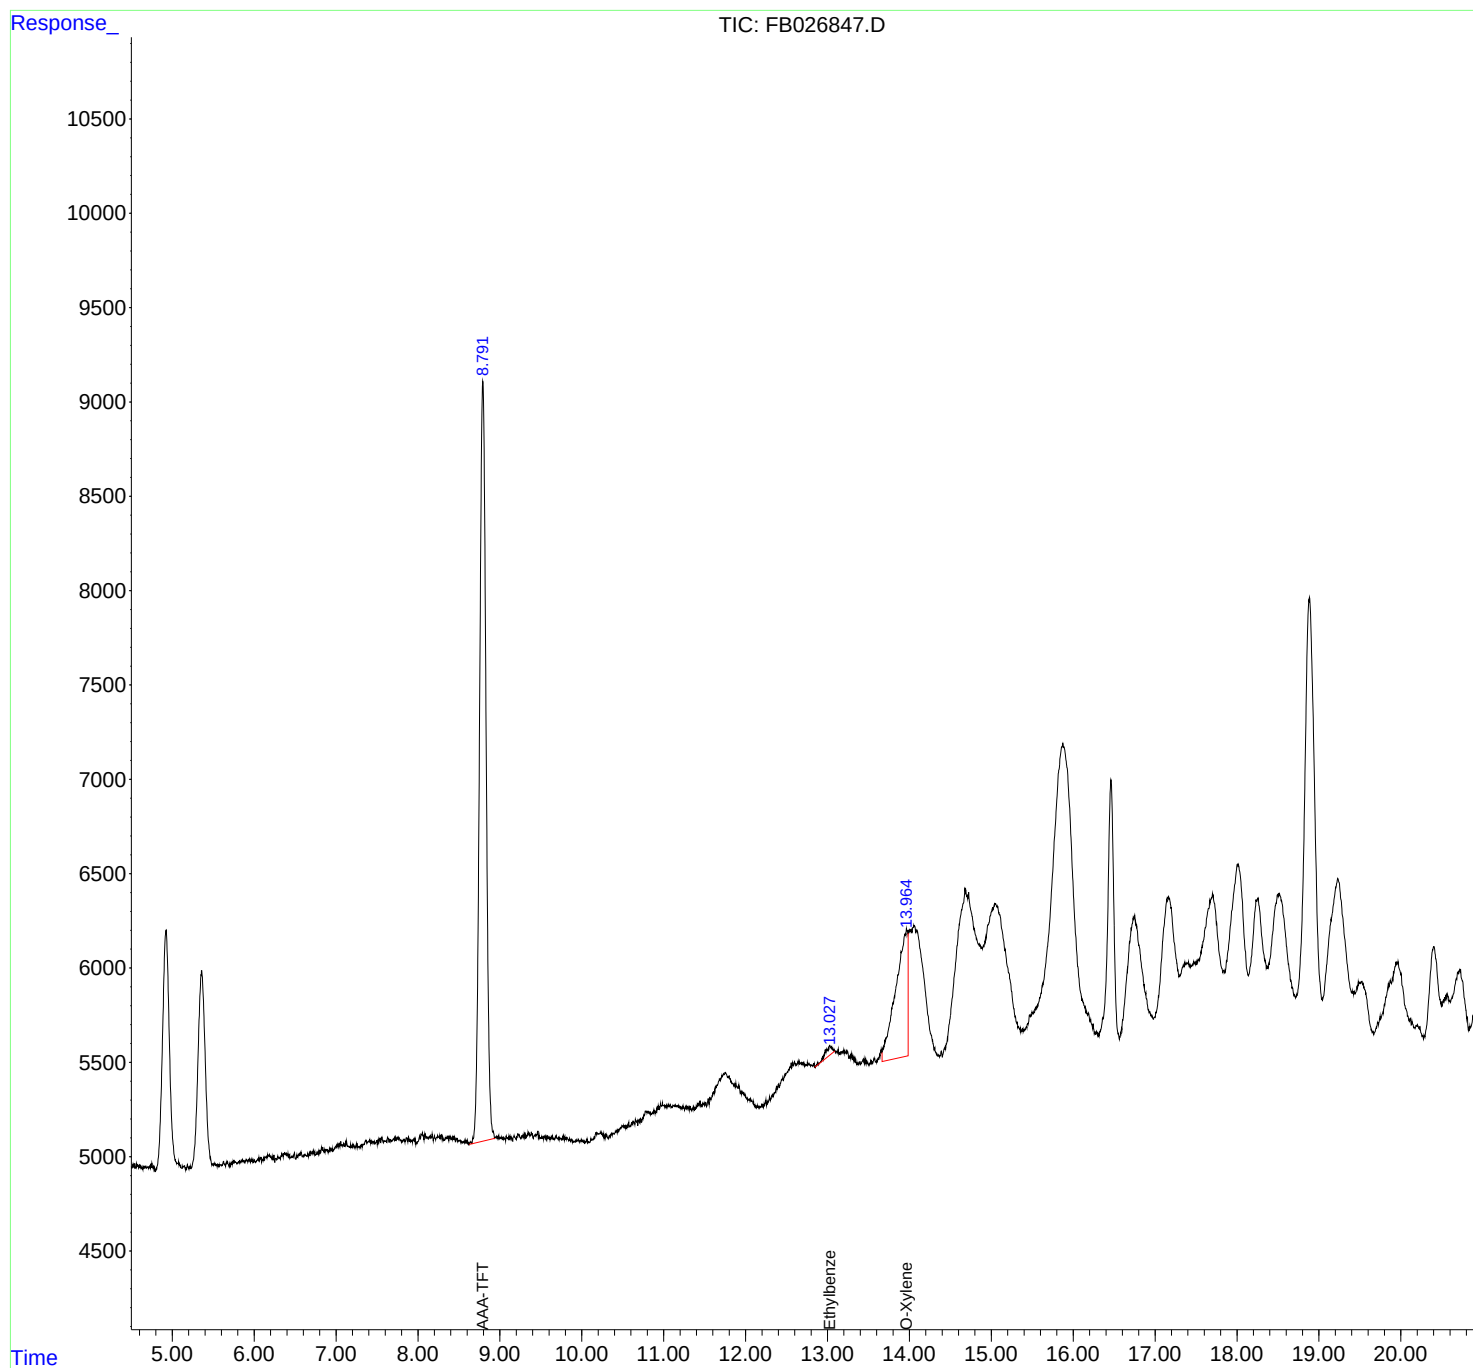


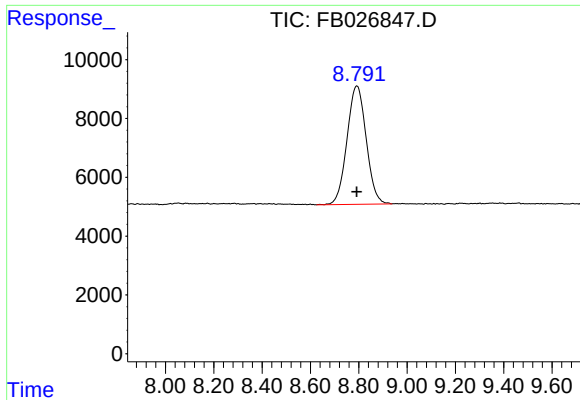

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: 0.000 min
Response: 221743
Conc: 21.13 ng/ml

Instrument :
FID_B
ClientSampleId :

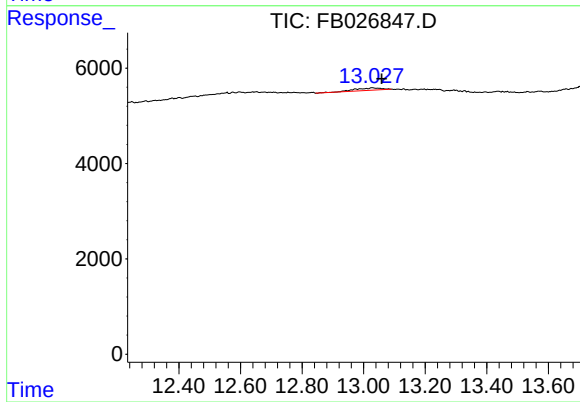

#7 Ethylbenzene

R.T.: 13.029 min
Delta R.T.: -0.030 min
Response: 2889
Conc: 0.14 ng/ml

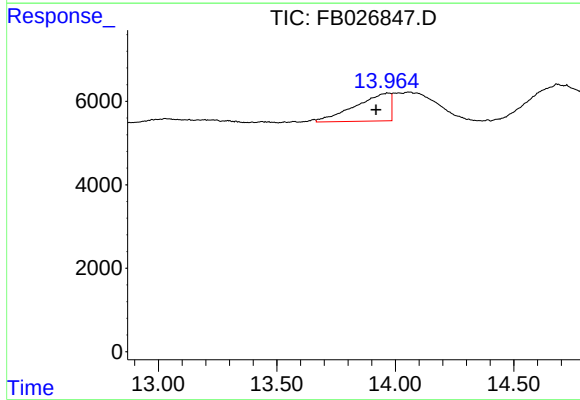

#9 O-Xylene

R.T.: 13.966 min
Delta R.T.: 0.047 min
Response: 68619
Conc: 3.44 ng/ml