

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040622\
 Data File : FB026845.D
 Signal(s) : FID2B.CH
 Acq On : 6 Apr 2022 12:00
 Operator : AJ/MA
 Sample : BSF0406S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0406S1

Integration File: SAMPLE.e
 Quant Time: Apr 06 16:12:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	221729	21.130 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.703	391198	20.662 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	472791	22.810 ng/ml
3) t n-Heptane	7.750	140400	7.093 ng/ml
4) t Benzene	7.885	203706	8.828 ng/ml
6) t Toluene	10.619	583470	26.651 ng/ml
7) t Ethylbenzene	13.055	184397	9.175 ng/ml
8) t m-Xylene	13.188	362133	17.970 ng/ml
9) t O-Xylene	13.915	362487	18.170 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	372312	18.686 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040622\
Data File : FB026845.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2022 12:00
Operator : AJ/MA
Sample : BSF0406S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0406S1

Integration File: SAMPLE.e
Quant Time: Apr 06 16:12:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

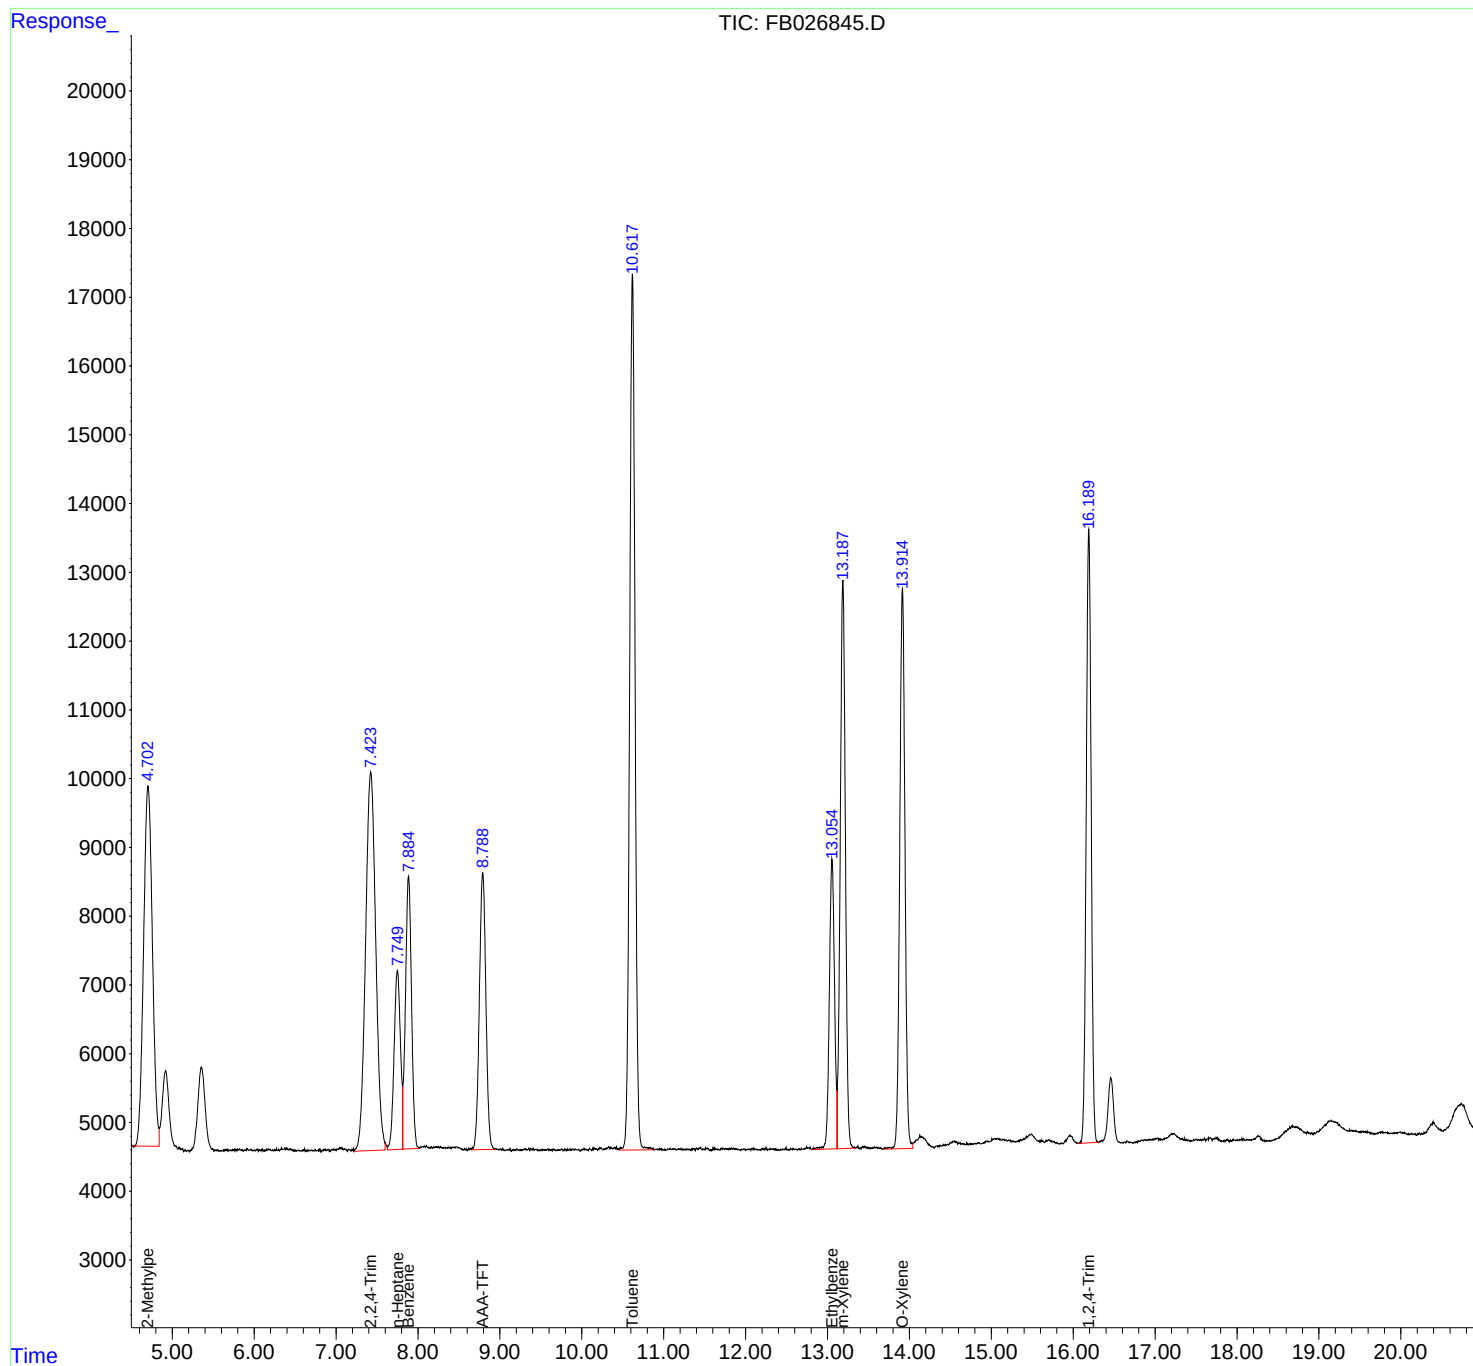


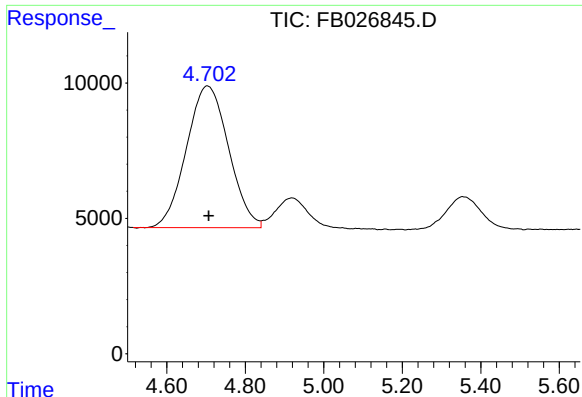

#1 2-Methylpentane


R.T.: 4.703 min
Delta R.T.: -0.004 min
Response: 391198
Conc: 20.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0406S1

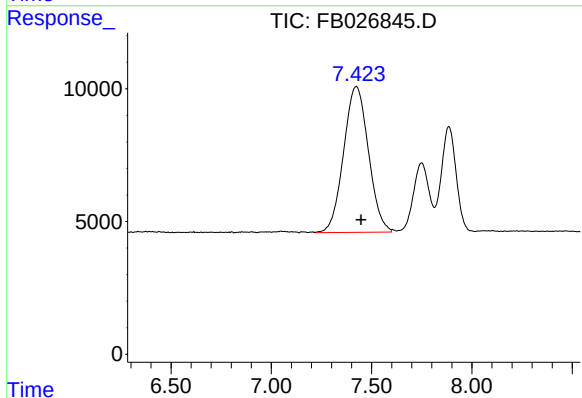


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.022 min
Response: 472791
Conc: 22.81 ng/ml

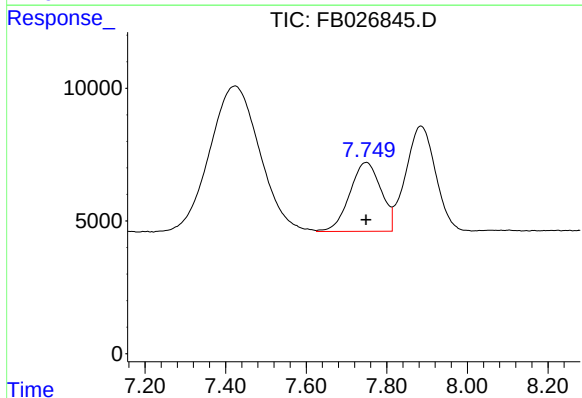


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 140400
Conc: 7.09 ng/ml

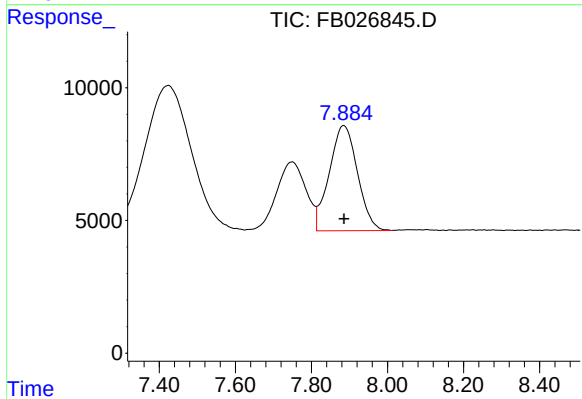

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 203706
Conc: 8.83 ng/ml

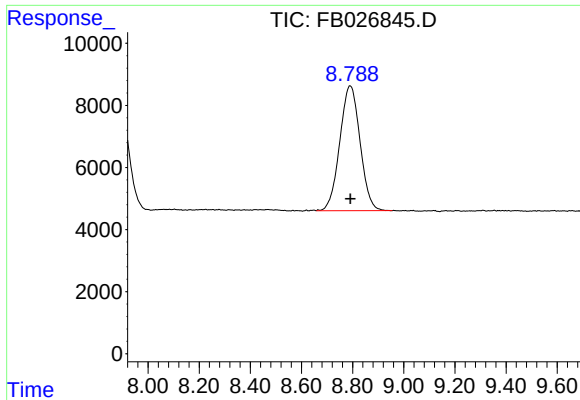

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 221729
Conc: 21.13 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0406S1

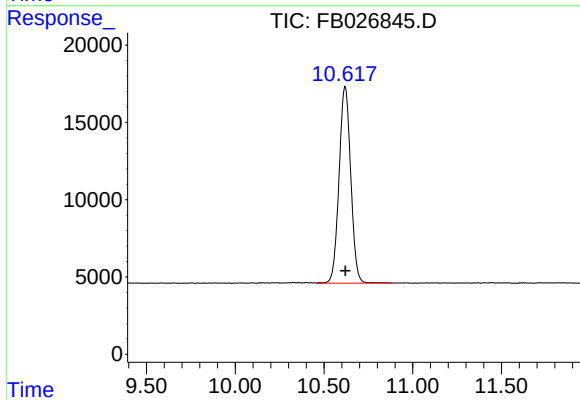


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 583470
Conc: 26.65 ng/ml

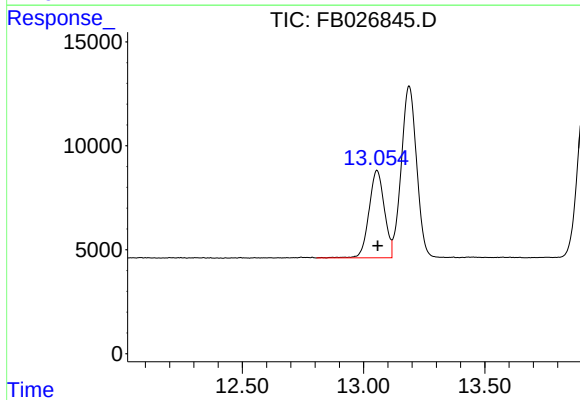


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.003 min
Response: 184397
Conc: 9.18 ng/ml

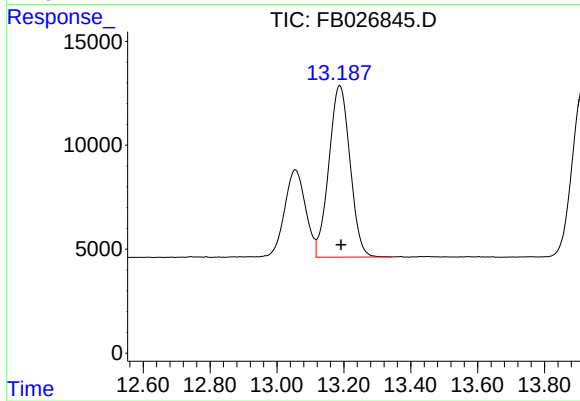

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 362133
Conc: 17.97 ng/ml

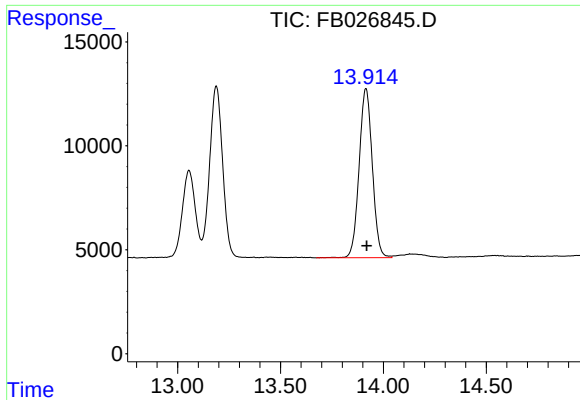

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.003 min
Response: 362487
Conc: 18.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0406S1

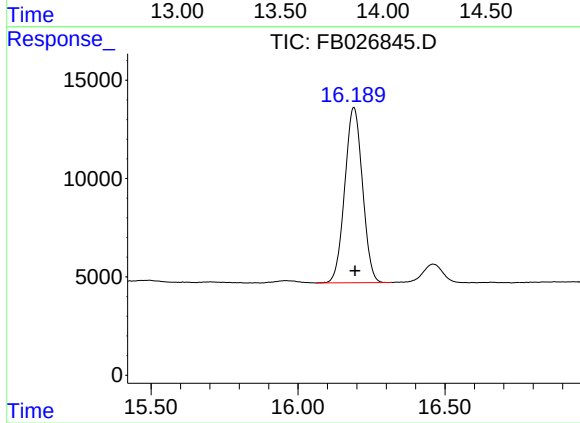

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 372312
Conc: 18.69 ng/ml