

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040623\
Data File : FB029581.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2023 10:57
Operator : YP/AJ
Sample : VBF0406S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0406S2

Integration File: Calibration.e
Quant Time: Apr 07 03:42:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	255679	17.938 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040623\
Data File : FB029581.D
Signal(s) : FID2B.CH
Acq On : 6 Apr 2023 10:57
Operator : YP/AJ
Sample : VBF0406S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0406S2

Integration File: Calibration.e
Quant Time: Apr 07 03:42:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

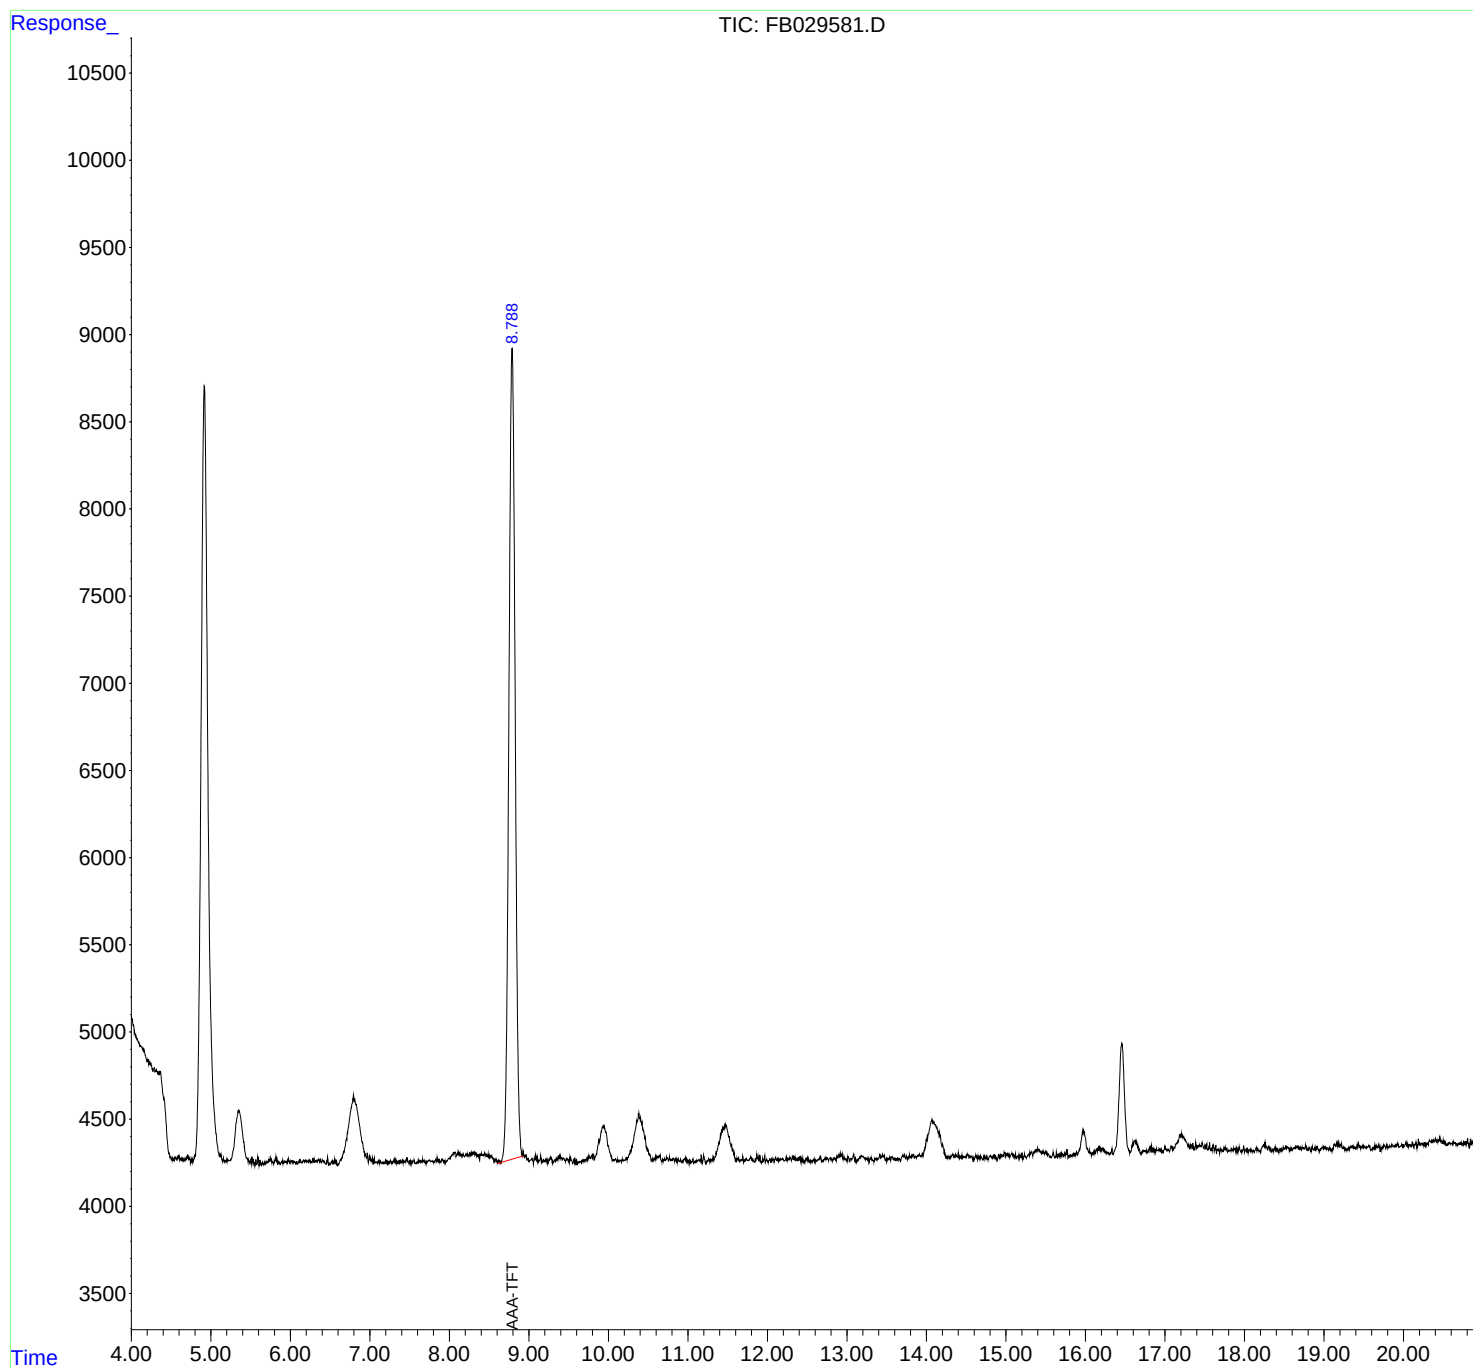

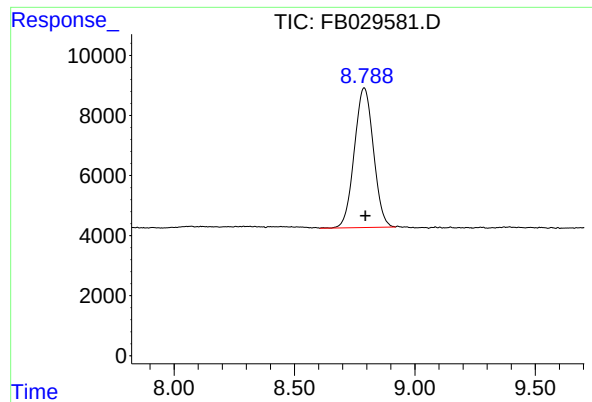

#5 AAA-TFT

R.T.: 8.790 min
Delta R.T.: -0.004 min
Response: 255679
Conc: 17.94 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0406S2