

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
Data File : FB026864.D
Signal(s) : FID2B.CH
Acq On : 7 Apr 2022 17:42
Operator : AJ/MA
Sample : N2254-01MSD
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 04:32:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.451	598	0.029 ng/ml
6) t Toluene	10.630	1482	0.068 ng/ml
7) t Ethylbenzene	13.034	17764	0.884 ng/ml
8) t m-Xylene	13.147	535	0.027 ng/ml
9) t O-Xylene	13.961	5883	0.295 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
Data File : FB026864.D
Signal(s) : FID2B.CH
Acq On : 7 Apr 2022 17:42
Operator : AJ/MA
Sample : N2254-01MSD
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 04:32:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

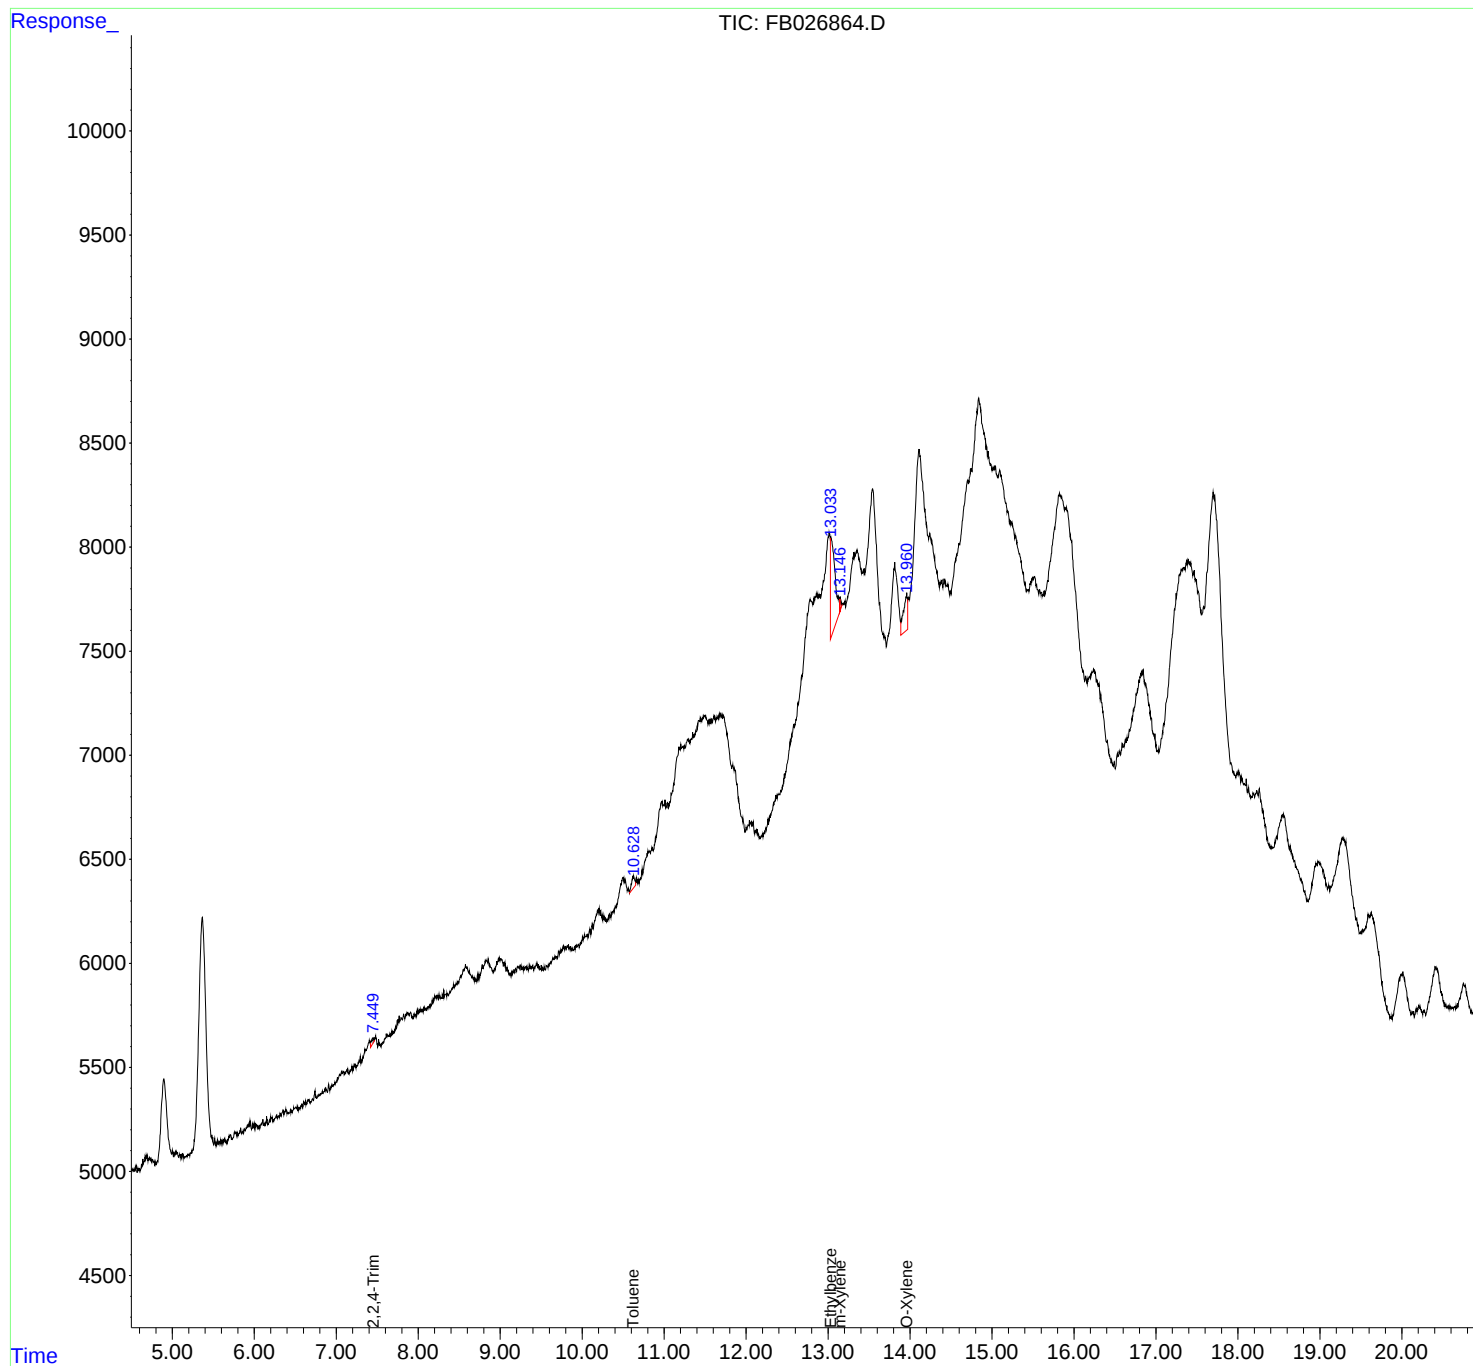


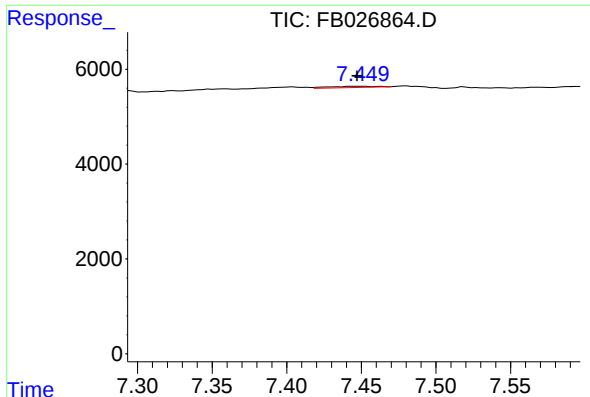

#2 2,2,4-Trimethylpentane


R.T.: 7.451 min
Delta R.T.: 0.004 min
Response: 598
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :

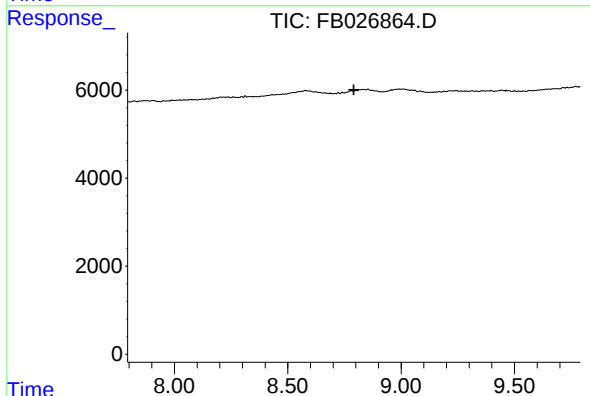


#5 AAA-TFT

R.T.: 0.000 min
Exp R.T. : 8.792 min
Response: 0
Conc: N.D.

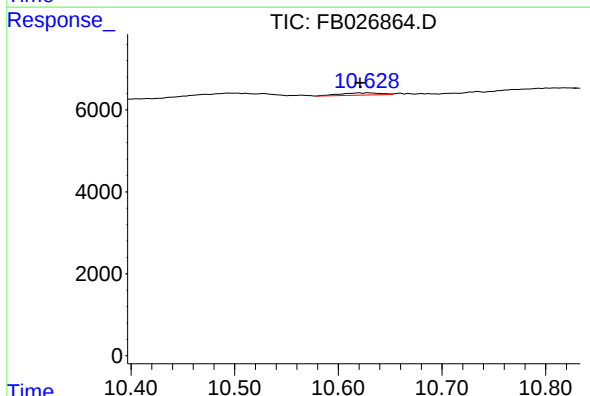


#6 Toluene

R.T.: 10.630 min
Delta R.T.: 0.008 min
Response: 1482
Conc: 0.07 ng/ml

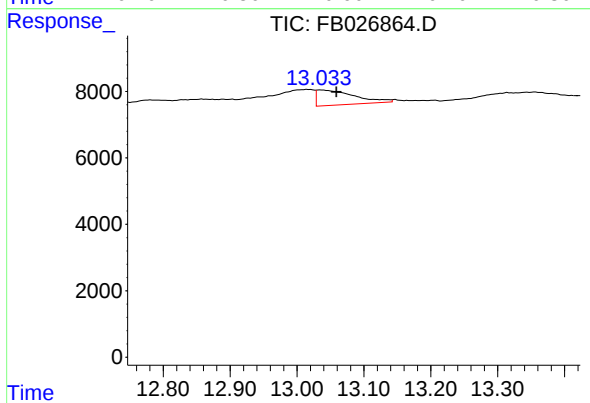

#7 Ethylbenzene


R.T.: 13.034 min
Delta R.T.: -0.024 min
Response: 17764
Conc: 0.88 ng/ml

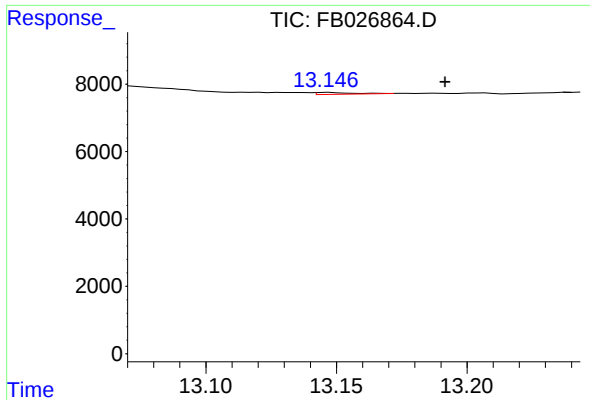

#8 m-Xylene

R.T.: 13.147 min
Delta R.T.: -0.044 min
Response: 535
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :

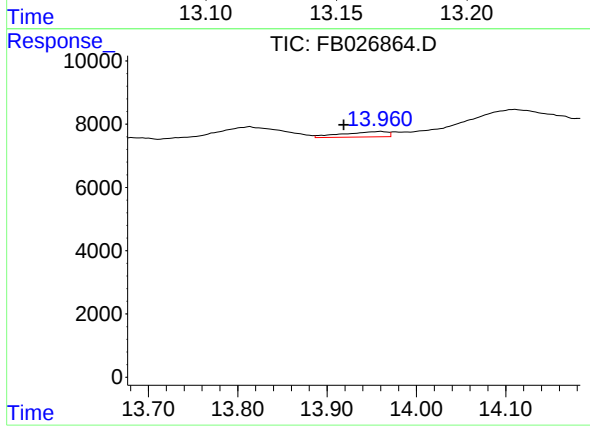

#9 o-Xylene

R.T.: 13.961 min
Delta R.T.: 0.042 min
Response: 5883
Conc: 0.29 ng/ml