

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
 Data File : FB026867.D
 Signal(s) : FID2B.CH
 Acq On : 7 Apr 2022 19:47
 Operator : AJ/MA
 Sample : N2254-03 50X
 Misc : 5.04G/5.00 ML DI WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 08 04:33:13 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	407920	38.874 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	21915	1.157 ng/ml
2) t 2,2,4-Trimethylpentane	7.468	76563	3.694 ng/ml
3) t n-Heptane	7.796	185022	9.348 ng/ml
7) t Ethylbenzene	13.017	446348	22.209 ng/ml
9) t O-Xylene	13.937	60574	3.036 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
Data File : FB026867.D
Signal(s) : FID2B.CH
Acq On : 7 Apr 2022 19:47
Operator : AJ/MA
Sample : N2254-03 50X
Misc : 5.04G/5.00 ML DI WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 04:33:13 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

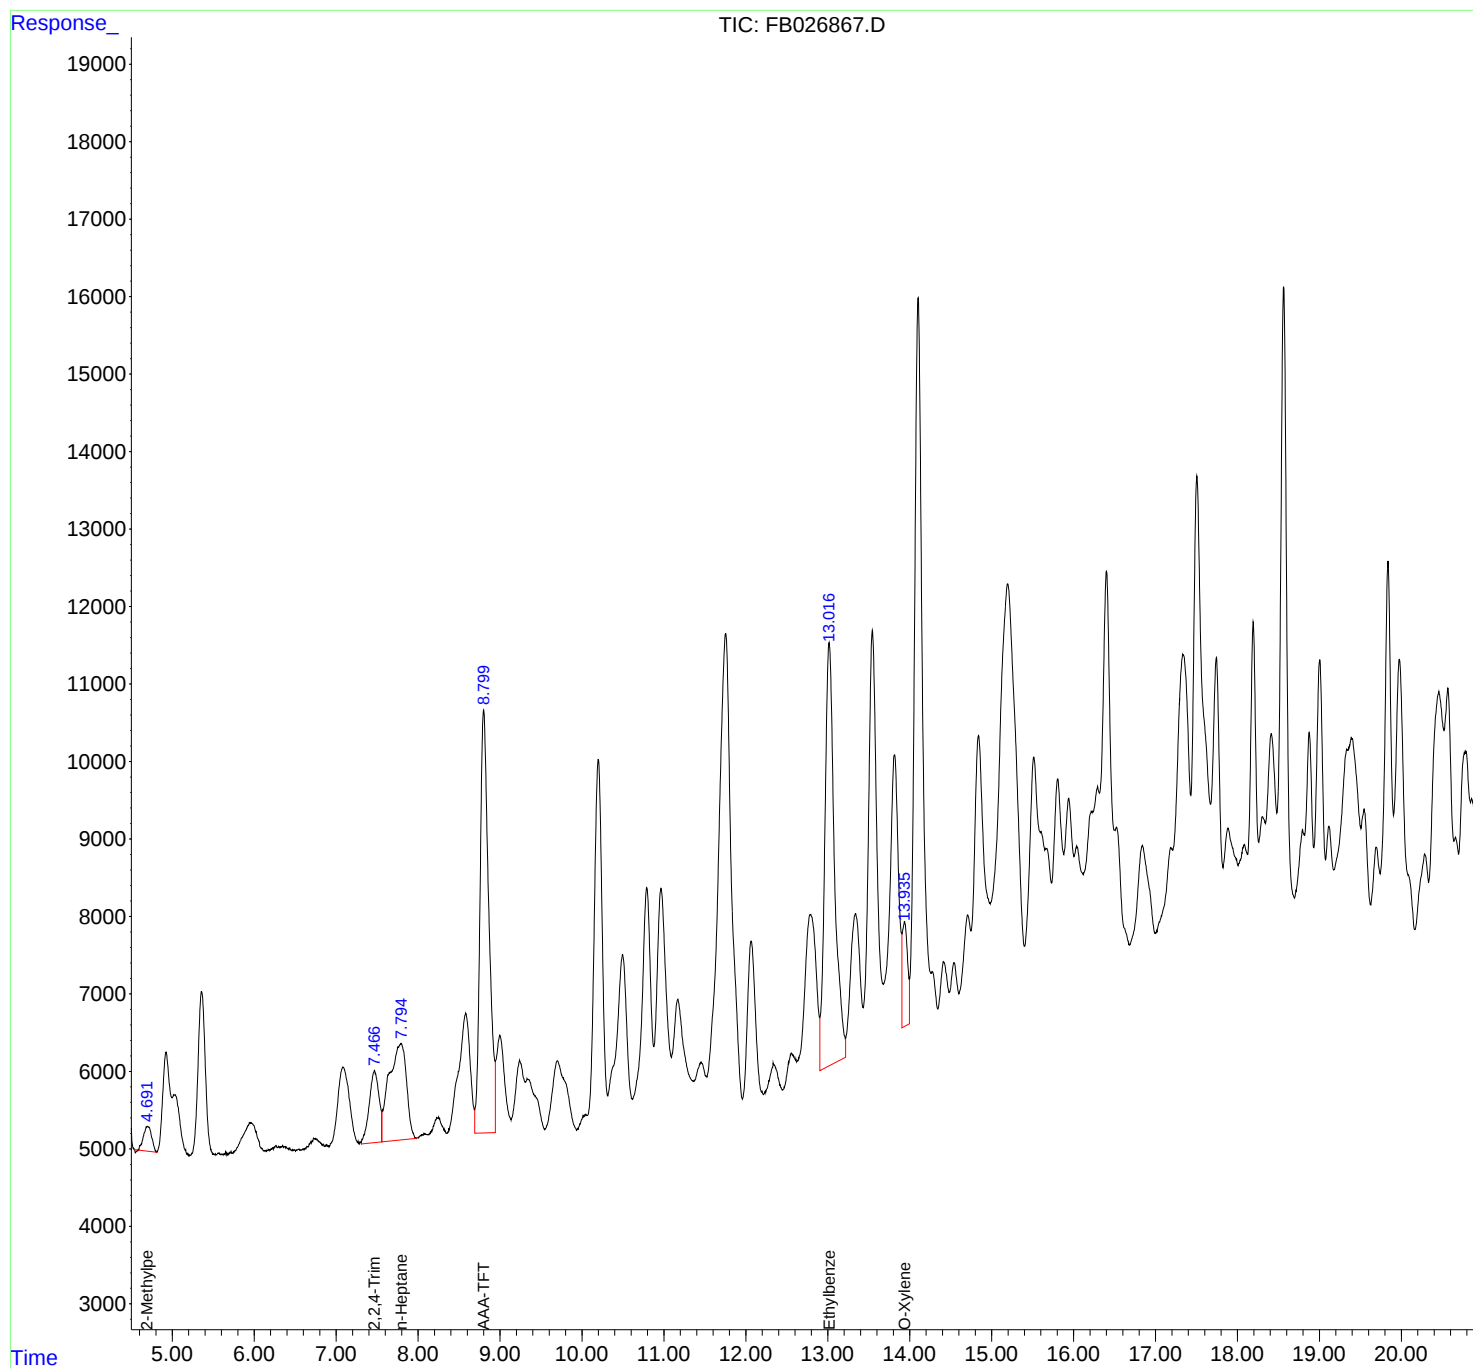


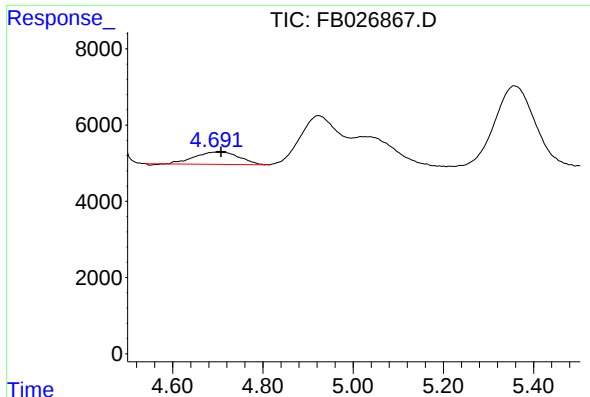

#1 2-Methylpentane


R.T.: 4.693 min
Delta R.T.: -0.014 min
Response: 21915
Conc: 1.16 ng/ml

Instrument :
FID_B
ClientSampleId :

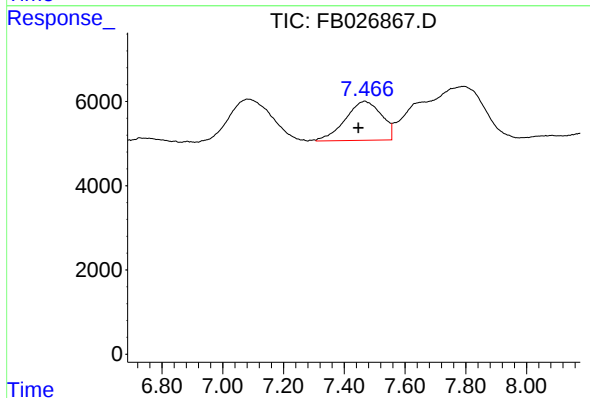


#2 2,2,4-Trimethylpentane

R.T.: 7.468 min
Delta R.T.: 0.021 min
Response: 76563
Conc: 3.69 ng/ml

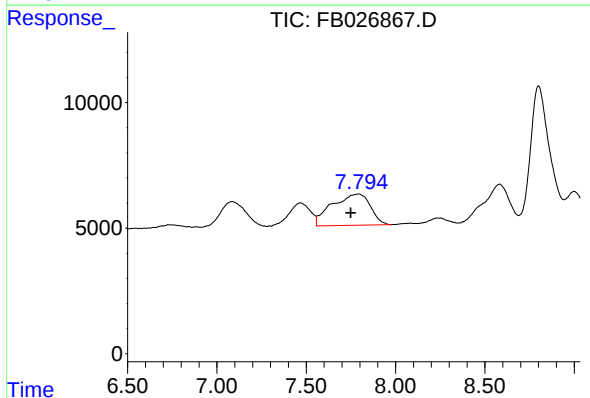


#3 n-Heptane

R.T.: 7.796 min
Delta R.T.: 0.047 min
Response: 185022
Conc: 9.35 ng/ml

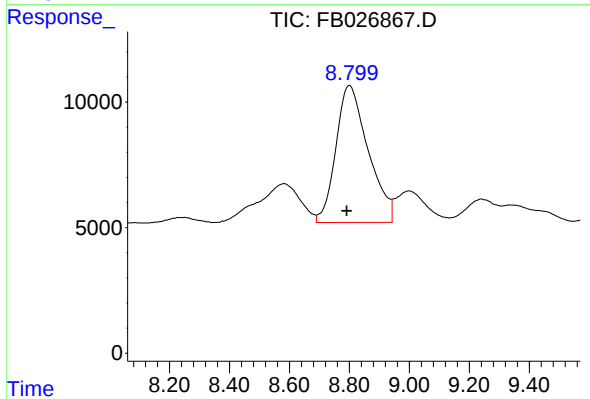

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.009 min
Response: 407920
Conc: 38.87 ng/ml

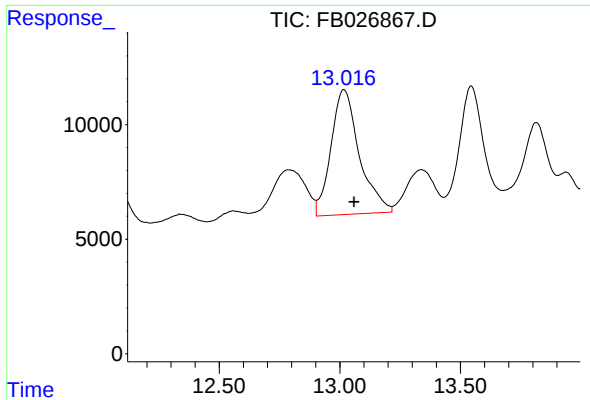

#7 Ethylbenzene

R.T.: 13.017 min
Delta R.T.: -0.042 min
Response: 446348
Conc: 22.21 ng/ml

Instrument :
FID_B
ClientSampleId :

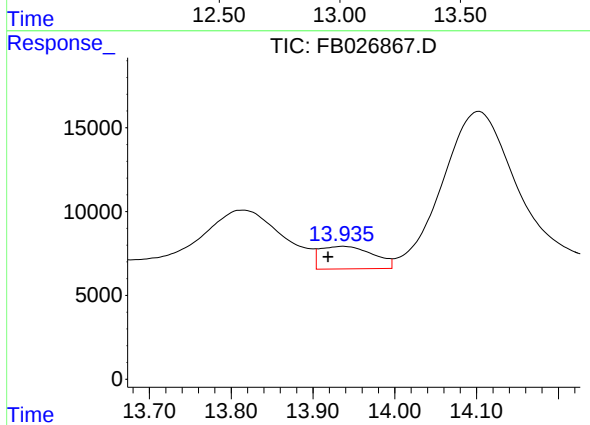

#9 O-Xylene

R.T.: 13.937 min
Delta R.T.: 0.019 min
Response: 60574
Conc: 3.04 ng/ml