

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
 Data File : FB026856.D
 Signal(s) : FID2B.CH
 Acq On : 7 Apr 2022 12:00
 Operator : AJ/MA
 Sample : BSF0407S1
 Misc : 5.0G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0407S1

Integration File: SAMPLE.e
 Quant Time: Apr 07 12:32:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	246011	23.444 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	346543	18.303 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	417547	20.145 ng/ml
3) t n-Heptane	7.750	122572	6.193 ng/ml
4) t Benzene	7.885	188730	8.179 ng/ml
6) t Toluene	10.619	541261	24.723 ng/ml
7) t Ethylbenzene	13.056	171913	8.554 ng/ml
8) t m-Xylene	13.188	336065	16.676 ng/ml
9) t O-Xylene	13.916	329314	16.507 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	331220	16.624 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040722\
Data File : FB026856.D
Signal(s) : FID2B.CH
Acq On : 7 Apr 2022 12:00
Operator : AJ/MA
Sample : BSF0407S1
Misc : 5.0G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0407S1

Integration File: SAMPLE.e
Quant Time: Apr 07 12:32:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

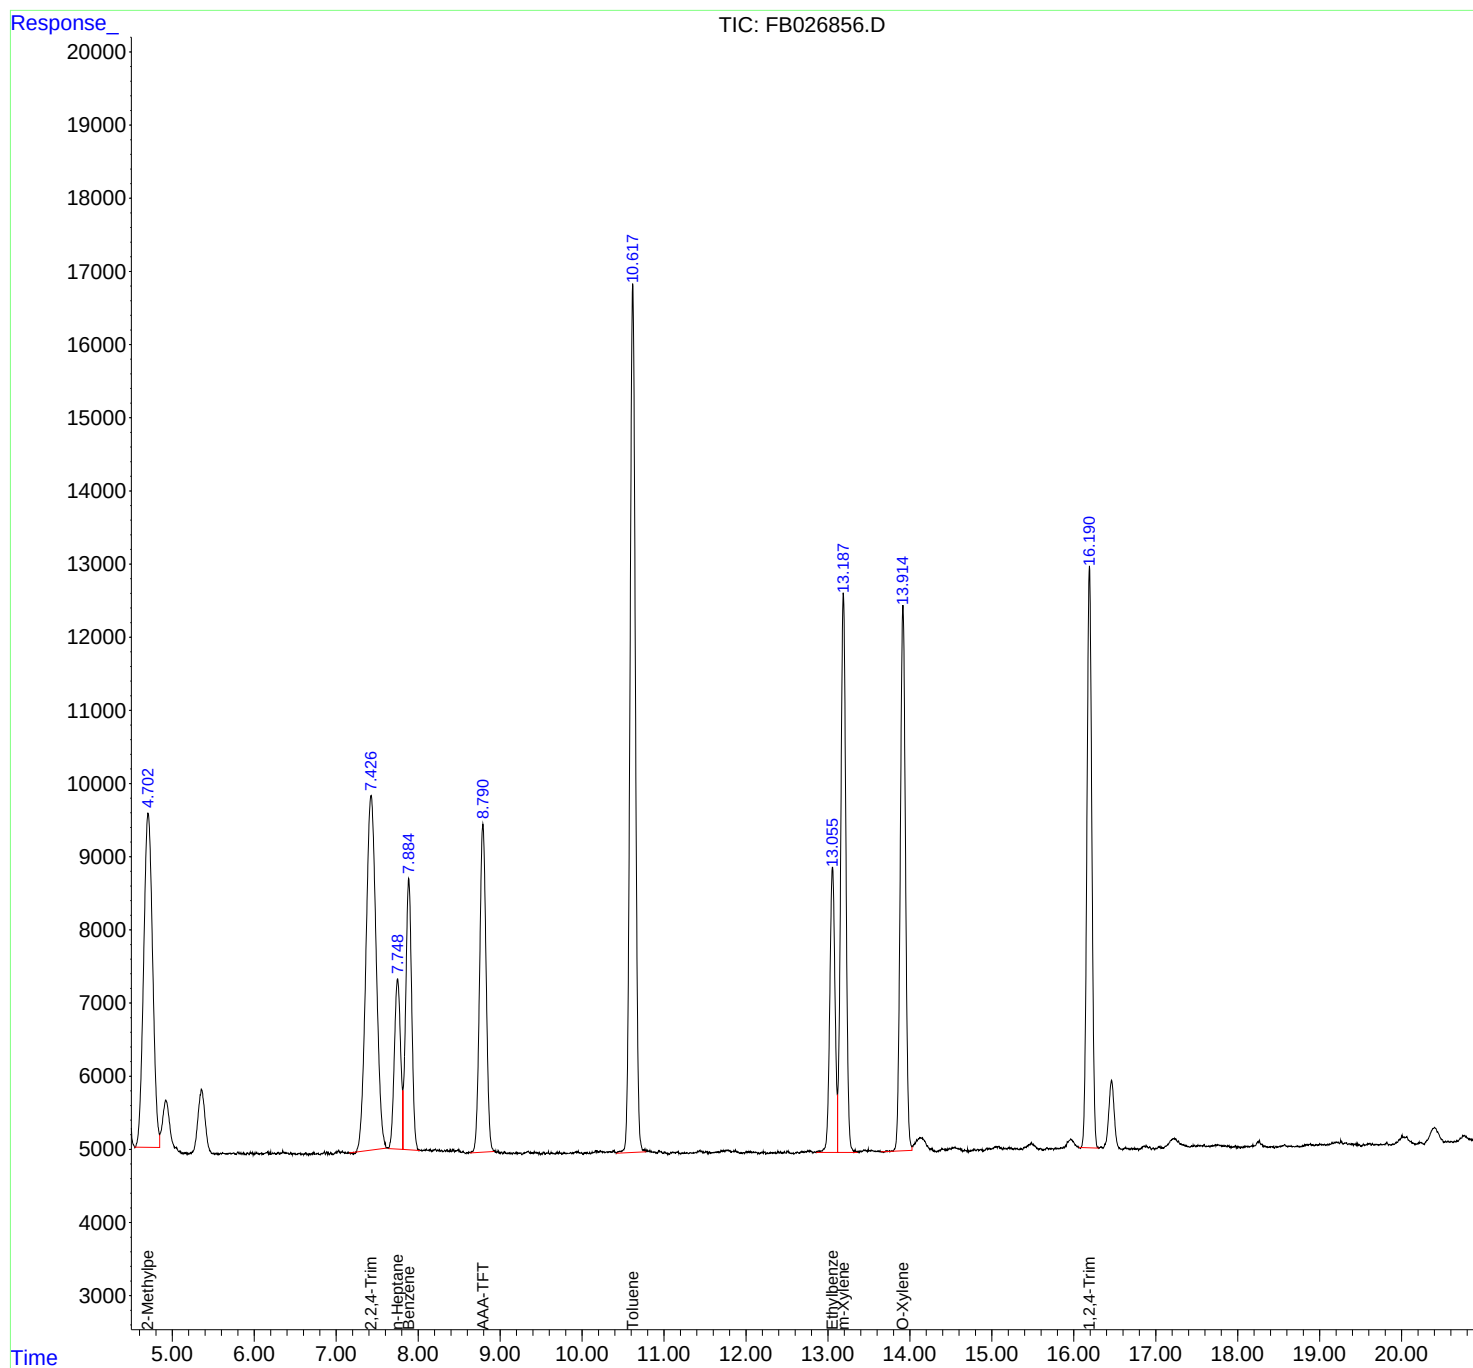


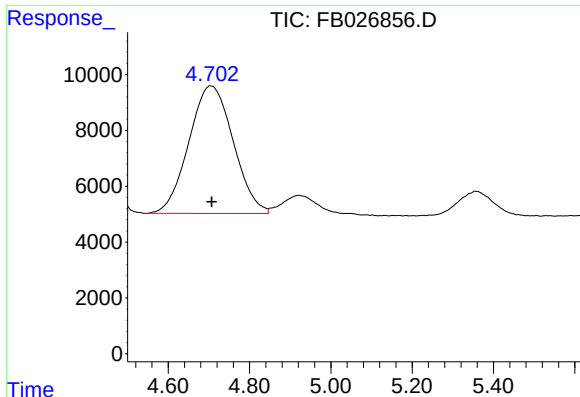

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 346543
Conc: 18.30 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0407S1

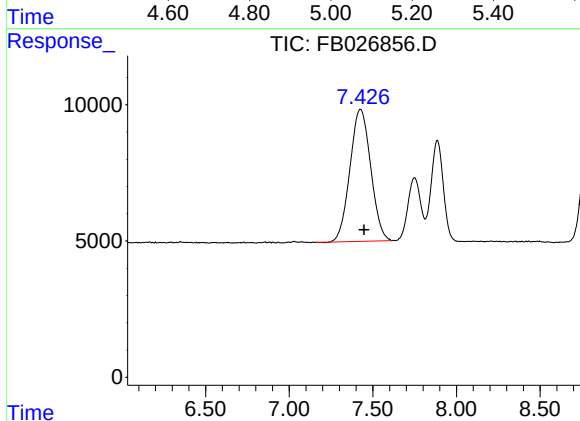


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 417547
Conc: 20.14 ng/ml

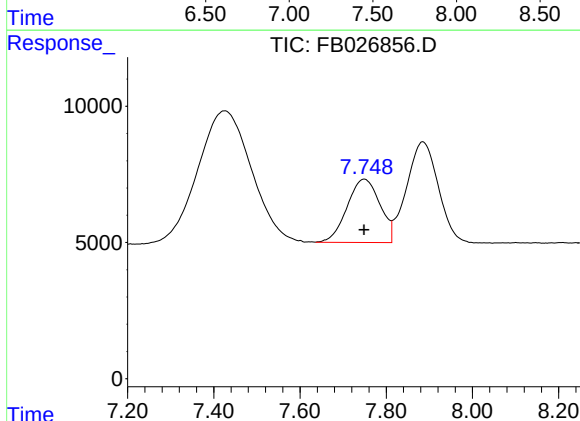


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: 0.001 min
Response: 122572
Conc: 6.19 ng/ml

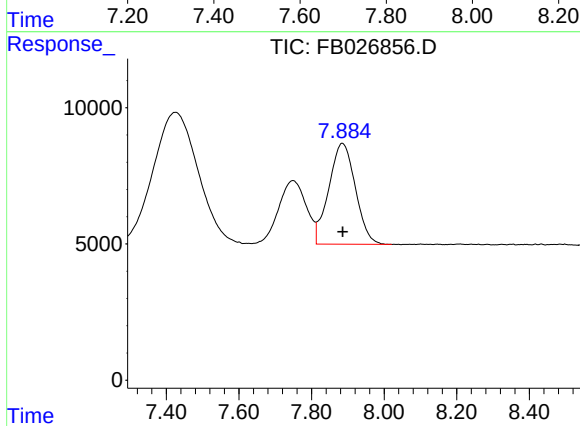

#4 Benzene


R.T.: 7.885 min
Delta R.T.: 0.000 min
Response: 188730
Conc: 8.18 ng/ml

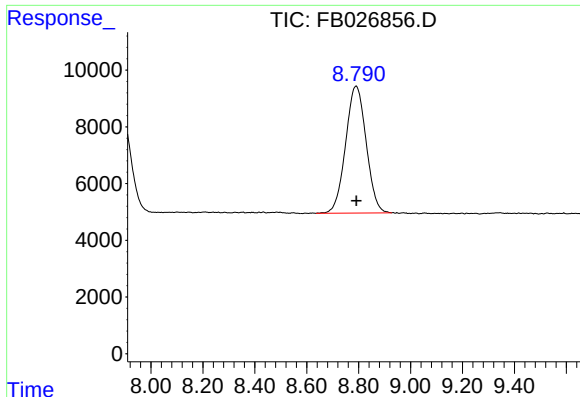

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 246011
Conc: 23.44 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0407S1

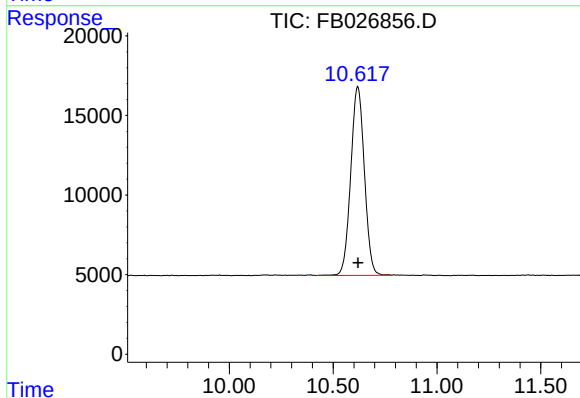


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 541261
Conc: 24.72 ng/ml

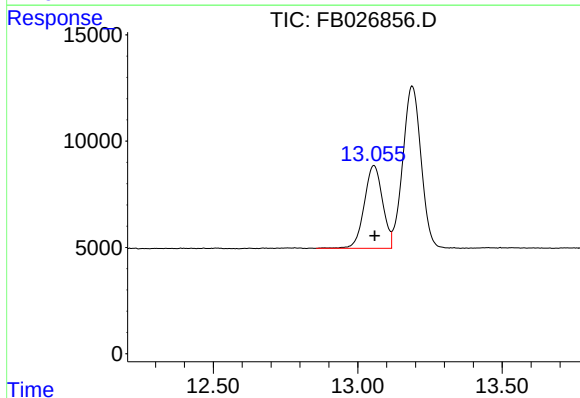


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 171913
Conc: 8.55 ng/ml

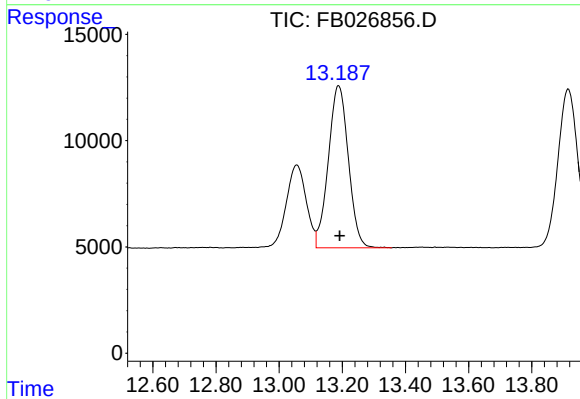

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.003 min
Response: 336065
Conc: 16.68 ng/ml

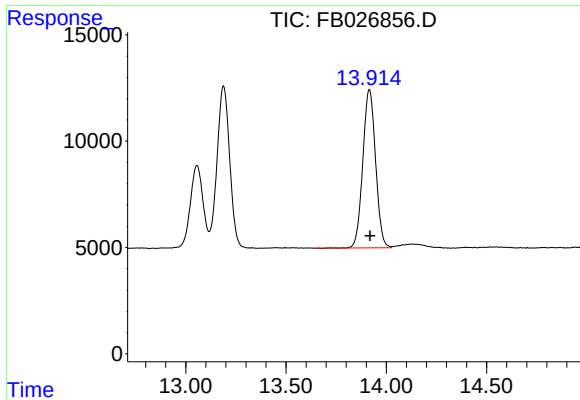

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.003 min
Response: 329314
Conc: 16.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0407S1

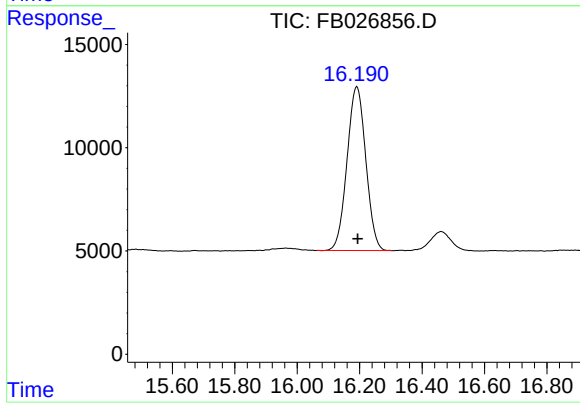

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.003 min
Response: 331220
Conc: 16.62 ng/ml