

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040723\
 Data File : FB029597.D
 Signal(s) : FID2B.CH
 Acq On : 7 Apr 2023 10:51
 Operator : YP/AJ
 Sample : BSF0407S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 10 03:51:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	273370	19.179 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	504779	30.066 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	558832	30.355 ng/ml
3) t n-Heptane	7.746	186070	9.552 ng/ml
4) t Benzene	7.882	221162	9.789 ng/ml
6) t Toluene	10.614	636277	28.863 ng/ml
7) t Ethylbenzene	13.050	204526	9.894 ng/ml
8) t m-Xylene	13.183	404500	19.769 ng/ml
9) t O-Xylene	13.910	392485	19.812 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	401390	21.025 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040723\
Data File : FB029597.D
Signal(s) : FID2B.CH
Acq On : 7 Apr 2023 10:51
Operator : YP/AJ
Sample : BSF0407S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 10 03:51:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

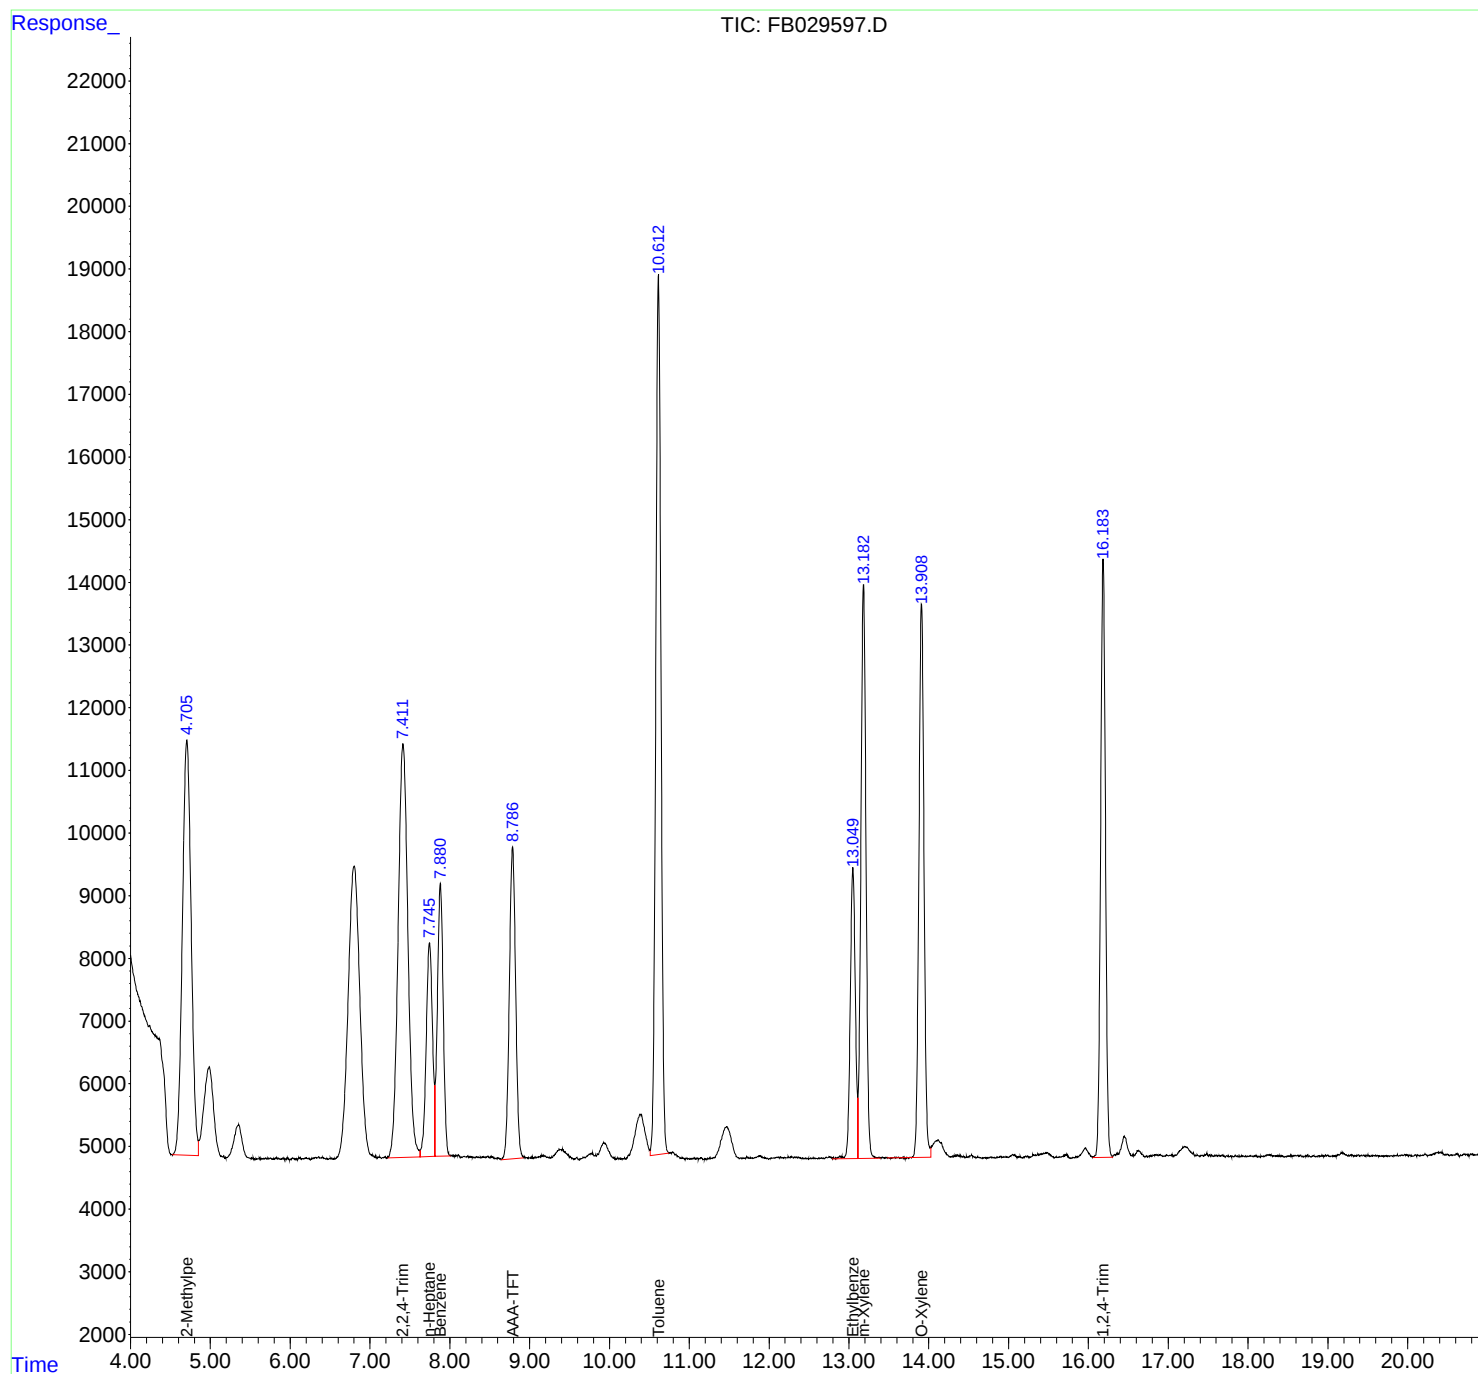

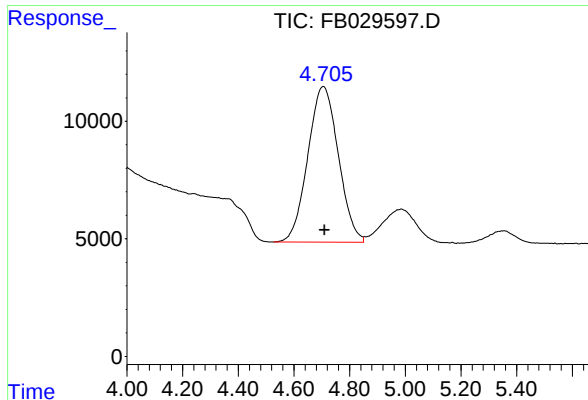


#1 2-Methylpentane

R.T.: 4.706 min
Delta R.T.: -0.004 min
Response: 504779
Conc: 30.07 ng/ml

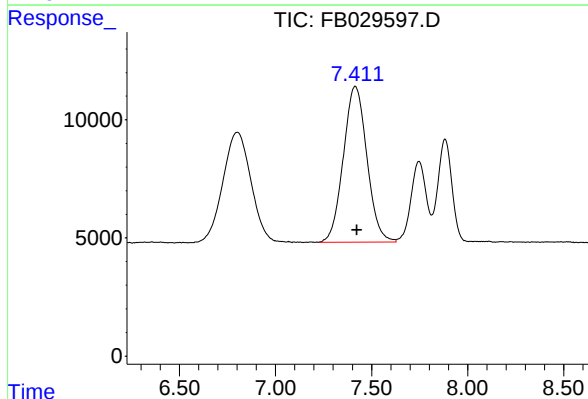


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.010 min
Response: 558832
Conc: 30.36 ng/ml

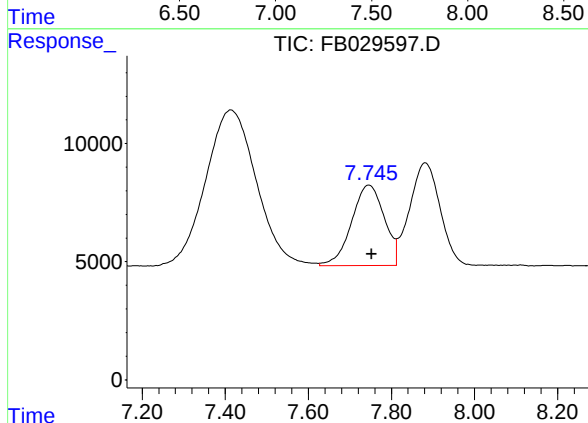


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.007 min
Response: 186070
Conc: 9.55 ng/ml

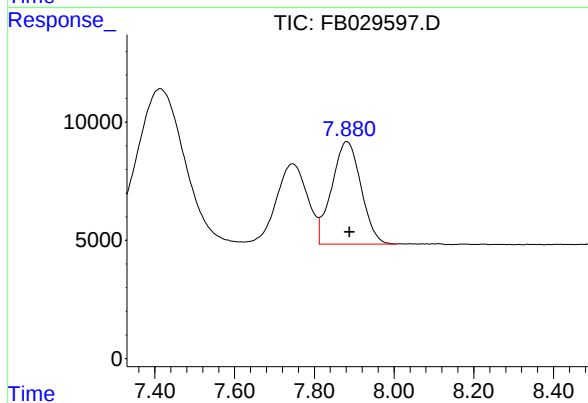


#4 Benzene

R.T.: 7.882 min
Delta R.T.: -0.007 min
Response: 221162
Conc: 9.79 ng/ml

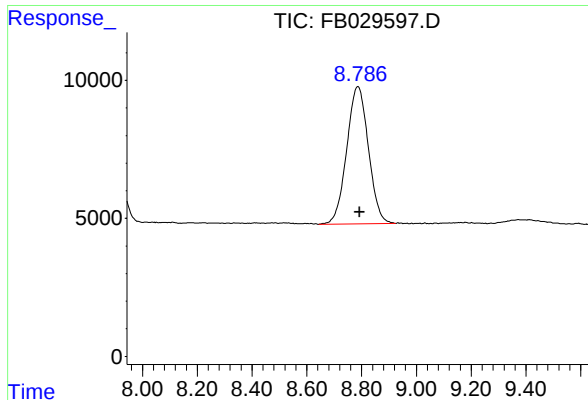


#5 AAA-TFT

R.T.: 8.787 min
Delta R.T.: -0.007 min
Response: 273370
Conc: 19.18 ng/ml

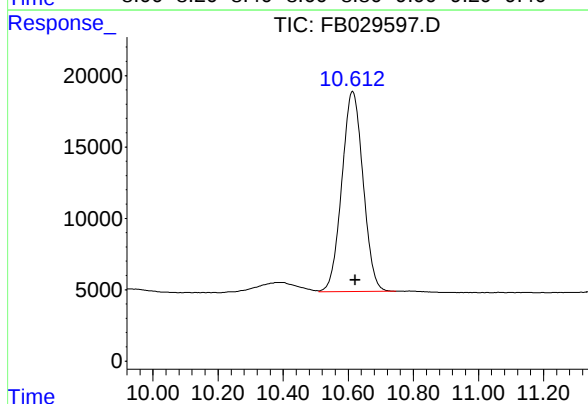


#6 Toluene

R.T.: 10.614 min
Delta R.T.: -0.008 min
Response: 636277
Conc: 28.86 ng/ml

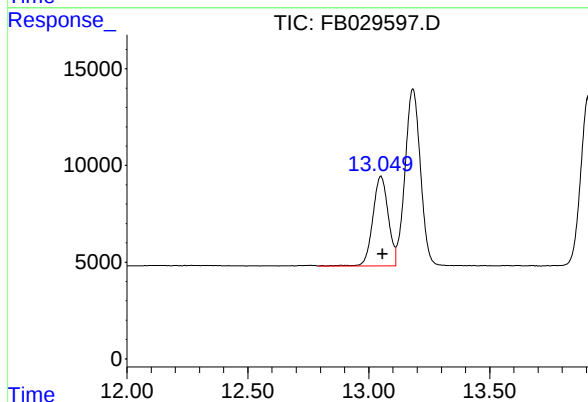


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: -0.008 min
Response: 204526
Conc: 9.89 ng/ml

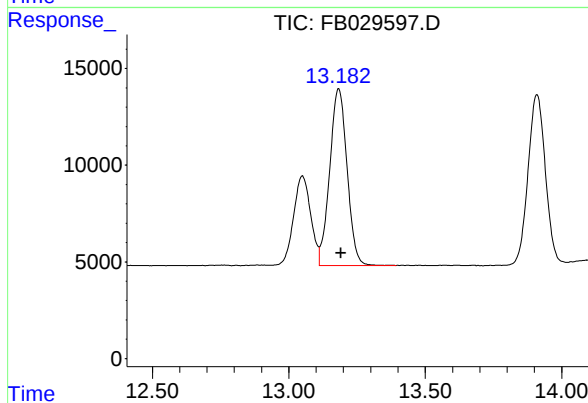


#8 m-Xylene

R.T.: 13.183 min
Delta R.T.: -0.008 min
Response: 404500
Conc: 19.77 ng/ml

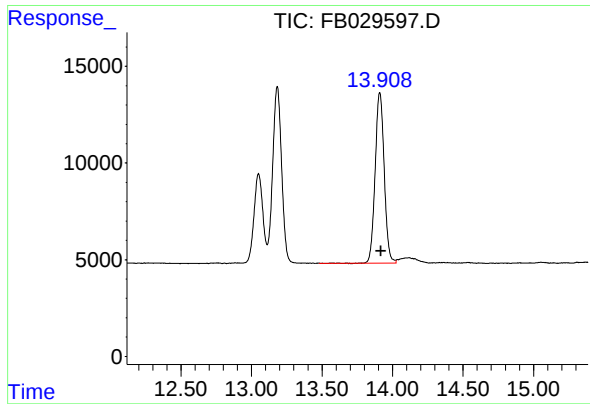

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.008 min
Response: 392485
Conc: 19.81 ng/ml

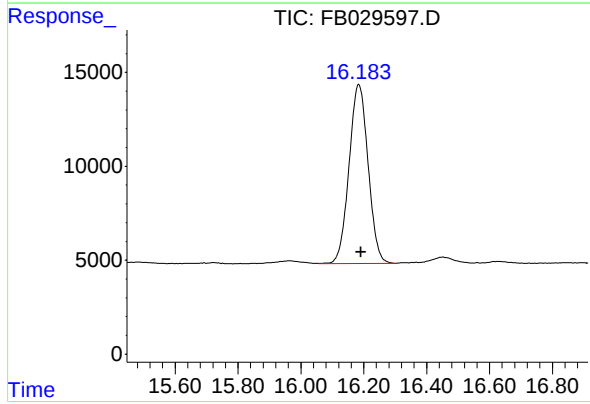

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: -0.007 min
Response: 401390
Conc: 21.02 ng/ml