

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040819\
 Data File : FB020583.D
 Signal(s) : FID2B.CH
 Acq On : 8 Apr 2019 15:24
 Operator : MJ/SJ
 Sample : K2309-01MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 09 02:10:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.001	338425	18.348 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.869	851326	24.183 ng/ml
2) t	2,2,4-Trimethylpentane	7.630	626085	21.000 ng/ml
3) t	n-Heptane	7.958	260502	6.636 ng/ml
4) t	Benzene	8.094	368850	8.980 ng/ml
6) t	Toluene	10.845	770556	25.502 ng/ml
7) t	Ethylbenzene	13.296	213760	8.356 ng/ml
8) t	m-Xylene	13.429	436019	16.498 ng/ml
9) t	O-Xylene	14.160	450098	16.626 ng/ml
10) t	1,2,4-Trimethylbenzene	16.444	411643	15.755 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040819\
Data File : FB020583.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2019 15:24
Operator : MJ/SJ
Sample : K2309-01MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 09 02:10:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

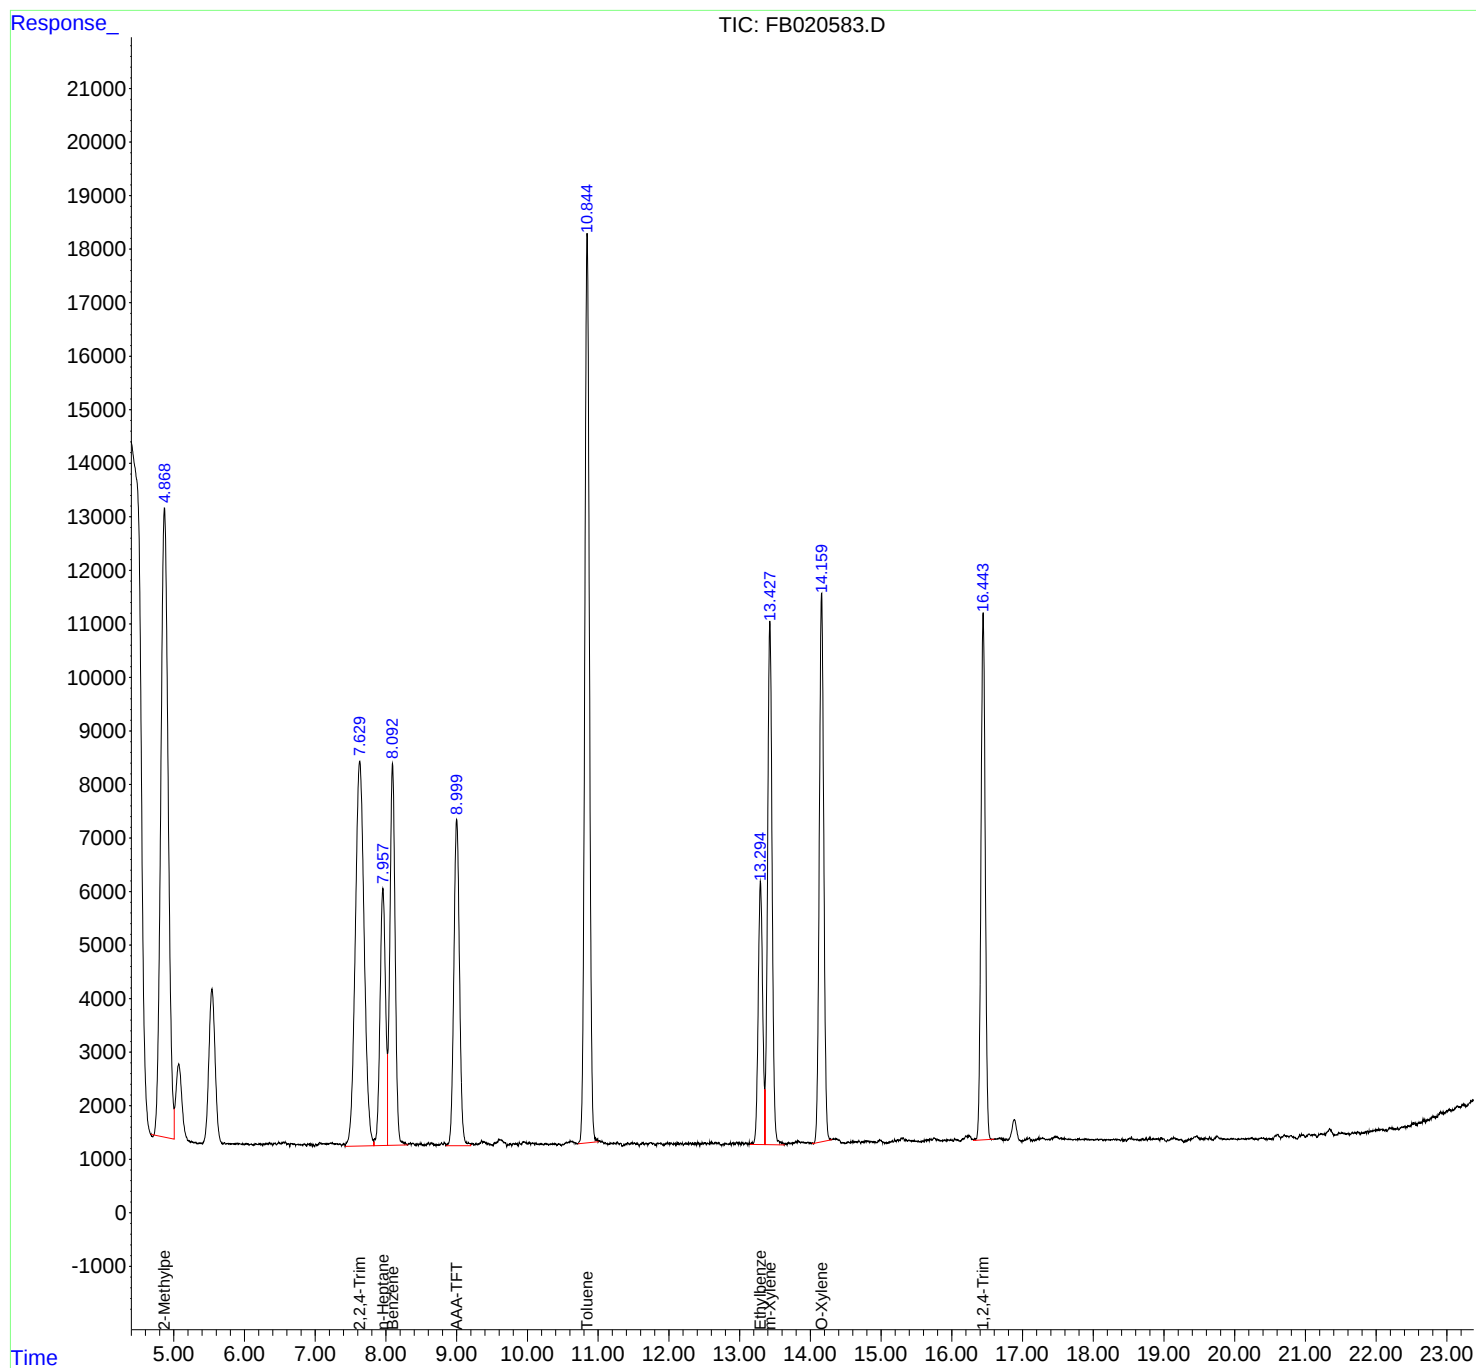

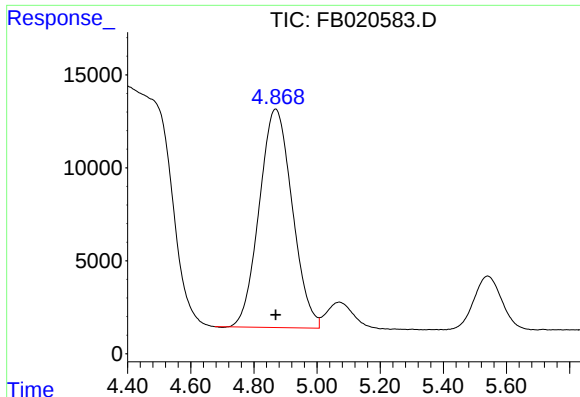


#1 2-Methylpentane

R.T.: 4.869 min
Delta R.T.: 0.000 min
Response: 851326
Conc: 24.18 ng/ml

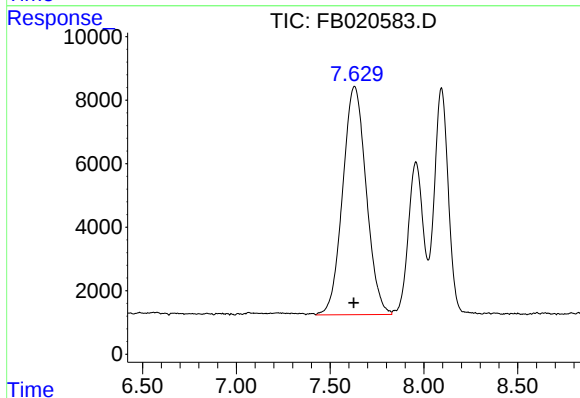


#2 2,2,4-Trimethylpentane

R.T.: 7.630 min
Delta R.T.: 0.004 min
Response: 626085
Conc: 21.00 ng/ml

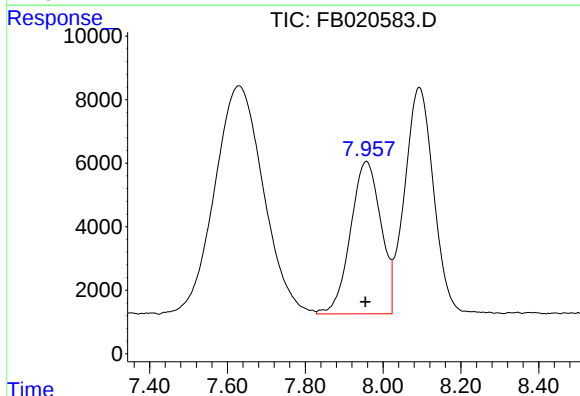


#3 n-Heptane

R.T.: 7.958 min
Delta R.T.: 0.002 min
Response: 260502
Conc: 6.64 ng/ml

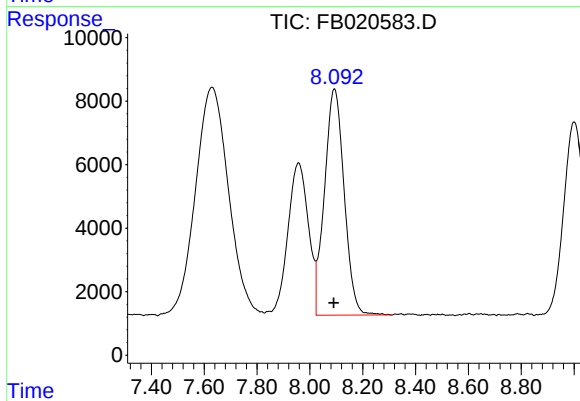


#4 Benzene

R.T.: 8.094 min
Delta R.T.: 0.003 min
Response: 368850
Conc: 8.98 ng/ml

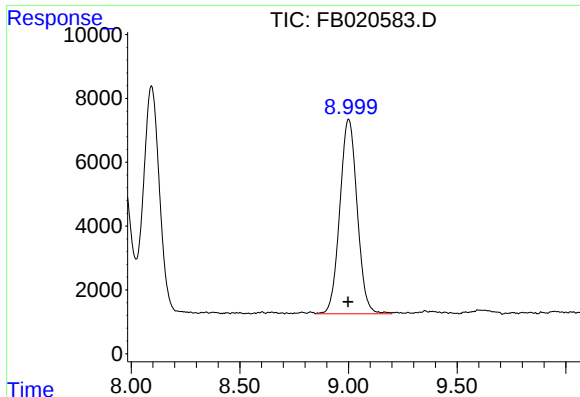


#5 AAA-TFT

R.T.: 9.001 min
Delta R.T.: 0.002 min
Response: 338425
Conc: 18.35 ng/ml

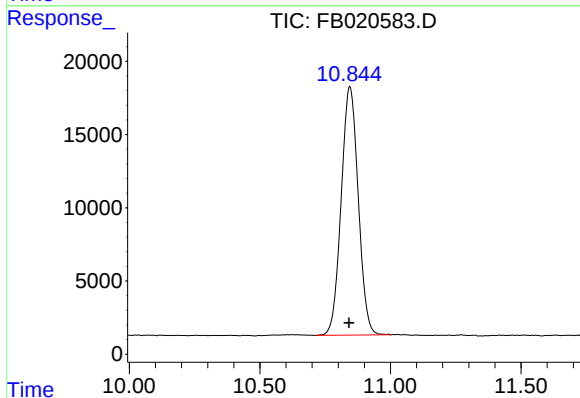


#6 Toluene

R.T.: 10.845 min
Delta R.T.: 0.003 min
Response: 770556
Conc: 25.50 ng/ml

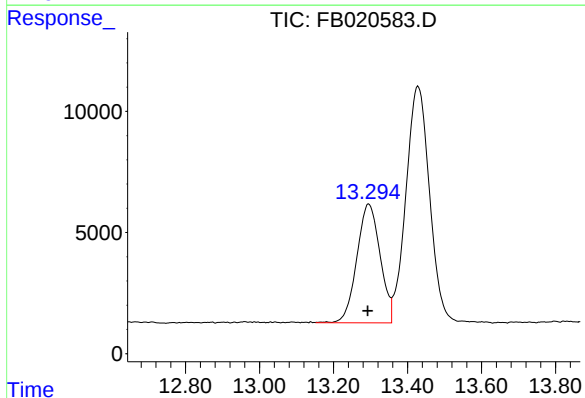


#7 Ethylbenzene

R.T.: 13.296 min
Delta R.T.: 0.003 min
Response: 213760
Conc: 8.36 ng/ml

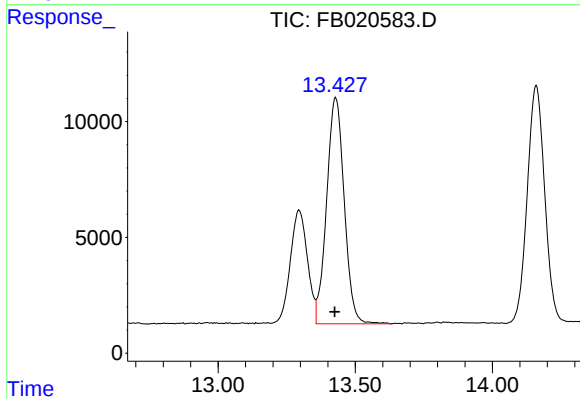


#8 m-Xylene

R.T.: 13.429 min
Delta R.T.: 0.003 min
Response: 436019
Conc: 16.50 ng/ml

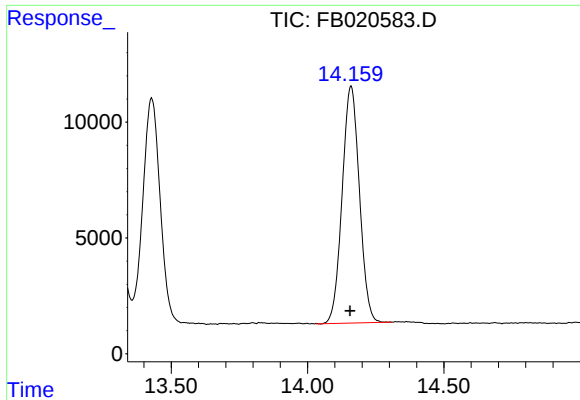

#9 O-Xylene

R.T.: 14.160 min
Delta R.T.: 0.003 min
Response: 450098
Conc: 16.63 ng/ml

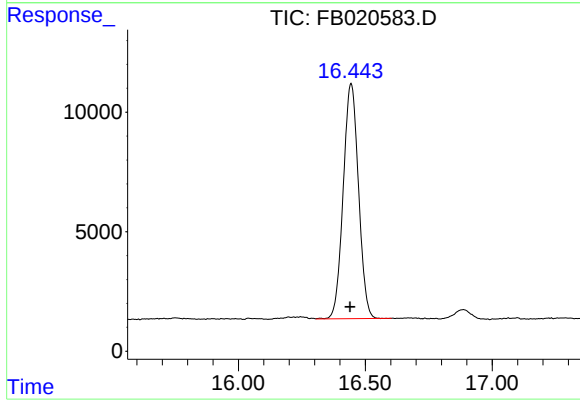

#10 1,2,4-Trimethylbenzene

R.T.: 16.444 min
Delta R.T.: 0.004 min
Response: 411643
Conc: 15.76 ng/ml