

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
Data File : FB026874.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2022 10:09
Operator : AJ/MA
Sample : VBF0408S1 50X
Misc : 5.02G/5.00 ML DI MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 14:15:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	173616	16.545 ng/ml
Target Compounds			
6) t Toluene	10.625	12135	0.554 ng/ml
8) t m-Xylene	13.185	7561	0.375 ng/ml
9) t O-Xylene	13.910	7461	0.374 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	9017	0.453 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
Data File : FB026874.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2022 10:09
Operator : AJ/MA
Sample : VBF0408S1 50X
Misc : 5.02G/5.00 ML DI MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 14:15:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

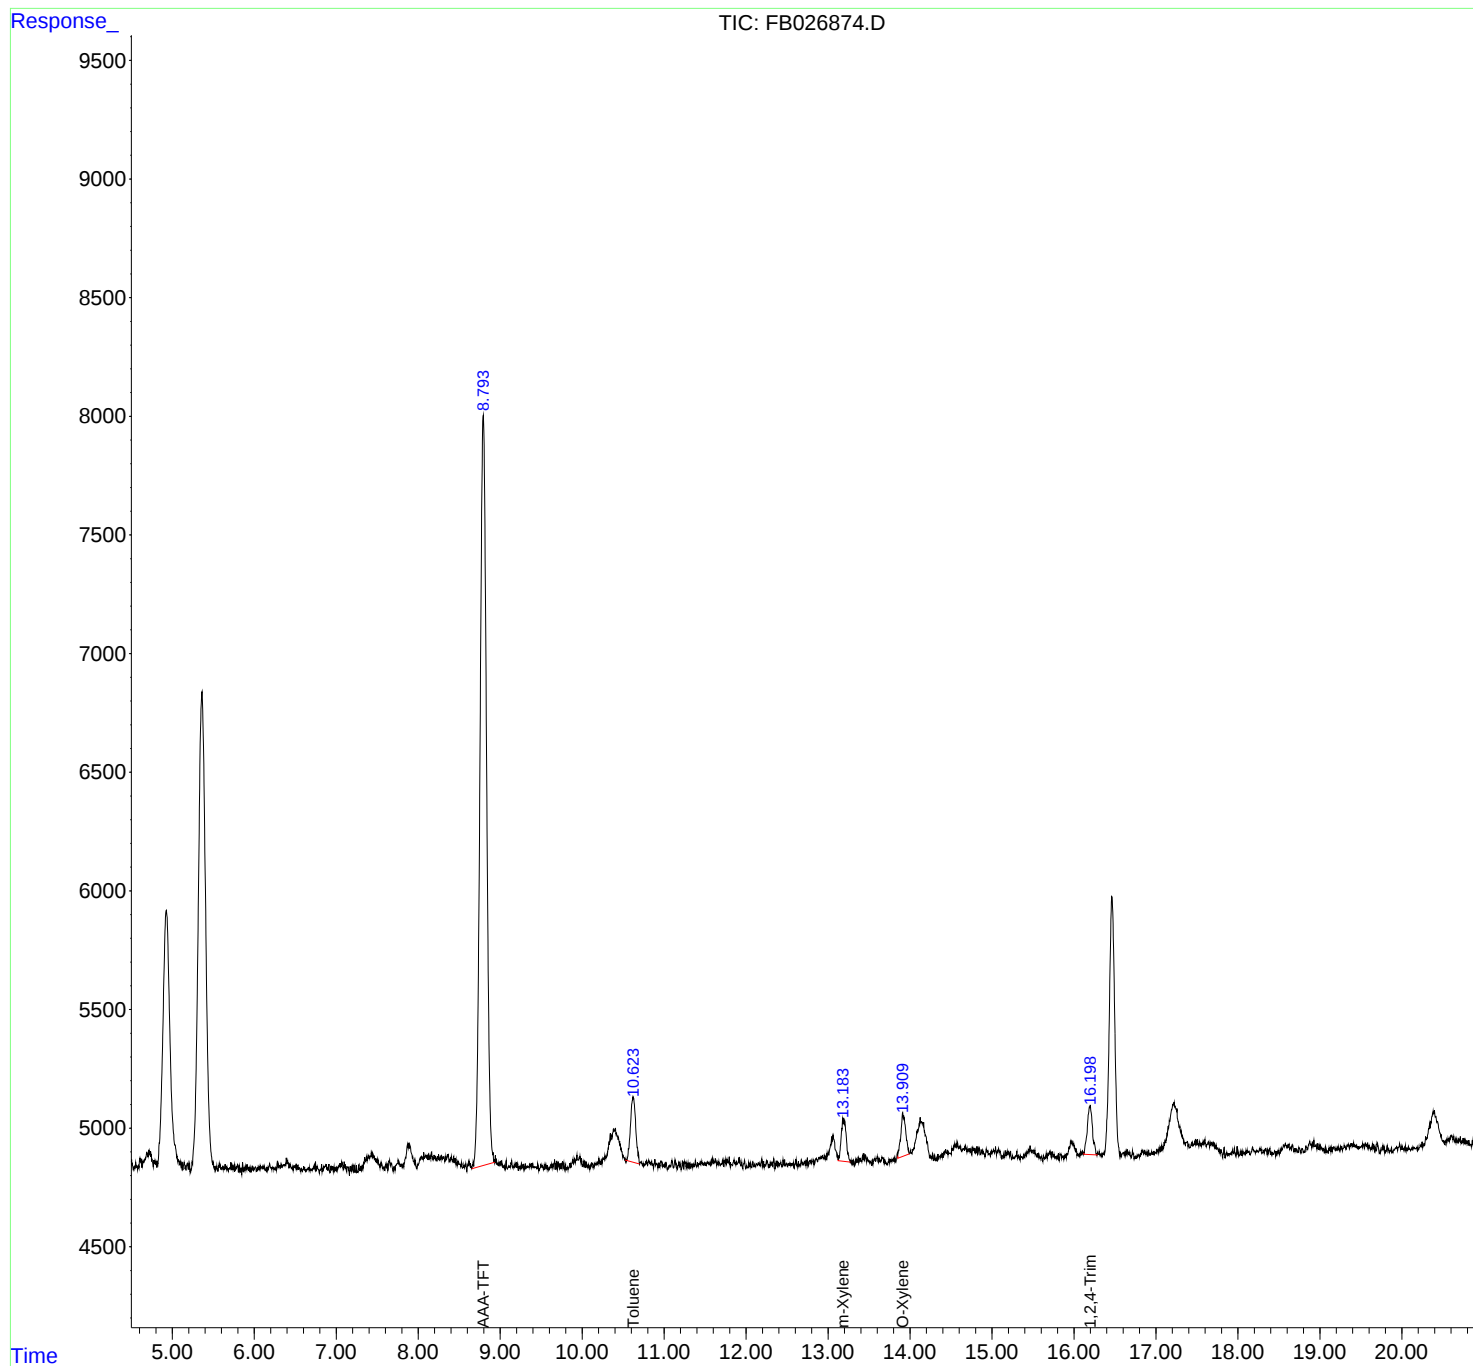


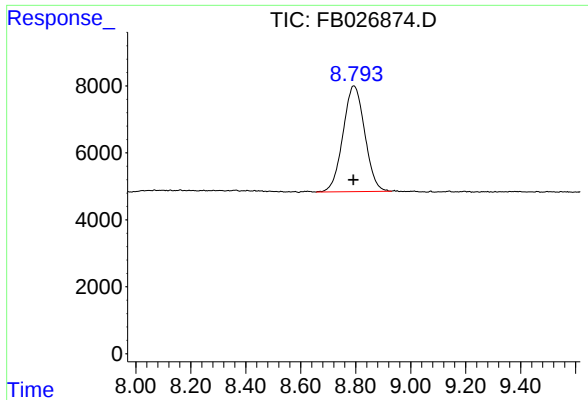

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 173616
Conc: 16.55 ng/ml

Instrument :
FID_B
ClientSampleId :

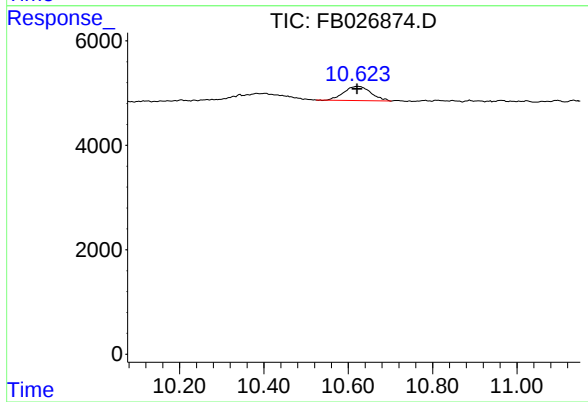


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.004 min
Response: 12135
Conc: 0.55 ng/ml

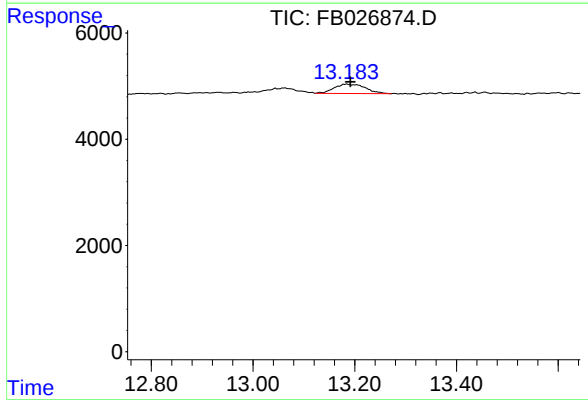


#8 m-Xylene

R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 7561
Conc: 0.38 ng/ml

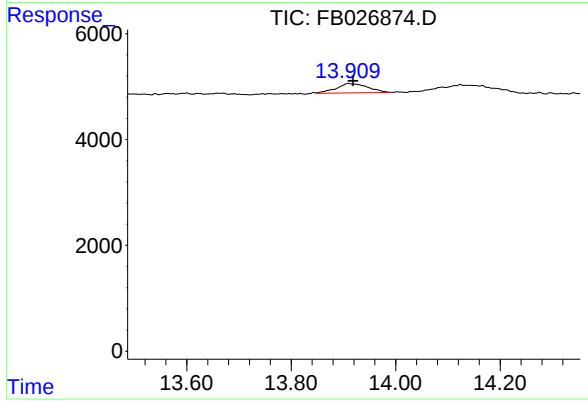

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: -0.008 min
Response: 7461
Conc: 0.37 ng/ml

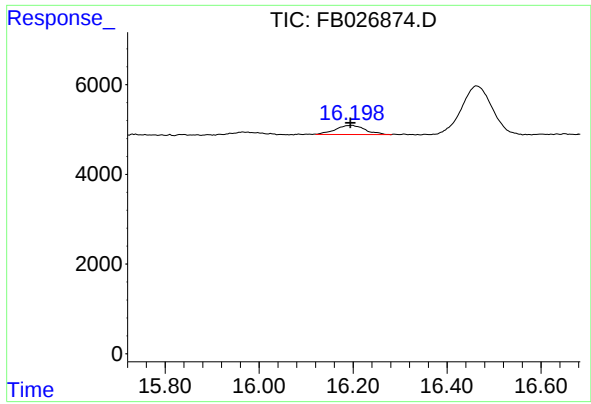

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: 0.005 min
Response: 9017
Conc: 0.45 ng/ml

Instrument :

FID_B

ClientSampleId :