

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
 Data File : FB026883.D
 Signal(s) : FID2B.CH
 Acq On : 8 Apr 2022 17:05
 Operator : AJ/MA
 Sample : N2254-01 50X
 Misc : 5.08G/5.00 ML DI MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 08 18:41:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.796	254574	24.260 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.693	22469	1.187 ng/ml
2) t 2,2,4-Trimethylpentane	7.452	85080	4.105 ng/ml
3) t n-Heptane	7.812	98192	4.961 ng/ml
6) t Toluene	10.618	2001	0.091 ng/ml
7) t Ethylbenzene	13.023	325870	16.214 ng/ml
9) t O-Xylene	13.934	68768	3.447 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
Data File : FB026883.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2022 17:05
Operator : AJ/MA
Sample : N2254-01 50X
Misc : 5.08G/5.00 ML DI MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 08 18:41:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

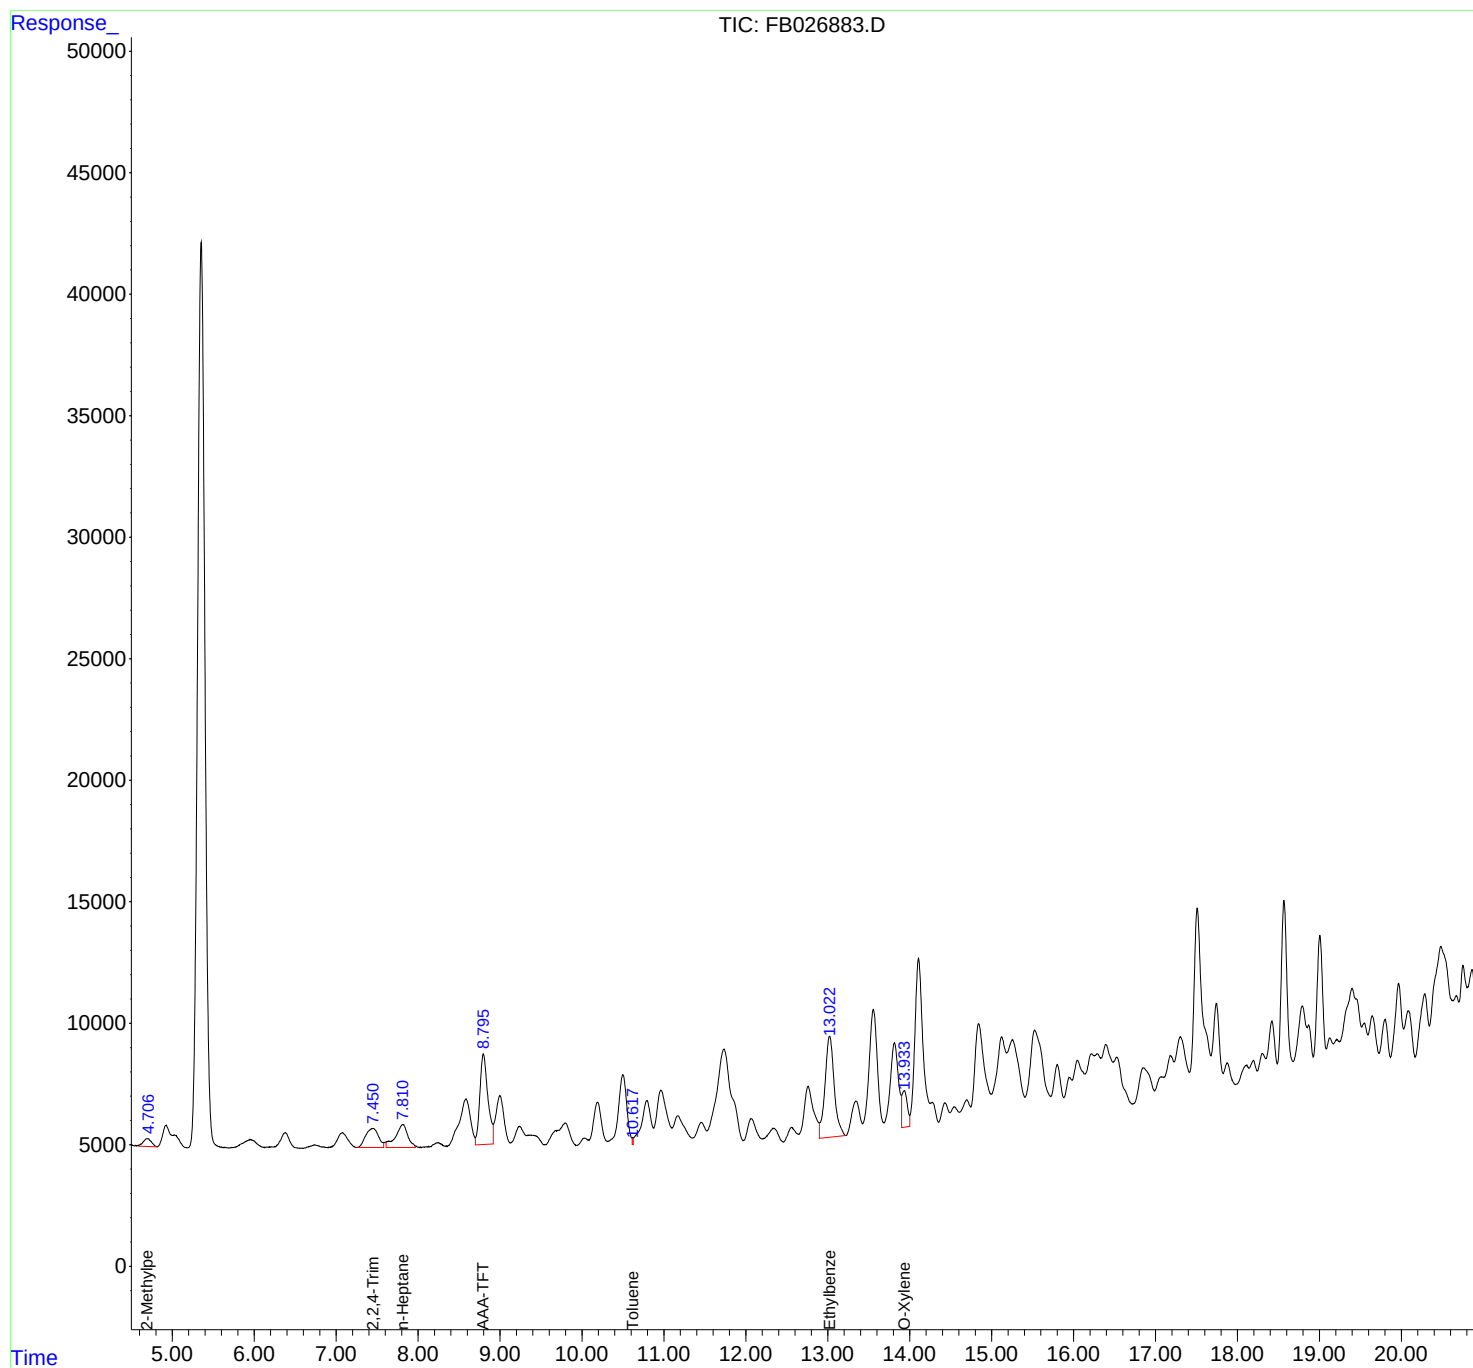


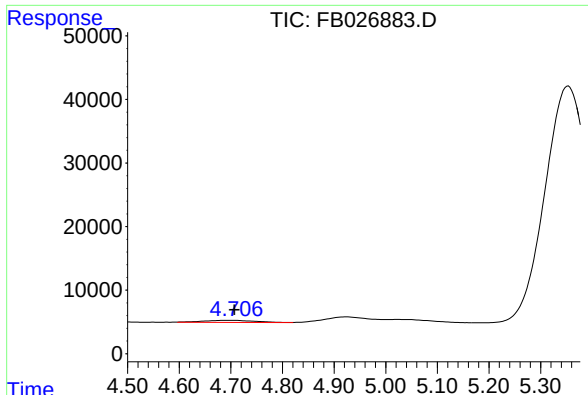

#1 2-Methylpentane


R.T.: 4.693 min
 Delta R.T.: -0.014 min
 Response: 22469
 Conc: 1.19 ng/ml

Instrument :
 FID_B
 ClientSampleId :

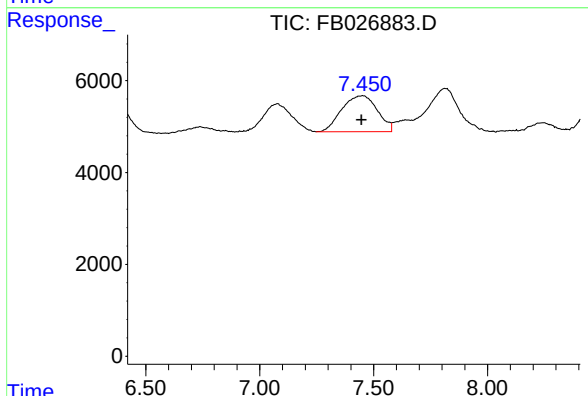


#2 2,2,4-Trimethylpentane

R.T.: 7.452 min
 Delta R.T.: 0.005 min
 Response: 85080
 Conc: 4.10 ng/ml

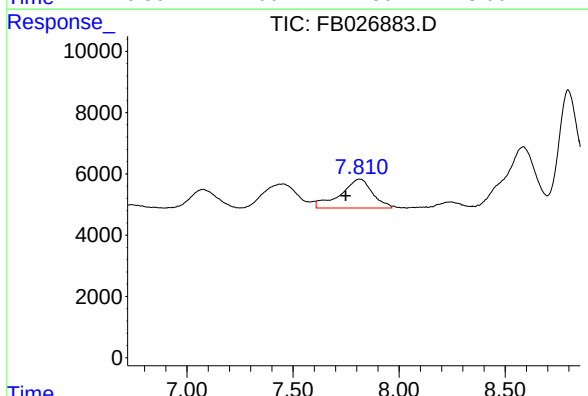


#3 n-Heptane

R.T.: 7.812 min
 Delta R.T.: 0.063 min
 Response: 98192
 Conc: 4.96 ng/ml

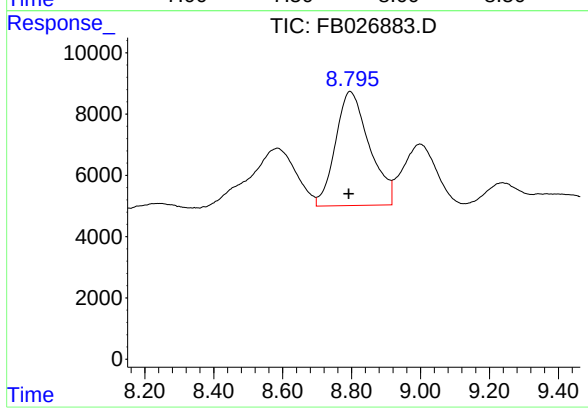

#5 AAA-TFT


R.T.: 8.796 min
 Delta R.T.: 0.004 min
 Response: 254574
 Conc: 24.26 ng/ml

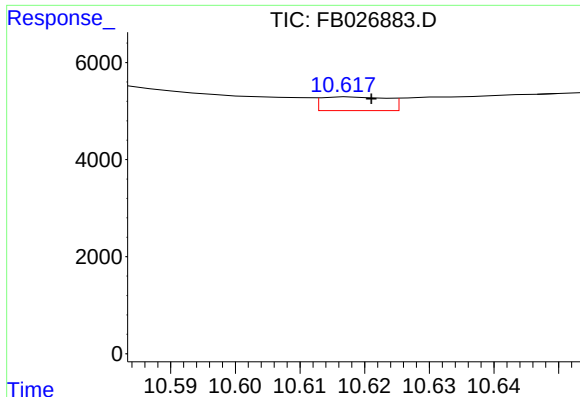

#6 Toluene


R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 2001
Conc: 0.09 ng/ml

Instrument :
FID_B
ClientSampleId :

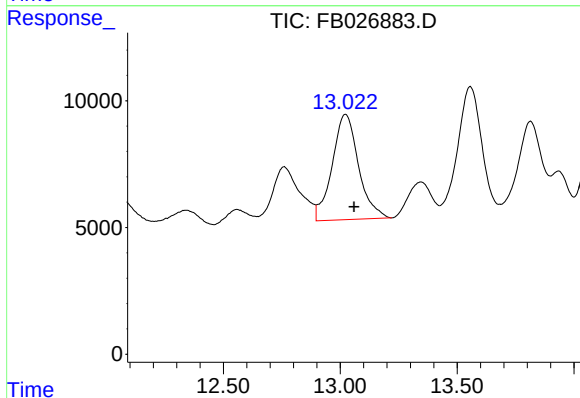

#7 Ethylbenzene

R.T.: 13.023 min
Delta R.T.: -0.036 min
Response: 325870
Conc: 16.21 ng/ml

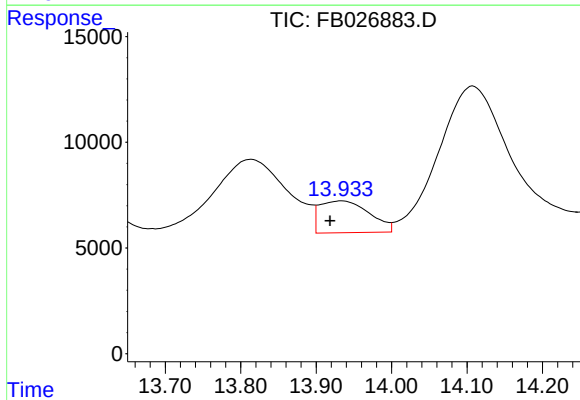

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.016 min
Response: 68768
Conc: 3.45 ng/ml