

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040822\
 Data File : PS018948.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Apr 2022 14:49
 Operator : AJ\MA
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 08 23:06:49 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 31 16:06:48 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	6.805	2266.1E6	500.4E6	776.206	700.940
Target Compounds							
1) T	Dalapon	3.029	2.531	2690.7E6	580.2E6	588.196	625.546
2) T	3,5-DICHL...	6.435	5.979	3030.1E6	720.6E6	755.328	653.549
3) T	4-Nitroph...	7.060	6.420	642.2E6	259.7E6	562.556	611.457
5) T	DICAMBA	7.416	6.971	8753.3E6	2118.6E6	696.191	665.498
6) T	MCPD	7.588	7.069	696.2E6	167.7E6	68.238	65.558
7) T	MCPA	7.737	7.282	953.6E6	231.6E6	66.992	64.646
8) T	DICHLORPROP	8.112	7.594	2212.1E6	541.1E6	663.589	657.938
9) T	2,4-D	8.341	7.885	2606.0E6	618.8E6	652.118	669.546
10) T	Pentachlo...	8.650	8.314	29515.0E6	7077.7E6	659.677	672.581
11) T	2,4,5-TP ...	9.203	8.675	12340.6E6	3113.9E6	603.112	681.181
12) T	2,4,5-T	9.488	9.054	12076.6E6	2876.2E6	589.064	690.700
13) T	2,4-DB	10.042	9.560	2051.3E6	388.6E6	604.218	682.249
14) T	DINOSEB	11.201	9.887	8395.4E6	2118.7E6	514.227	656.988 #
15) T	Picloram	11.022	10.869	14973.0E6	3717.6E6	535.170	657.491
16) T	DCPA	11.469	10.818	13675.6E6	3723.1E6	543.333	683.057 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS040822\
Data File : PS018948.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Apr 2022 14:49
Operator : AJ\MA
Sample : HSTDCCC750
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 08 23:06:49 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS033122.M
Quant Title : 8080.M
QLast Update : Thu Mar 31 16:06:48 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

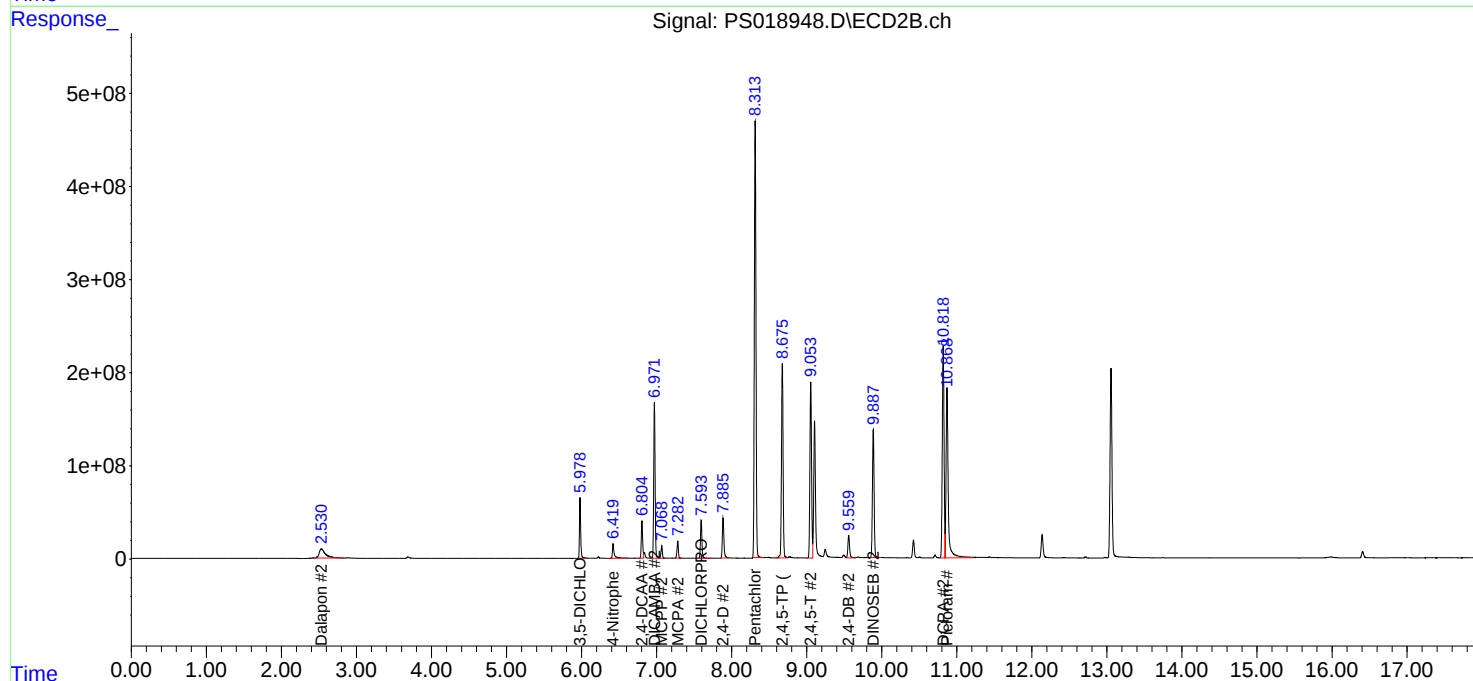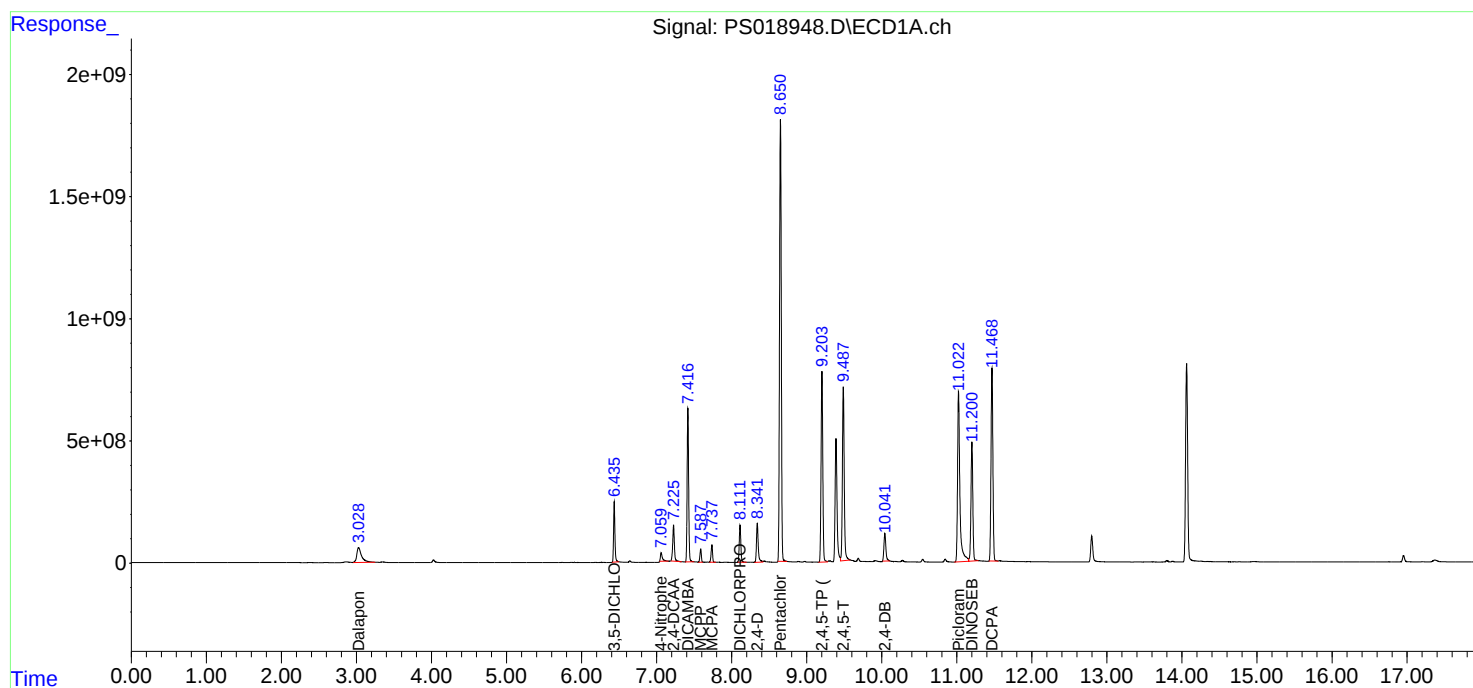


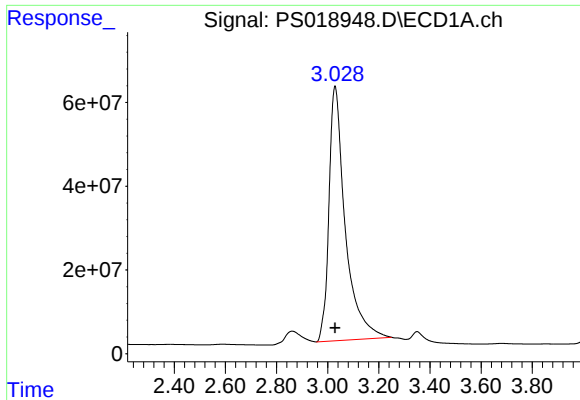

#1 Dalapon


R.T.: 3.029 min
Delta R.T.: 0.000 min
Response: 2690679966
Conc: 588.20 ng/ml

Instrument :
FID_B
ClientSampleId :

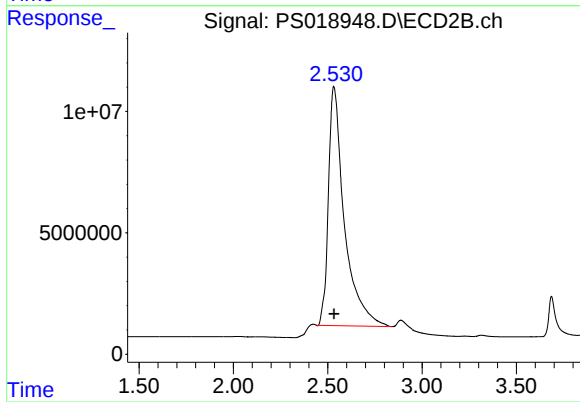


#1 Dalapon

R.T.: 2.531 min
Delta R.T.: -0.004 min
Response: 580208844
Conc: 625.55 ng/ml

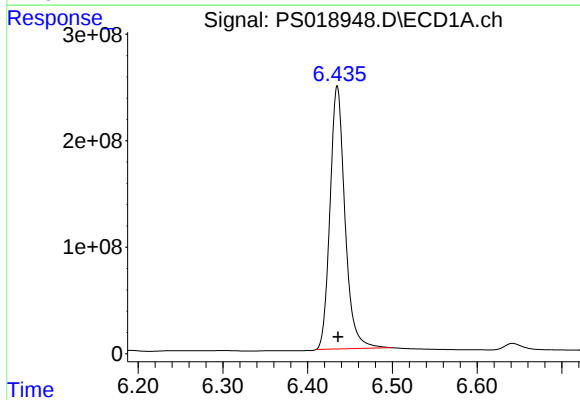


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.435 min
Delta R.T.: 0.000 min
Response: 3030108616
Conc: 755.33 ng/ml

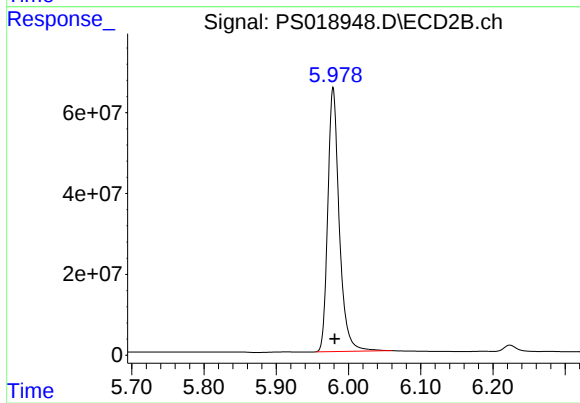

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.979 min
Delta R.T.: -0.002 min
Response: 720618204
Conc: 653.55 ng/ml

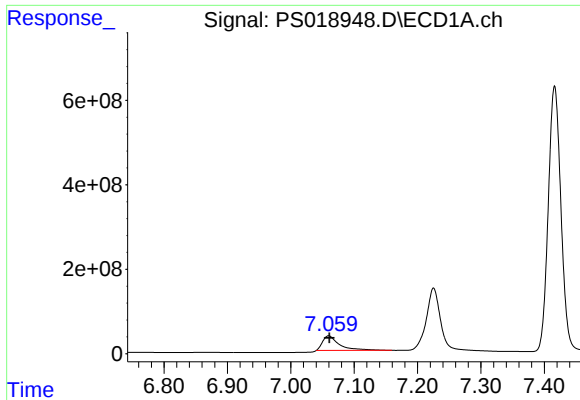

#3 4-Nitrophenol


R.T.: 7.060 min
Delta R.T.: -0.001 min
Response: 642159554
Conc: 562.56 ng/ml

Instrument : FID_B
ClientSampleId :

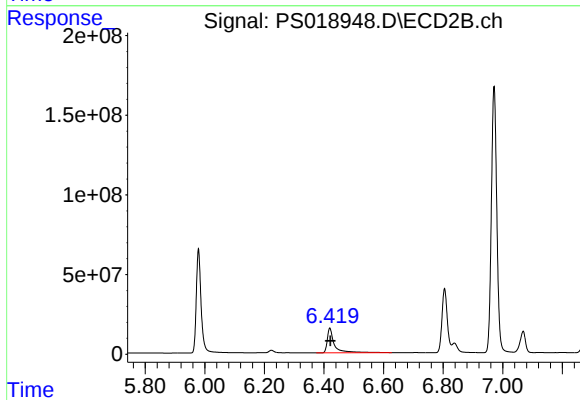


#3 4-Nitrophenol

R.T.: 6.420 min
Delta R.T.: -0.002 min
Response: 259728586
Conc: 611.46 ng/ml

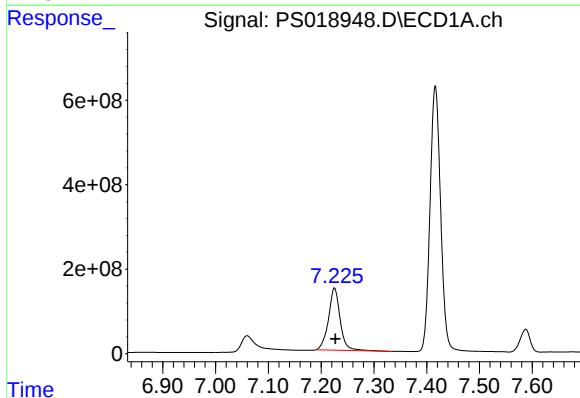


#4 2,4-DCAA

R.T.: 7.225 min
Delta R.T.: -0.002 min
Response: 2266102846
Conc: 776.21 ng/ml

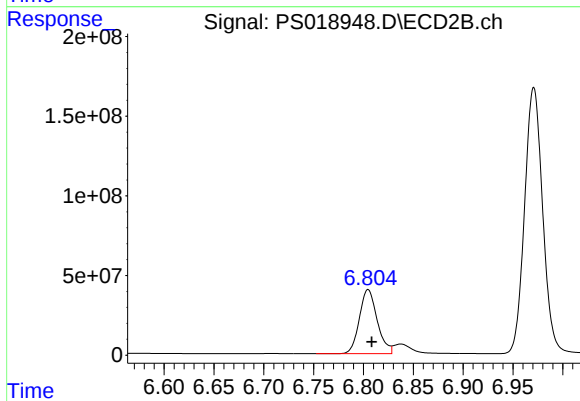

#4 2,4-DCAA


R.T.: 6.805 min
Delta R.T.: -0.004 min
Response: 500431266
Conc: 700.94 ng/ml

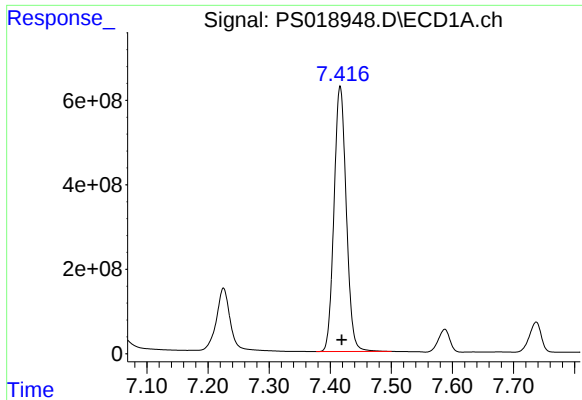

#5 DICAMBA


R.T.: 7.416 min
Delta R.T.: -0.002 min
Response: 8753250299
Conc: 696.19 ng/ml

Instrument :
FID_B
ClientSampleId :

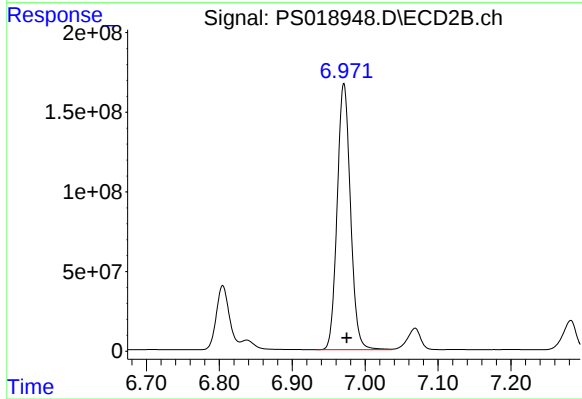


#5 DICAMBA

R.T.: 6.971 min
Delta R.T.: -0.004 min
Response: 2118552847
Conc: 665.50 ng/ml

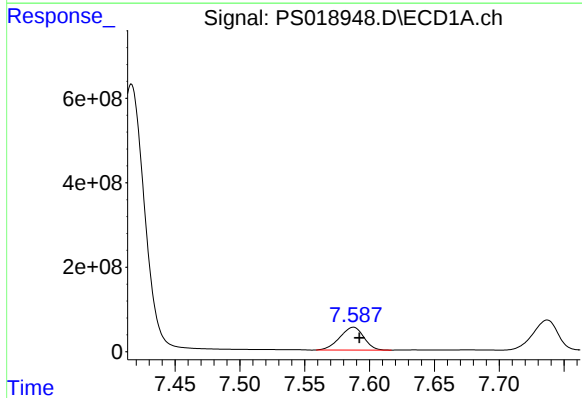


#6 MCP

R.T.: 7.588 min
Delta R.T.: -0.005 min
Response: 696205214
Conc: 68.24 ug/ml

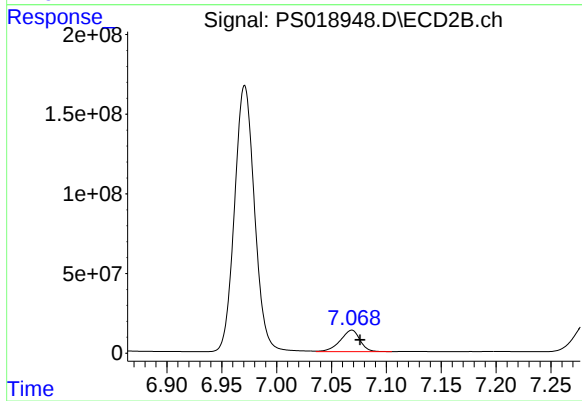

#6 MCP


R.T.: 7.069 min
Delta R.T.: -0.007 min
Response: 167729687
Conc: 65.56 ug/ml

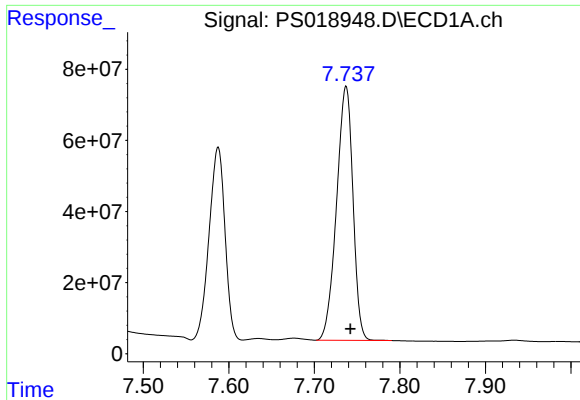

#7 MCPA


R.T.: 7.737 min
Delta R.T.: -0.005 min
Response: 953565488
Conc: 66.99 ug/ml

Instrument :
FID_B
ClientSampleId :

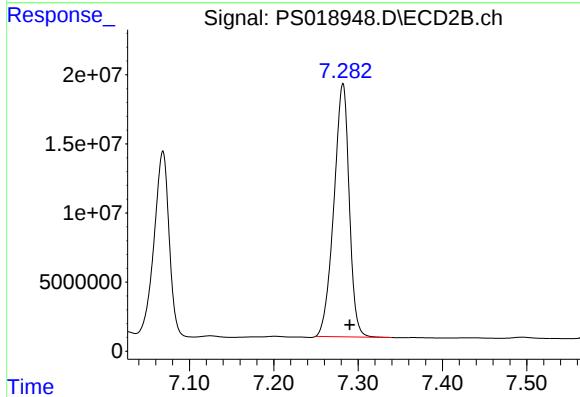


#7 MCPA

R.T.: 7.282 min
Delta R.T.: -0.008 min
Response: 231609860
Conc: 64.65 ug/ml

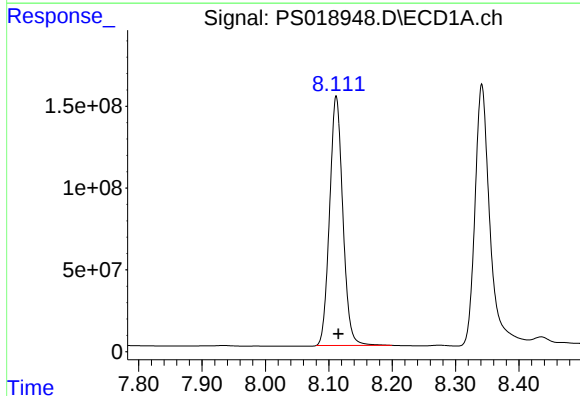


#8 DICHLORPROP

R.T.: 8.112 min
Delta R.T.: -0.003 min
Response: 2212076531
Conc: 663.59 ng/ml

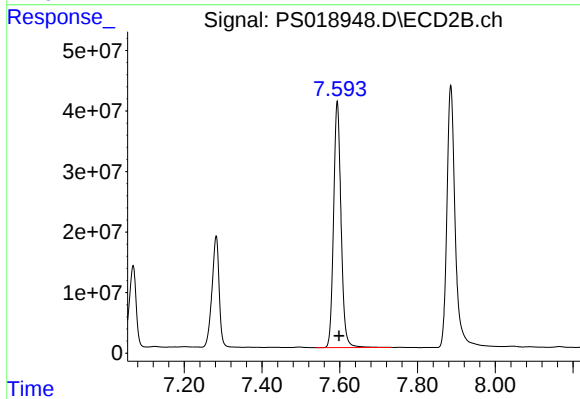

#8 DICHLORPROP


R.T.: 7.594 min
Delta R.T.: -0.005 min
Response: 541059490
Conc: 657.94 ng/ml

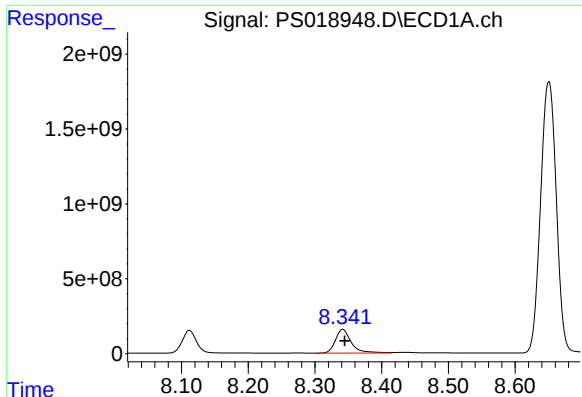

#9 2,4-D


R.T.: 8.341 min
Delta R.T.: -0.003 min
Response: 2606014611
Conc: 652.12 ng/ml

Instrument :
FID_B
ClientSampleId :

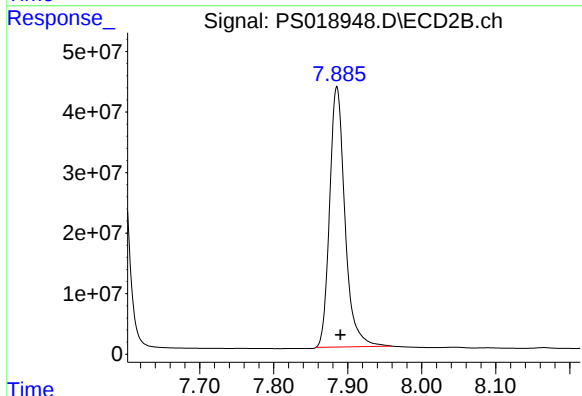


#9 2,4-D

R.T.: 7.885 min
Delta R.T.: -0.004 min
Response: 618814825
Conc: 669.55 ng/ml

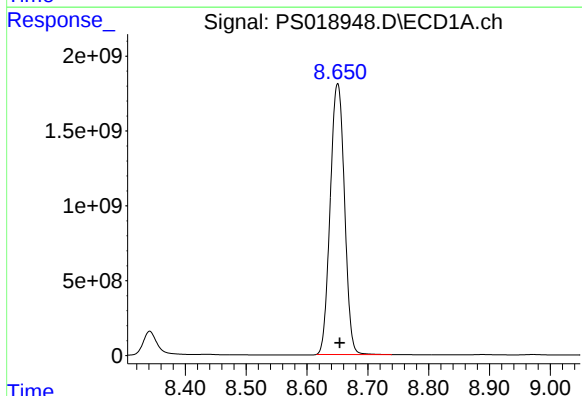


#10 Pentachlorophenol

R.T.: 8.650 min
Delta R.T.: -0.003 min
Response: 29514997462
Conc: 659.68 ng/ml

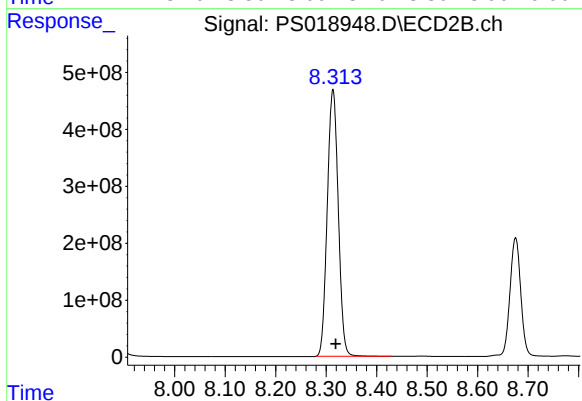

#10 Pentachlorophenol


R.T.: 8.314 min
Delta R.T.: -0.005 min
Response: 7077671058
Conc: 672.58 ng/ml

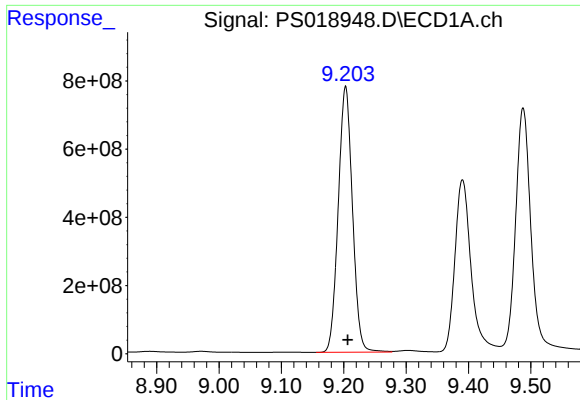

#11 2,4,5-TP (SILVEX)


R.T.: 9.203 min
Delta R.T.: -0.003 min
Response: 12340593832
Conc: 603.11 ng/ml

Instrument : FID_B
ClientSampleId :

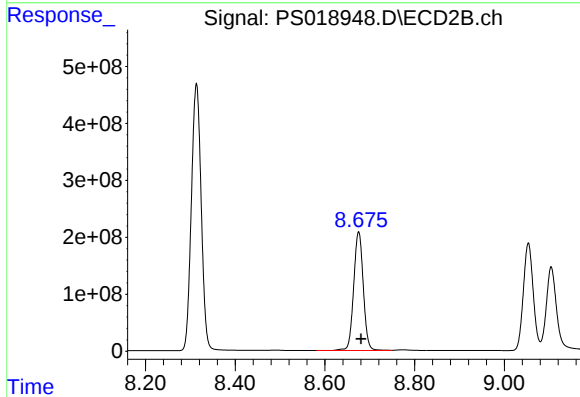


#11 2,4,5-TP (SILVEX)

R.T.: 8.675 min
Delta R.T.: -0.005 min
Response: 3113885929
Conc: 681.18 ng/ml

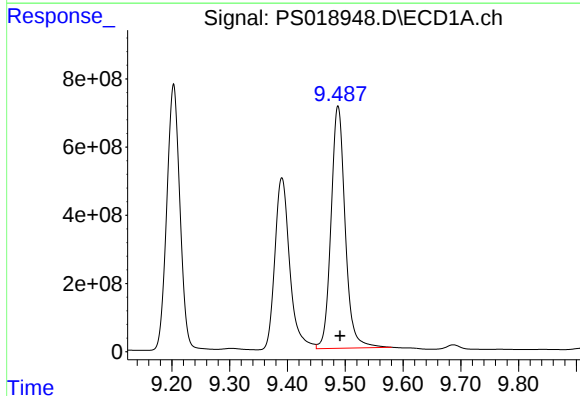


#12 2,4,5-T

R.T.: 9.488 min
Delta R.T.: -0.004 min
Response: 12076591787
Conc: 589.06 ng/ml

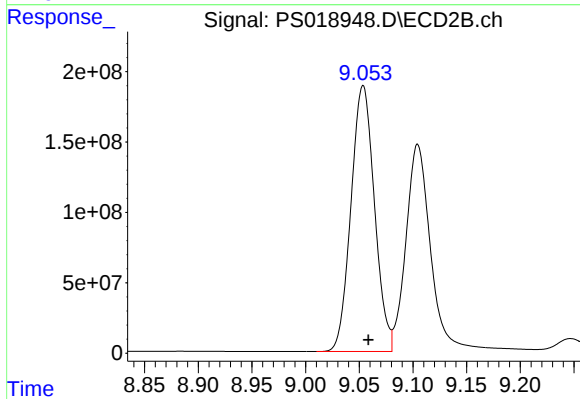

#12 2,4,5-T


R.T.: 9.054 min
Delta R.T.: -0.005 min
Response: 2876224641
Conc: 690.70 ng/ml

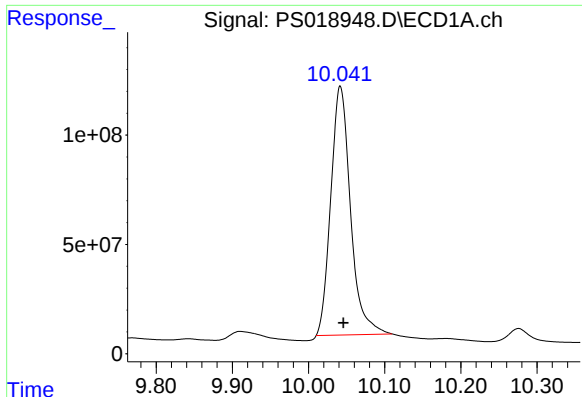

#13 2,4-DB


R.T.: 10.042 min
Delta R.T.: -0.004 min
Response: 2051254610
Conc: 604.22 ng/ml

Instrument :
FID_B
ClientSampleId :

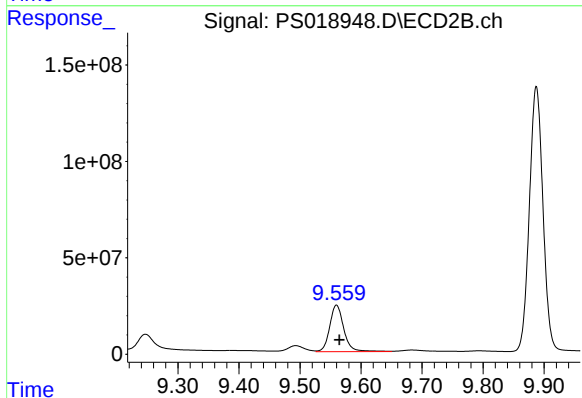


#13 2,4-DB

R.T.: 9.560 min
Delta R.T.: -0.005 min
Response: 388591460
Conc: 682.25 ng/ml

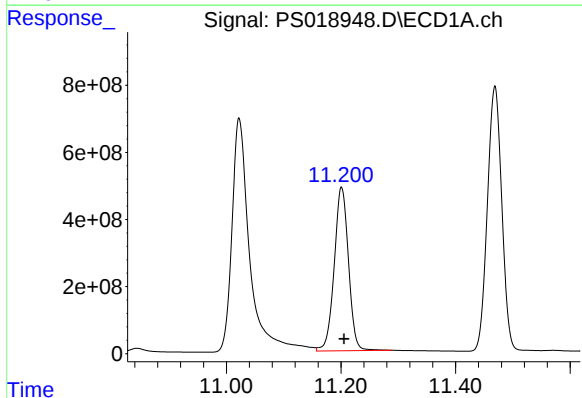


#14 DINOSEB

R.T.: 11.201 min
Delta R.T.: -0.005 min
Response: 8395439427
Conc: 514.23 ng/ml

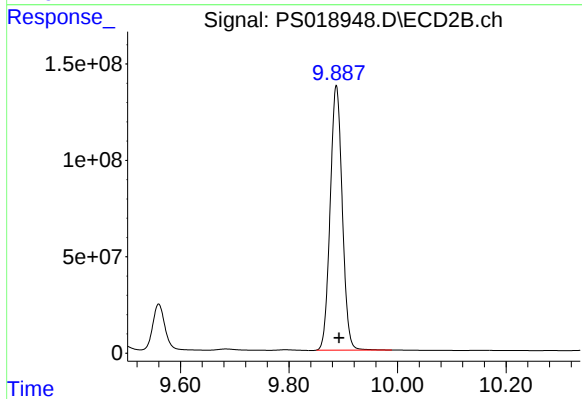

#14 DINOSEB


R.T.: 9.887 min
Delta R.T.: -0.005 min
Response: 2118665223
Conc: 656.99 ng/ml

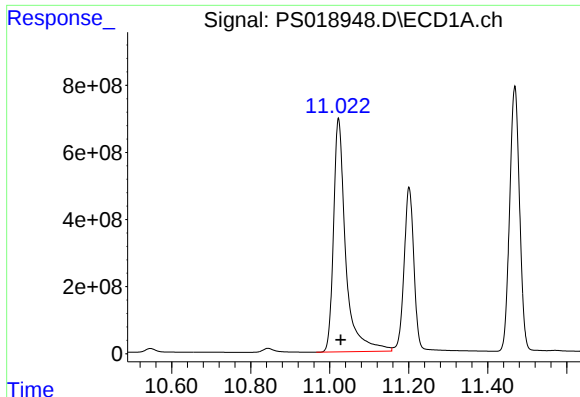

#15 Picloram


R.T.: 11.022 min
Delta R.T.: -0.006 min
Response: 14973022858
Conc: 535.17 ng/ml

Instrument :
FID_B
ClientSampleId :

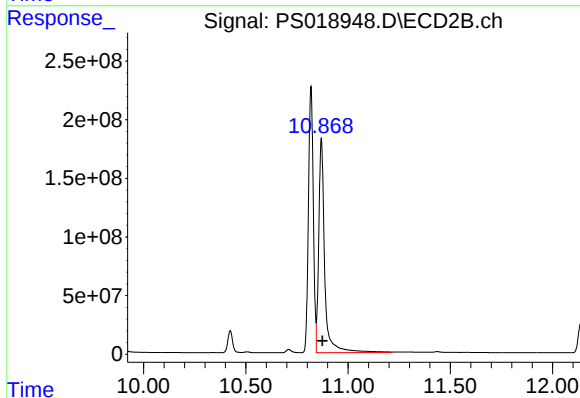


#15 Picloram

R.T.: 10.869 min
Delta R.T.: -0.006 min
Response: 3717596148
Conc: 657.49 ng/ml

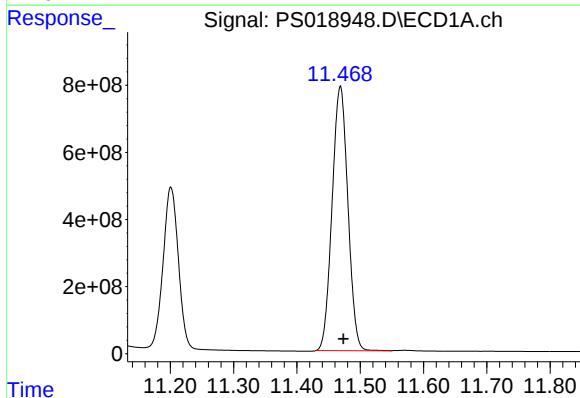

#16 DCPA

R.T.: 11.469 min
Delta R.T.: -0.005 min
Response: 13675643248
Conc: 543.33 ng/ml

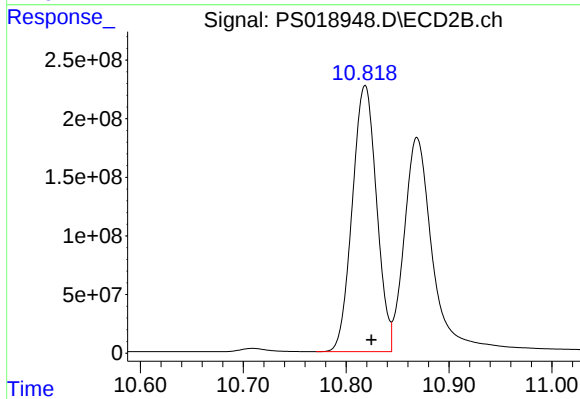

#16 DCPA

R.T.: 10.818 min
Delta R.T.: -0.006 min
Response: 3723083412
Conc: 683.06 ng/ml