

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
 Data File : FB026876.D
 Signal(s) : FID2B.CH
 Acq On : 8 Apr 2022 11:24
 Operator : AJ/MA
 Sample : BSF0408S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0408S1

Integration File: SAMPLE.e
 Quant Time: Apr 08 14:16:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	305309	29.095 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	327599	17.303 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	425479	20.527 ng/ml
3) t n-Heptane	7.751	108376	5.475 ng/ml
4) t Benzene	7.889	168537	7.304 ng/ml
6) t Toluene	10.621	496440	22.676 ng/ml
7) t Ethylbenzene	13.058	163314	8.126 ng/ml
8) t m-Xylene	13.190	325643	16.159 ng/ml
9) t O-Xylene	13.918	327753	16.429 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	351252	17.629 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
Data File : FB026876.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2022 11:24
Operator : AJ/MA
Sample : BSF0408S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0408S1

Integration File: SAMPLE.e
Quant Time: Apr 08 14:16:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

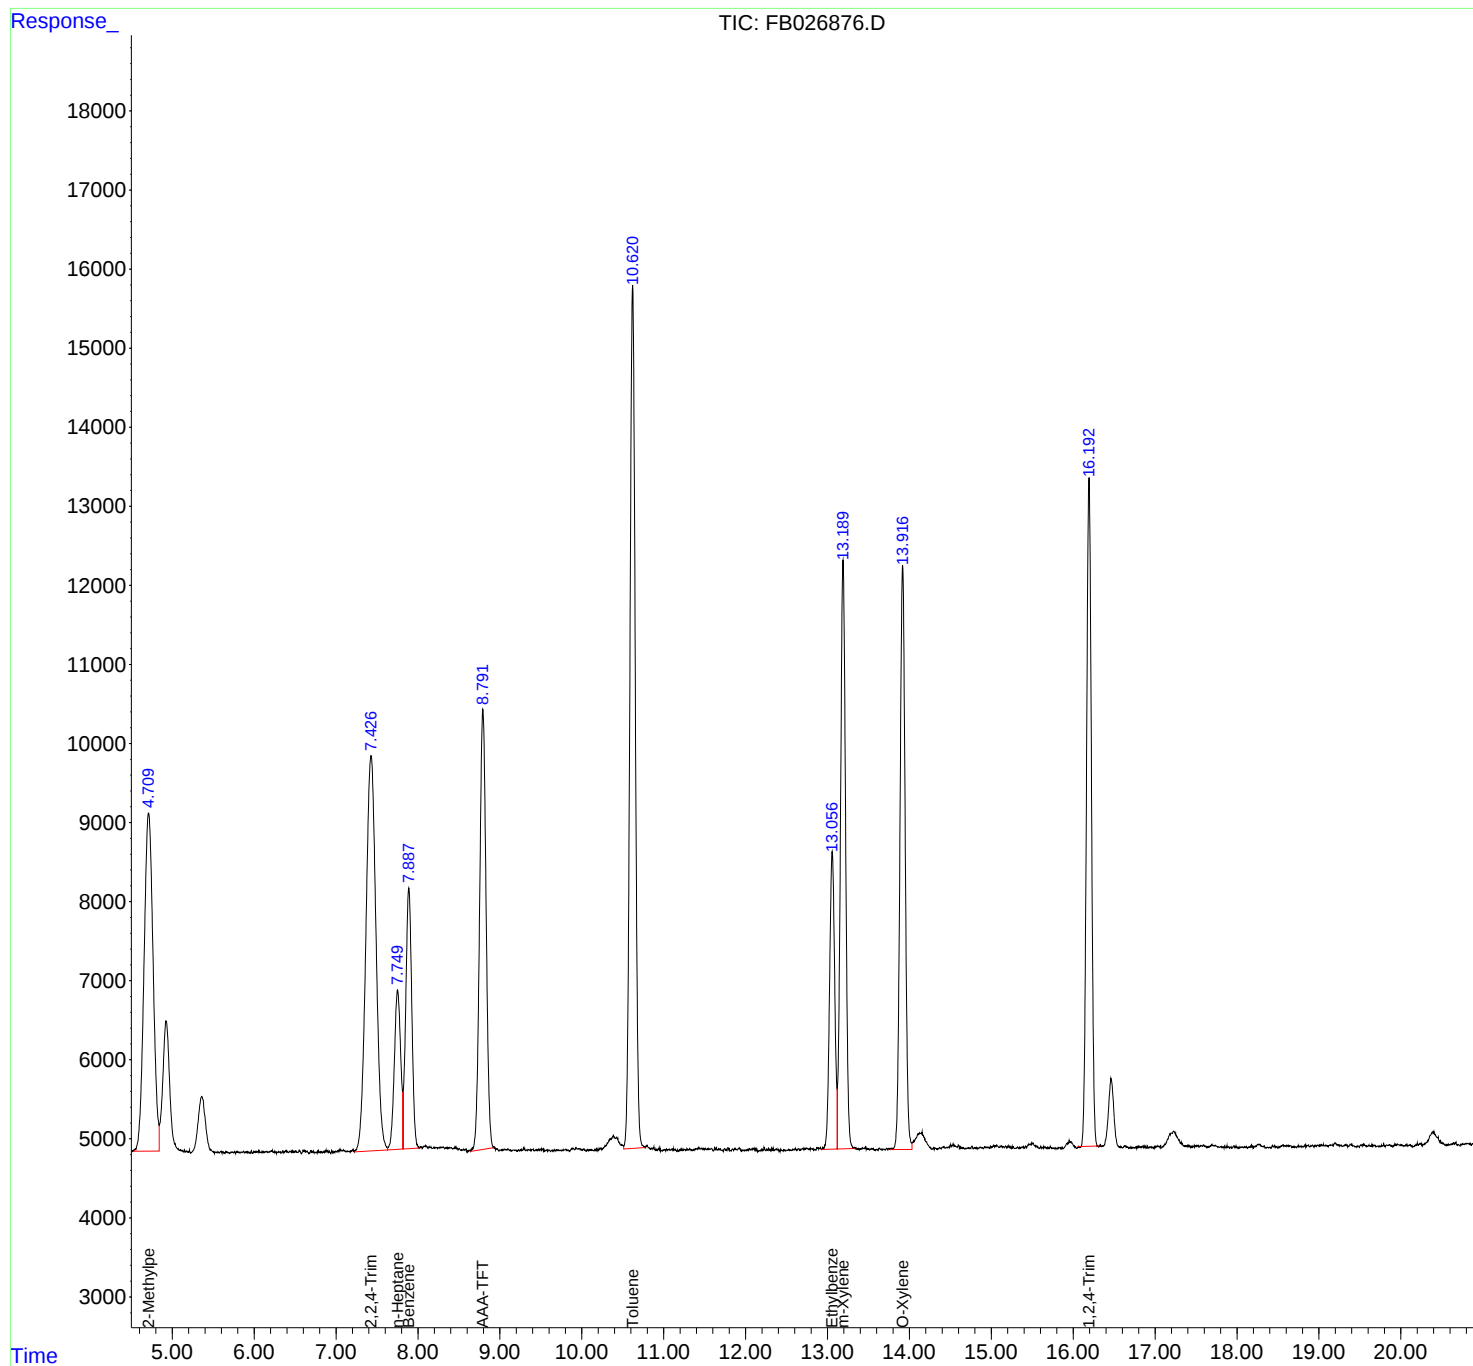


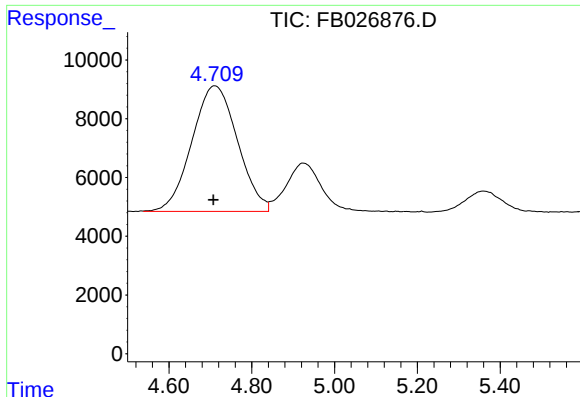

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.004 min
Response: 327599
Conc: 17.30 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

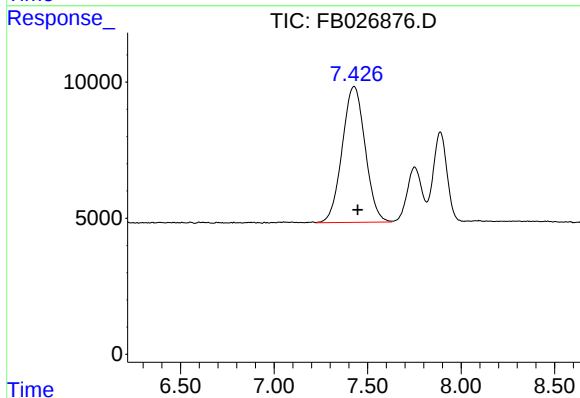


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.019 min
Response: 425479
Conc: 20.53 ng/ml

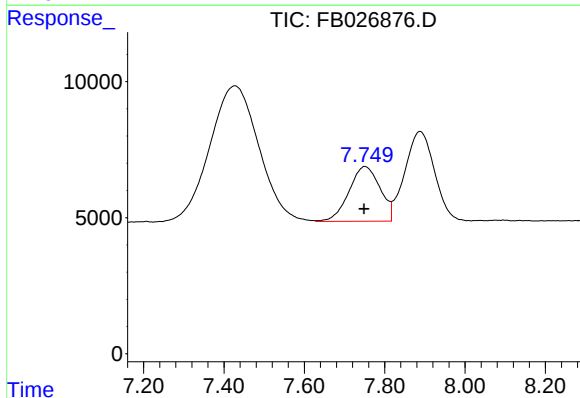


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.002 min
Response: 108376
Conc: 5.48 ng/ml

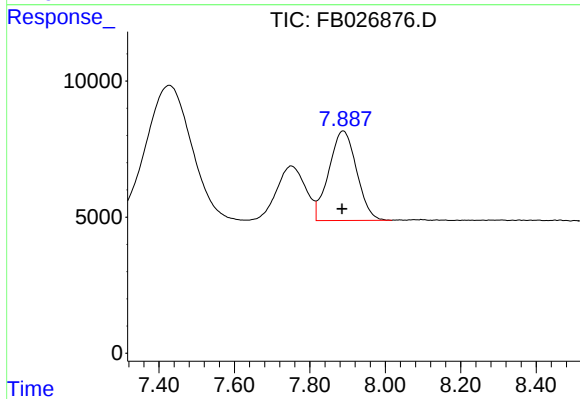

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.003 min
Response: 168537
Conc: 7.30 ng/ml

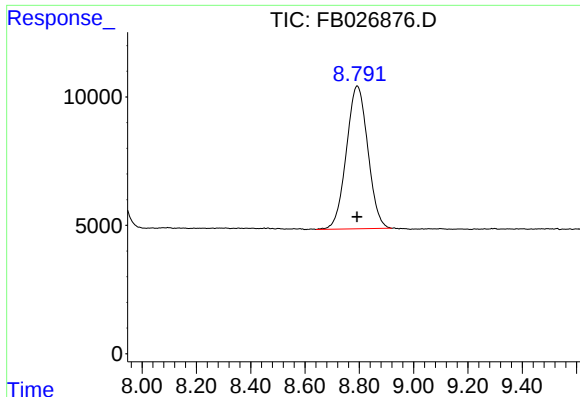

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.001 min
Response: 305309
Conc: 29.10 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

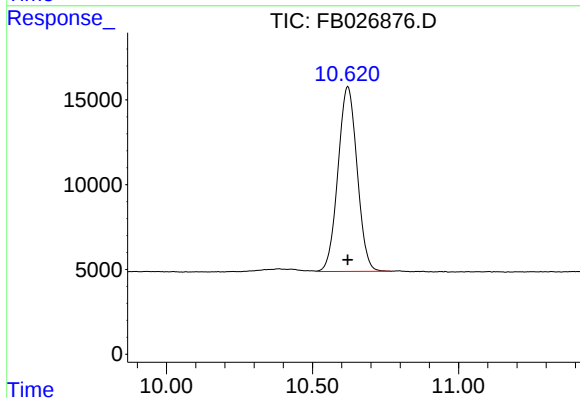


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 496440
Conc: 22.68 ng/ml

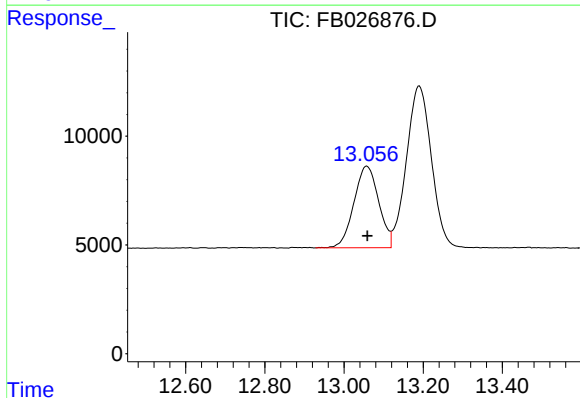


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.001 min
Response: 163314
Conc: 8.13 ng/ml

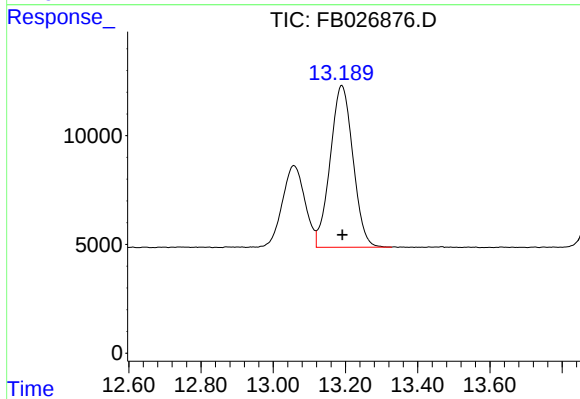

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: -0.001 min
Response: 325643
Conc: 16.16 ng/ml

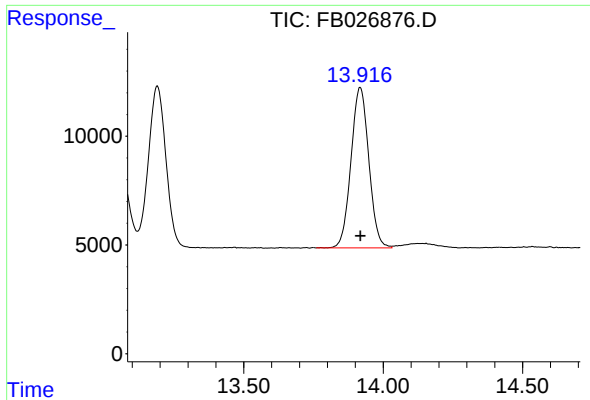

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 327753
Conc: 16.43 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

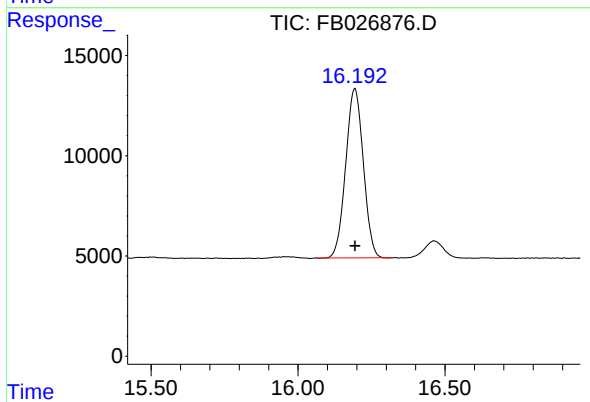

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.000 min
Response: 351252
Conc: 17.63 ng/ml