

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
 Data File : FB026893.D
 Signal(s) : FID2B.CH
 Acq On : 8 Apr 2022 23:07
 Operator : AJ/MA
 Sample : BSF0408S1
 Misc : 4.75G/5.00 ML DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0408S1

Integration File: SAMPLE.e
 Quant Time: Apr 09 00:55:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	150248	14.318 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	272504	14.393 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	308483	14.883 ng/ml
3) t n-Heptane	7.749	95291	4.814 ng/ml
4) t Benzene	7.887	133908	5.803 ng/ml
6) t Toluene	10.619	395489	18.065 ng/ml
7) t Ethylbenzene	13.056	128543	6.396 ng/ml
8) t m-Xylene	13.189	251877	12.498 ng/ml
9) t O-Xylene	13.917	240480	12.054 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	248013	12.448 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040822\
Data File : FB026893.D
Signal(s) : FID2B.CH
Acq On : 8 Apr 2022 23:07
Operator : AJ/MA
Sample : BSF0408S1
Misc : 4.75G/5.00 ML DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0408S1

Integration File: SAMPLE.e
Quant Time: Apr 09 00:55:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

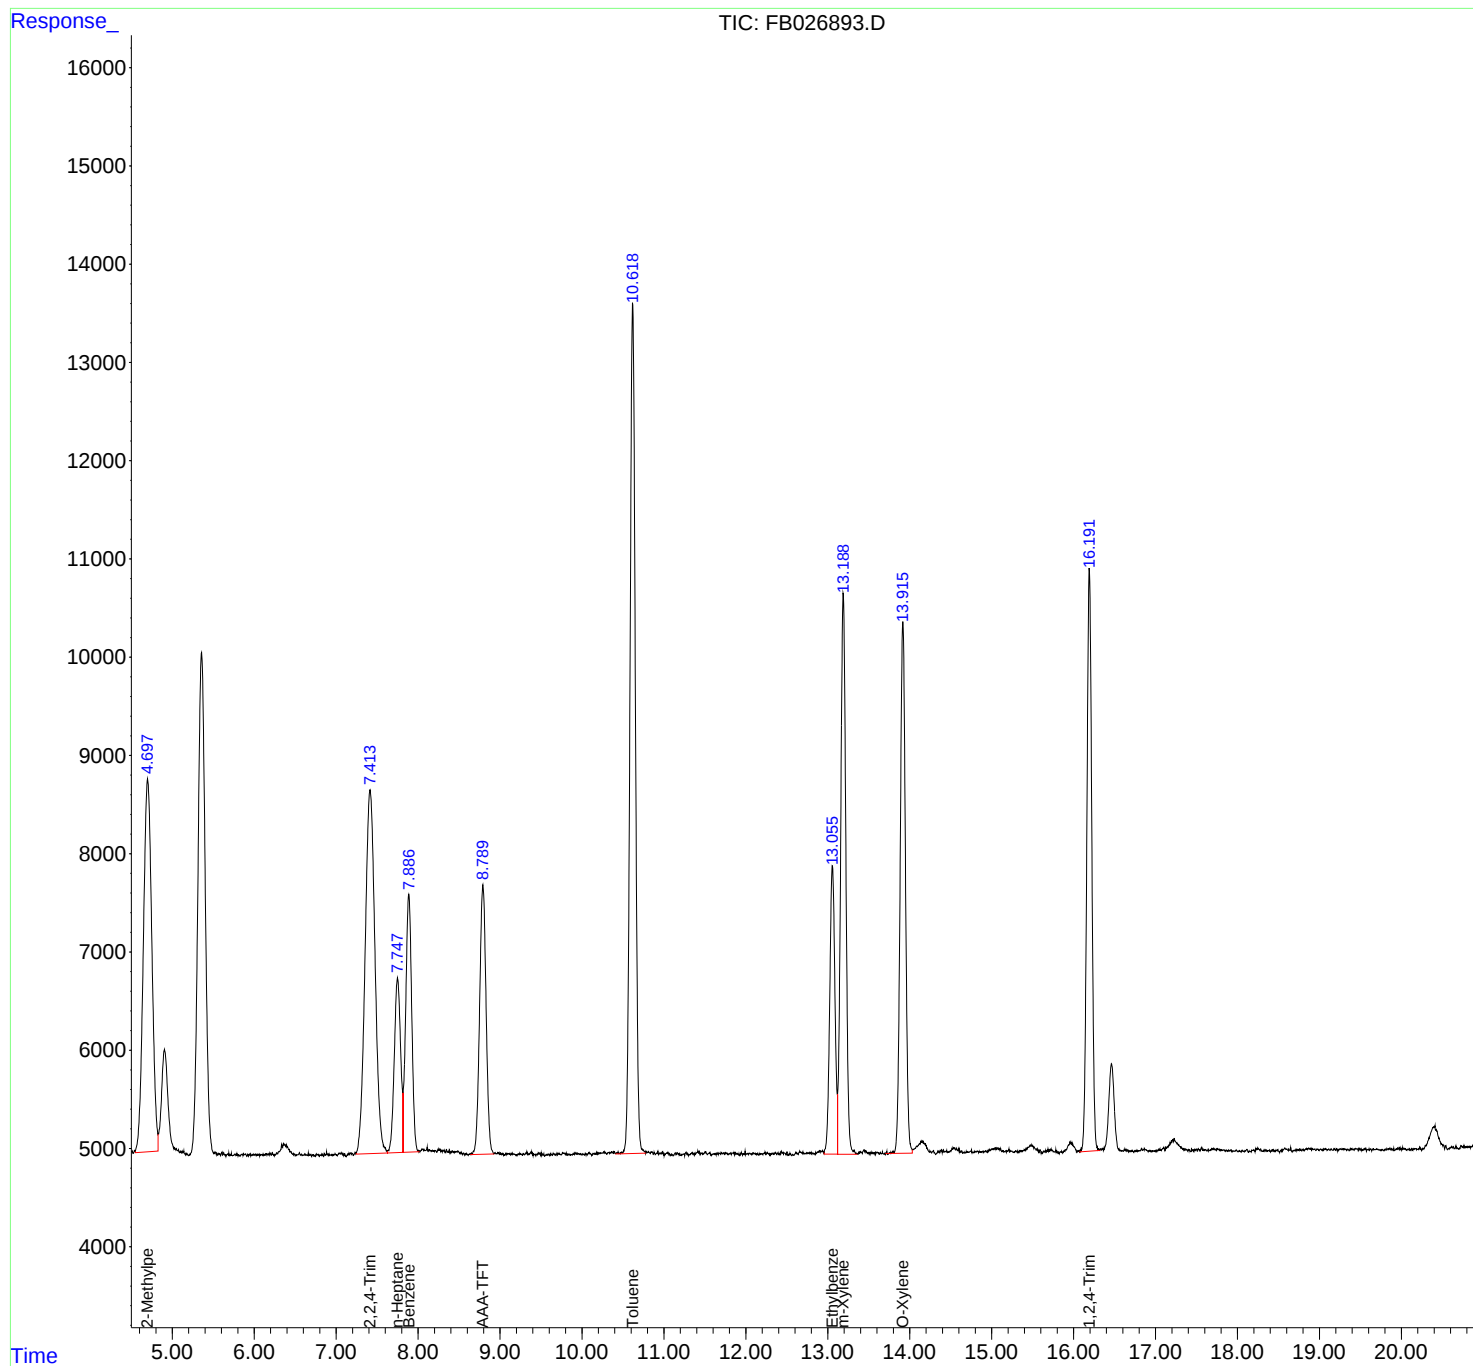


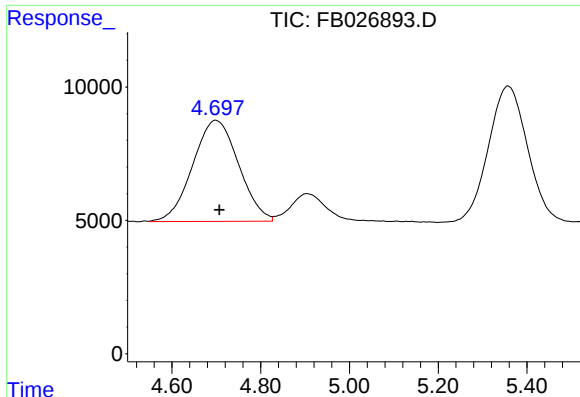

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.009 min
Response: 272504
Conc: 14.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

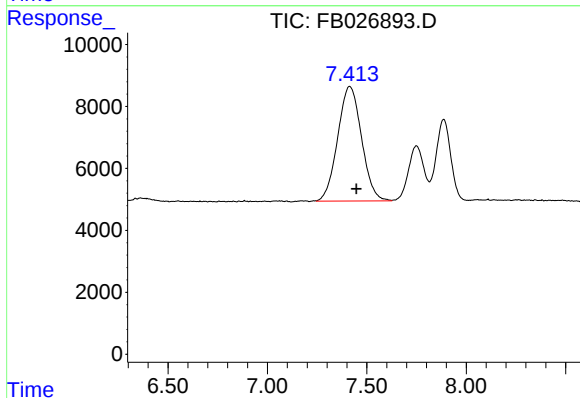


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.033 min
Response: 308483
Conc: 14.88 ng/ml

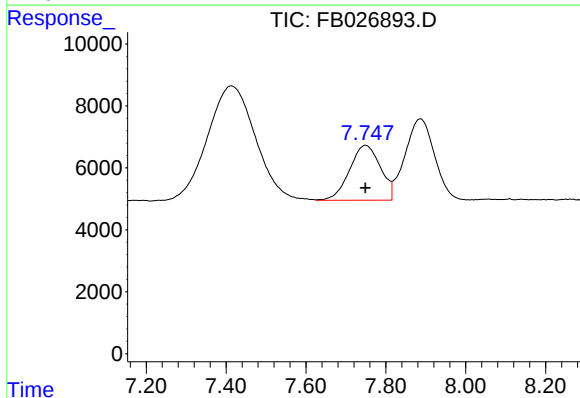


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 95291
Conc: 4.81 ng/ml

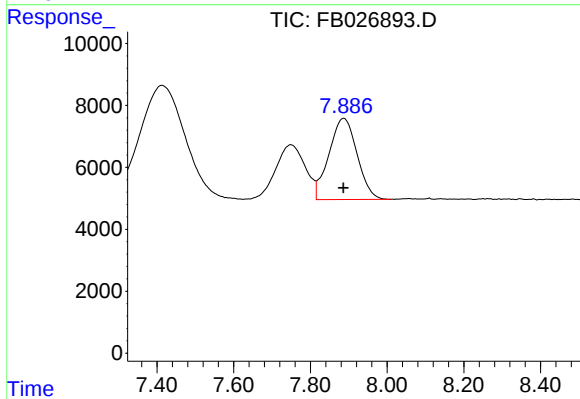

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 133908
Conc: 5.80 ng/ml

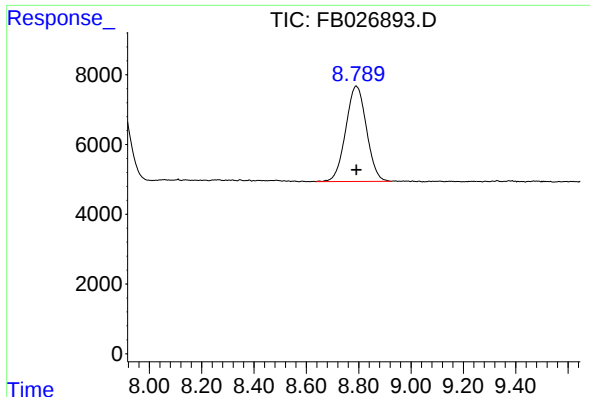

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 150248
Conc: 14.32 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

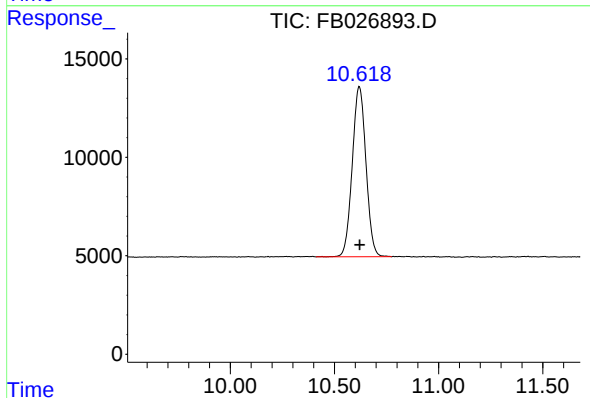


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 395489
Conc: 18.06 ng/ml

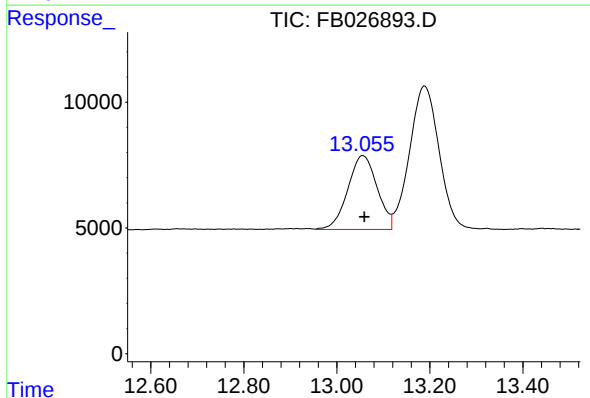


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.003 min
Response: 128543
Conc: 6.40 ng/ml

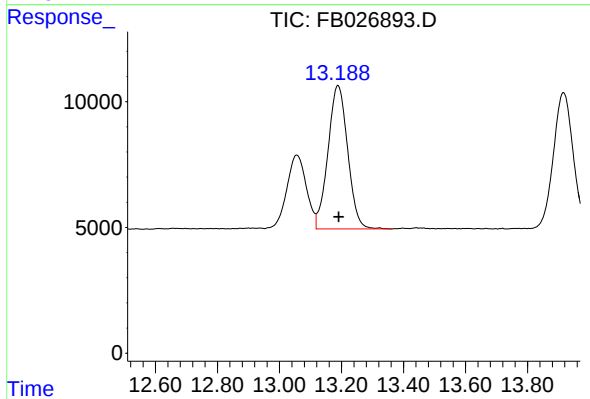

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.002 min
Response: 251877
Conc: 12.50 ng/ml

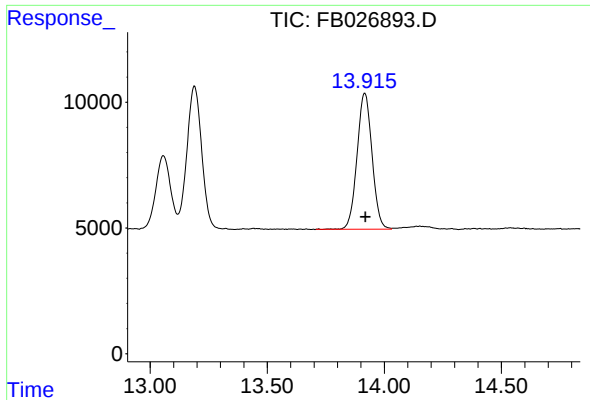

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: -0.002 min
Response: 240480
Conc: 12.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0408S1

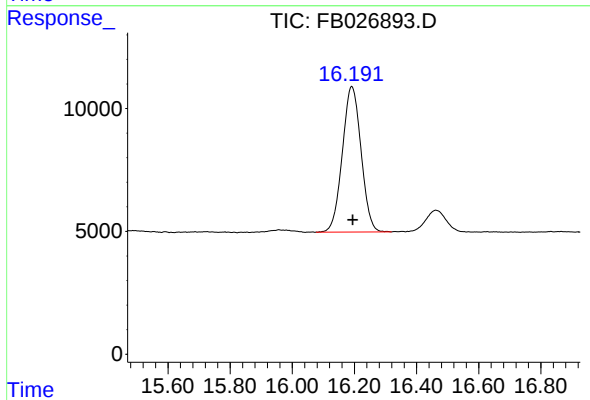

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: -0.002 min
Response: 248013
Conc: 12.45 ng/ml