

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
 Data File : FB026898.D
 Signal(s) : FID2B.CH
 Acq On : 9 Apr 2022 3:19
 Operator : AJ/MA
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 09 03:49:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 03:48:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	563816	50.854 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	1376266	73.866 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	1486892	74.984 ng/ml
3) t n-Heptane	7.751	483832	24.757 ng/ml
4) t Benzene	7.888	533481	24.267 ng/ml
6) t Toluene	10.621	1513244	73.742 ng/ml
7) t Ethylbenzene	13.058	465349	24.451 ng/ml
8) t m-Xylene	13.191	917613	49.012 ng/ml
9) t O-Xylene	13.918	878550	48.824 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	874047	47.836 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
Data File : FB026898.D
Signal(s) : FID2B.CH
Acq On : 9 Apr 2022 3:19
Operator : AJ/MA
Sample : 50 GRO STD
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 09 03:49:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 03:48:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

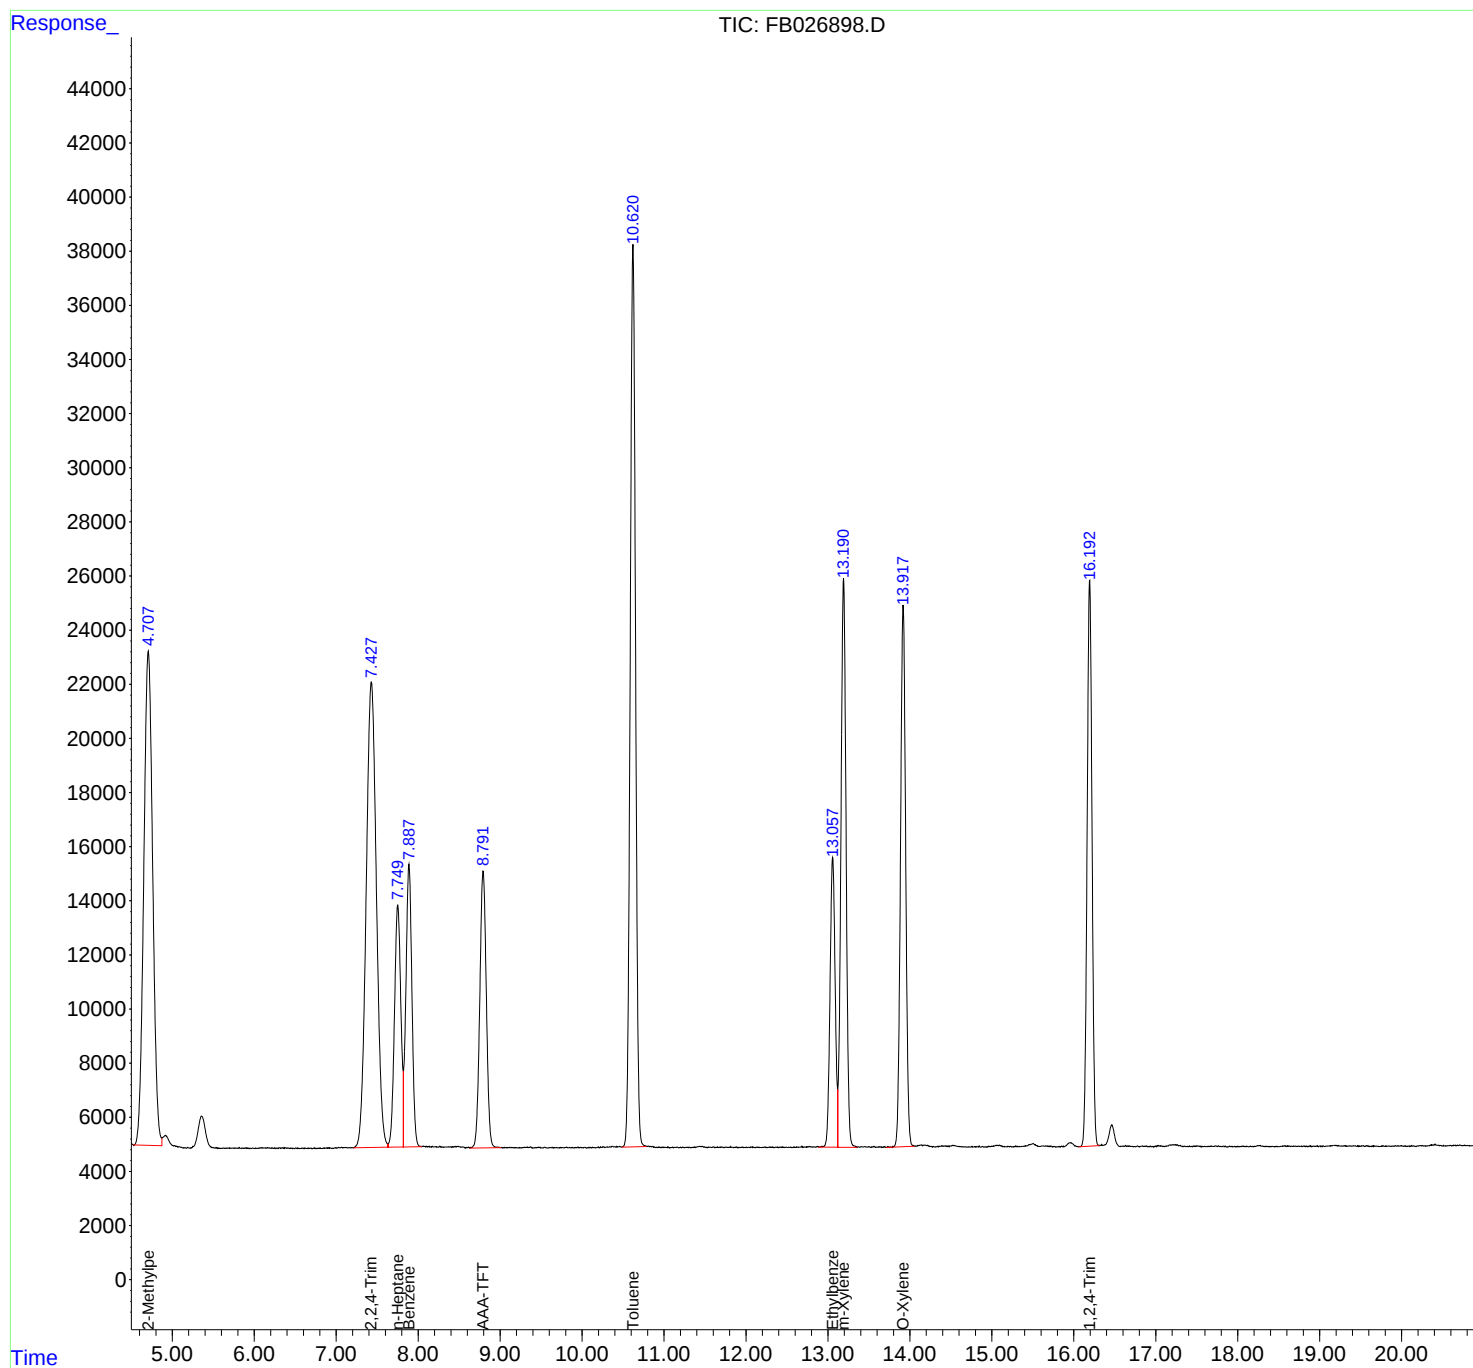


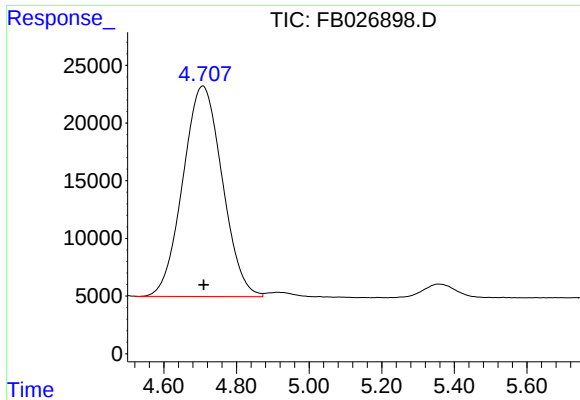

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: -0.002 min
Response: 1376266
Conc: 73.87 ng/ml

Instrument :
FID_B
ClientSampleId :

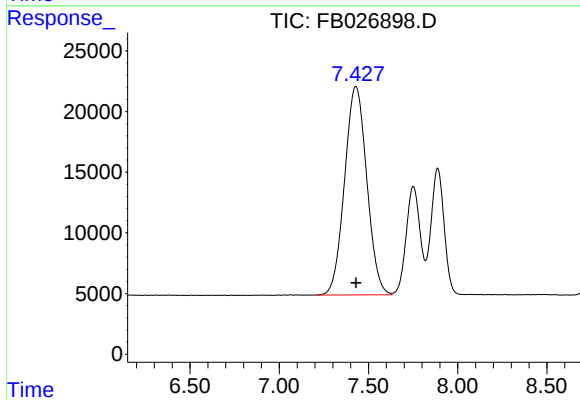


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.000 min
Response: 1486892
Conc: 74.98 ng/ml

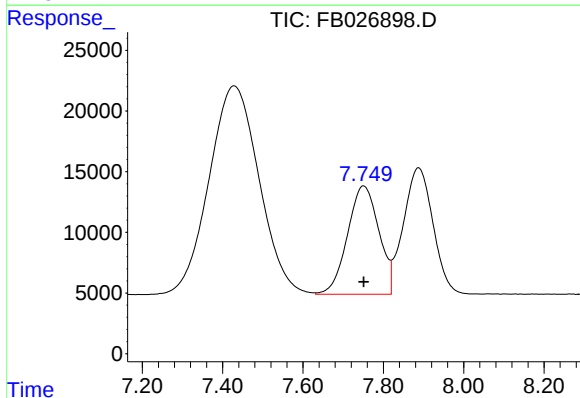


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: 0.000 min
Response: 483832
Conc: 24.76 ng/ml

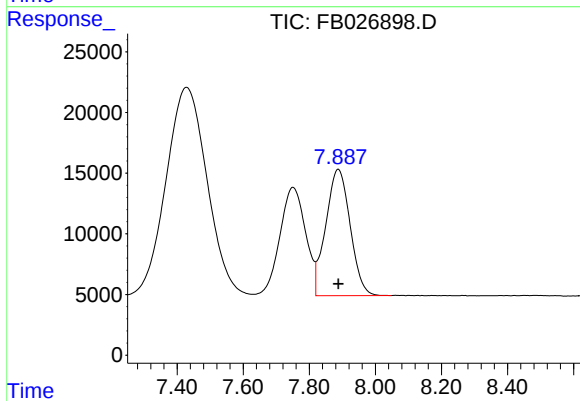

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 533481
Conc: 24.27 ng/ml

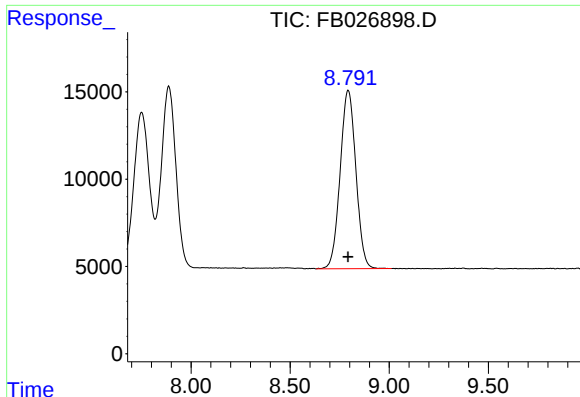

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 563816
Conc: 50.85 ng/ml

Instrument :
FID_B
ClientSampleId :

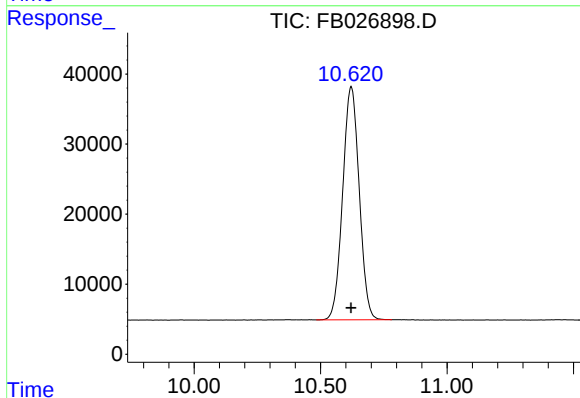


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 1513244
Conc: 73.74 ng/ml

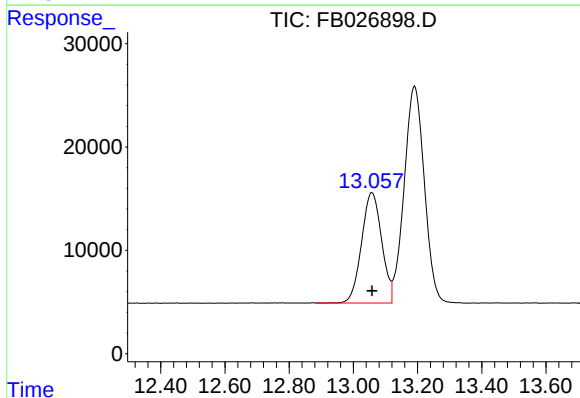


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 465349
Conc: 24.45 ng/ml

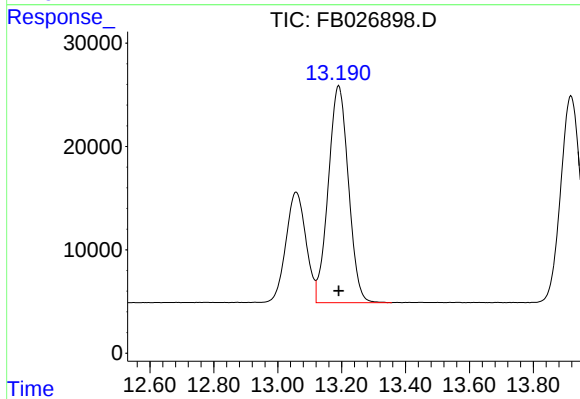

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 917613
Conc: 49.01 ng/ml

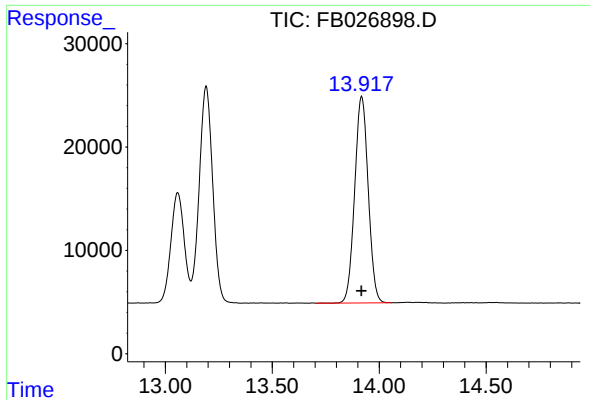

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 878550
Conc: 48.82 ng/ml

Instrument :
FID_B
ClientSampleId :

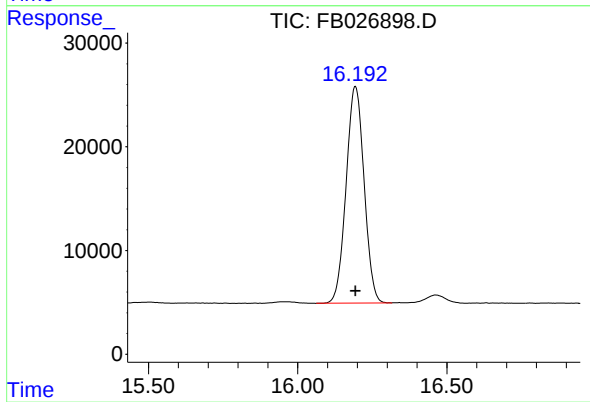

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 874047
Conc: 47.84 ng/ml