

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
 Data File : FB026937.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2022 5:57
 Operator : AJ/MA
 Sample : N2301-09
 Misc : 5.04G/5.05 ML DI WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 11 01:58:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.856	7880167	697.025 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.701	1870314	99.360 ng/ml
2) t 2,2,4-Trimethylpentane	7.477	17862110	892.856 ng/ml
3) t n-Heptane	7.740	4450578	227.515 ng/ml
7) t Ethylbenzene	13.032	68523603	3586.342 ng/ml
9) t O-Xylene	13.952	7985089	440.832 ng/ml
10) t 1,2,4-Trimethylbenzene	16.231	2282699	123.846 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
Data File : FB026937.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2022 5:57
Operator : AJ/MA
Sample : N2301-09
Misc : 5.04G/5.05 ML DI WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 11 01:58:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

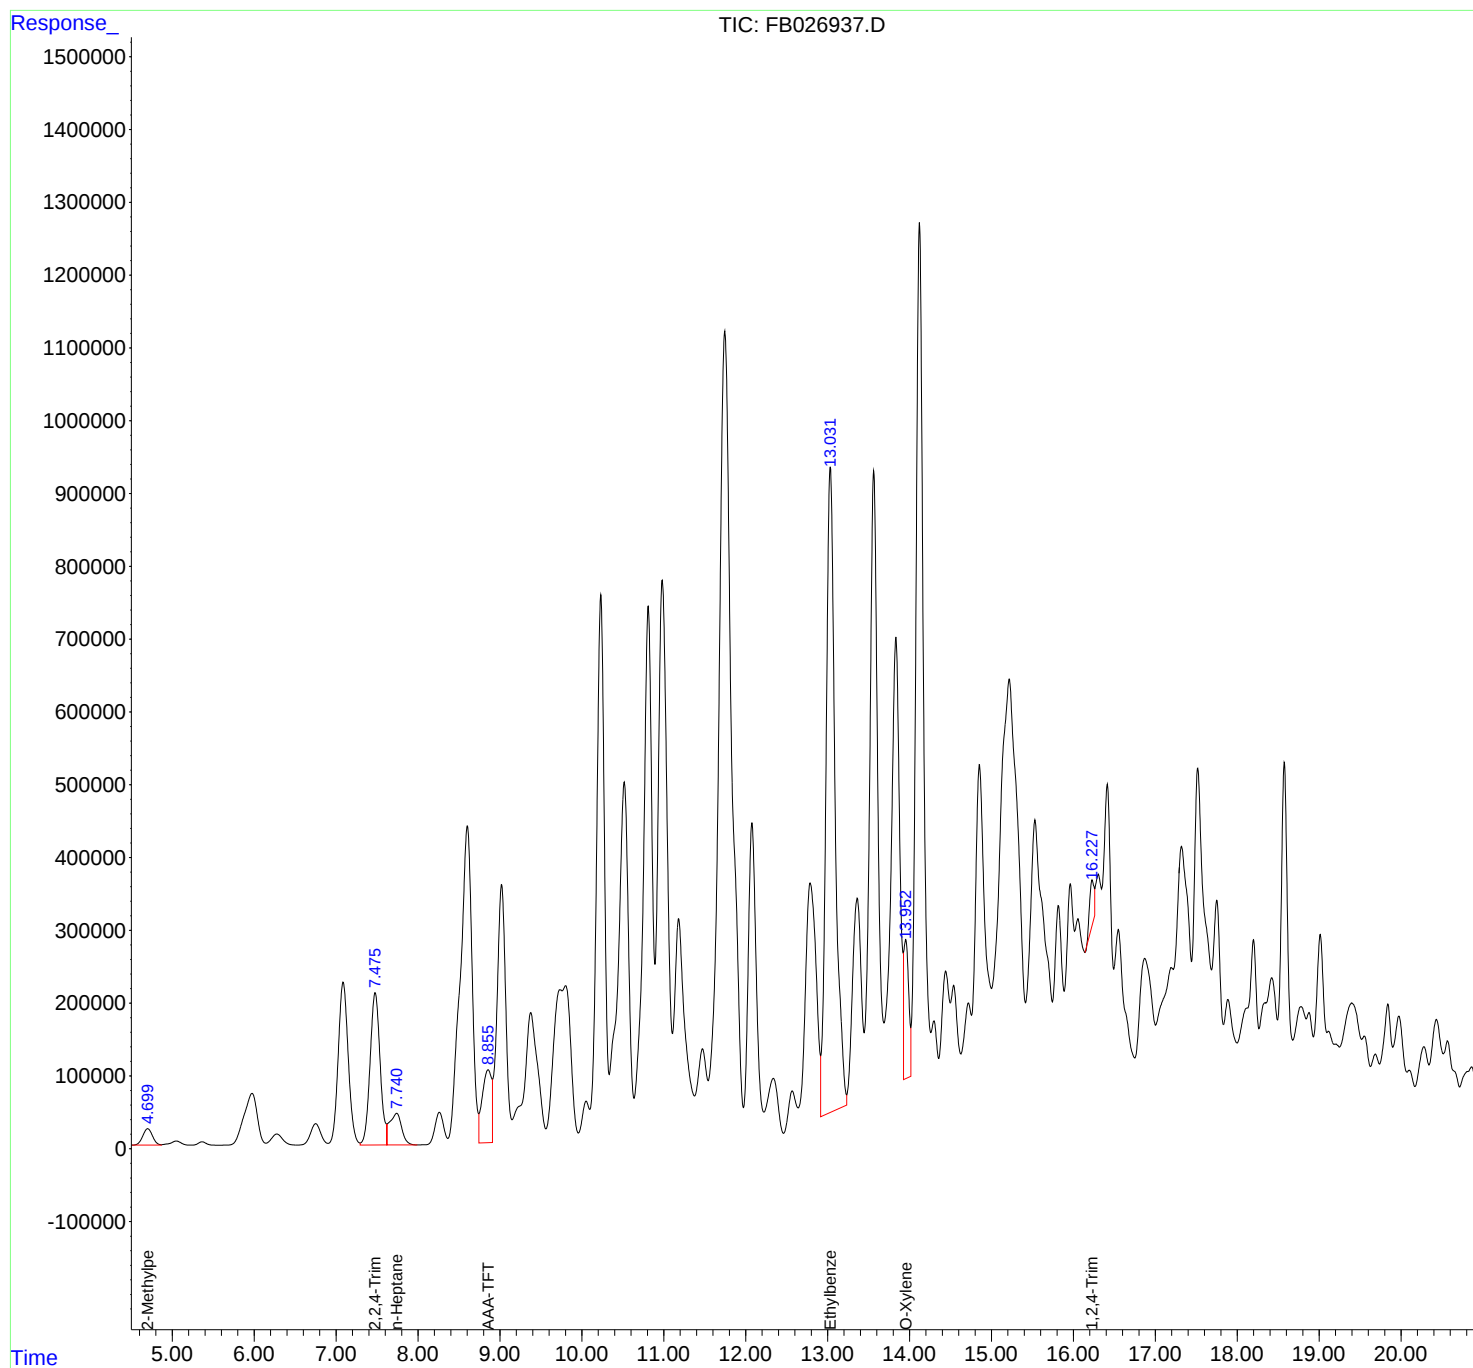


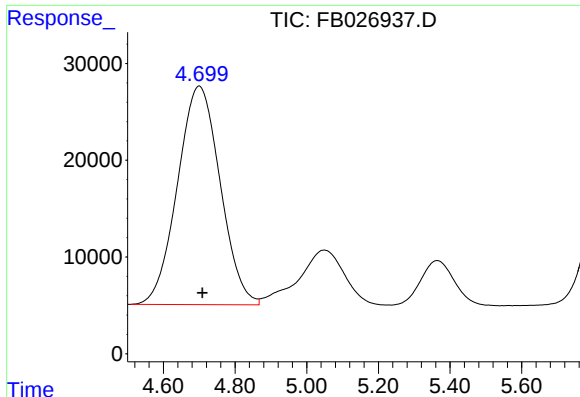

#1 2-Methylpentane


R.T.: 4.701 min
Delta R.T.: -0.008 min
Response: 1870314
Conc: 99.36 ng/ml

Instrument :
FID_B
ClientSampleId :

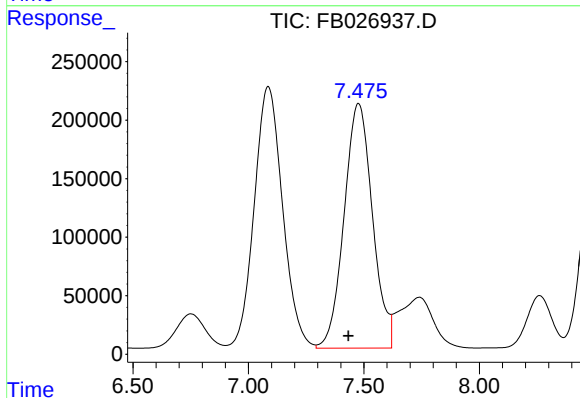


#2 2,2,4-Trimethylpentane

R.T.: 7.477 min
Delta R.T.: 0.044 min
Response: 17862110
Conc: 892.86 ng/ml

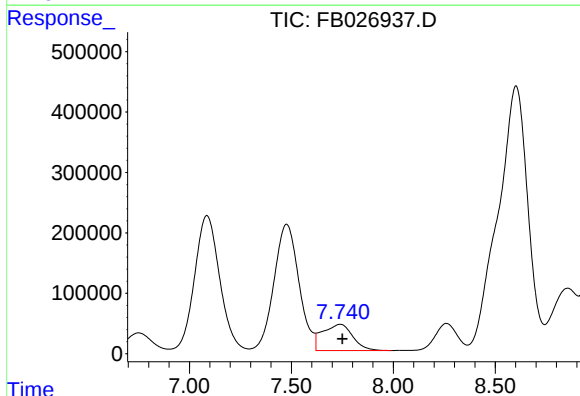


#3 n-Heptane

R.T.: 7.740 min
Delta R.T.: -0.010 min
Response: 4450578
Conc: 227.52 ng/ml

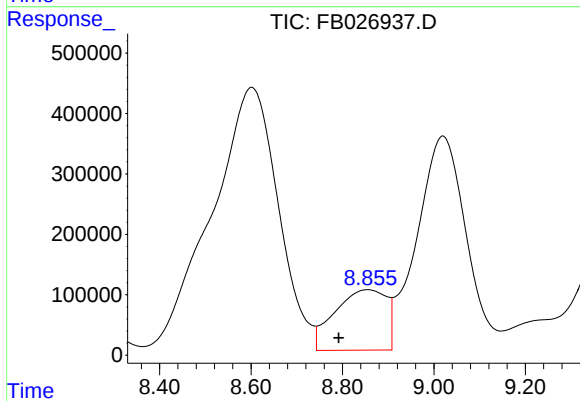

#5 AAA-TFT


R.T.: 8.856 min
Delta R.T.: 0.064 min
Response: 7880167
Conc: 697.02 ng/ml

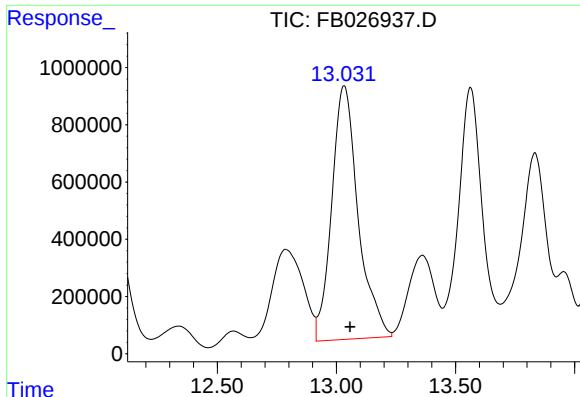

#7 Ethylbenzene


R.T.: 13.032 min
Delta R.T.: -0.026 min
Response: 68523603
Conc: 3586.34 ng/ml

Instrument :
FID_B
ClientSampleId :

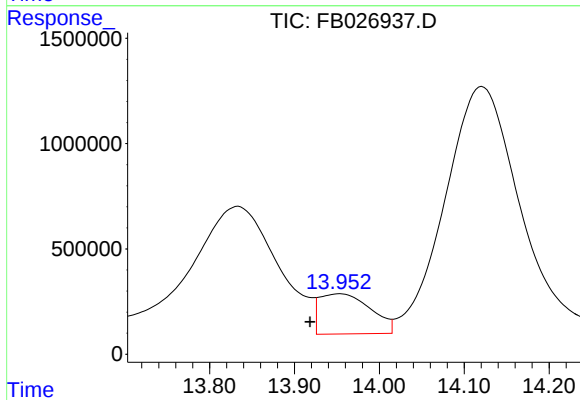

#9 O-Xylene

R.T.: 13.952 min
Delta R.T.: 0.034 min
Response: 7985089
Conc: 440.83 ng/ml

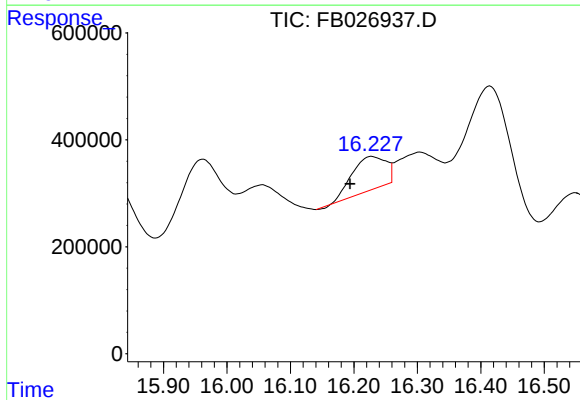

#10 1,2,4-Trimethylbenzene

R.T.: 16.231 min
Delta R.T.: 0.037 min
Response: 2282699
Conc: 123.85 ng/ml