

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
 Data File : FB026940.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2022 7:45
 Operator : AJ/MA
 Sample : N2301-12
 Misc : 5.04G/5.05 ML DI WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 11 01:59:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.854	450813	39.876 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.688	18833	1.001 ng/ml
2) t 2,2,4-Trimethylpentane	7.443	173868	8.691 ng/ml
3) t n-Heptane	7.803	226818	11.595 ng/ml
7) t Ethylbenzene	13.016	186791	9.776 ng/ml
9) t O-Xylene	13.936	9085	0.502 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
Data File : FB026940.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2022 7:45
Operator : AJ/MA
Sample : N2301-12
Misc : 5.04G/5.05 ML DI WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 11 01:59:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

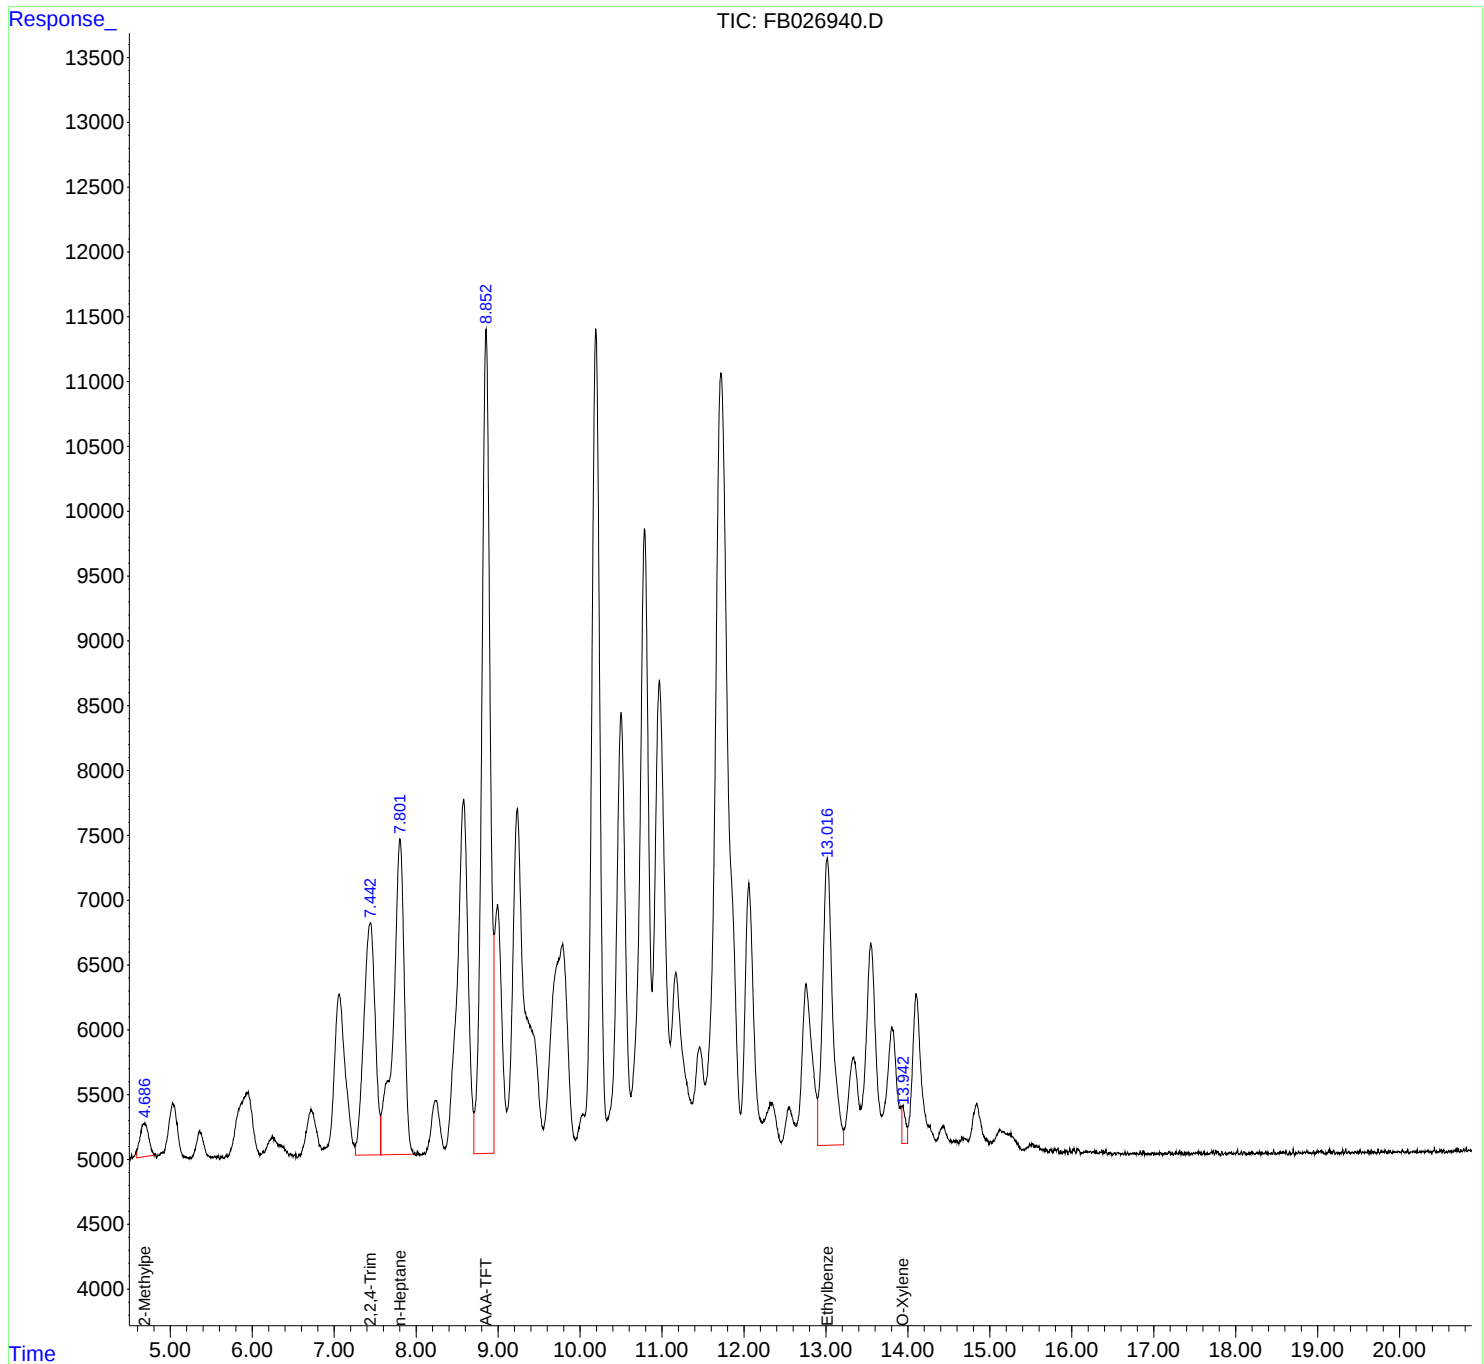


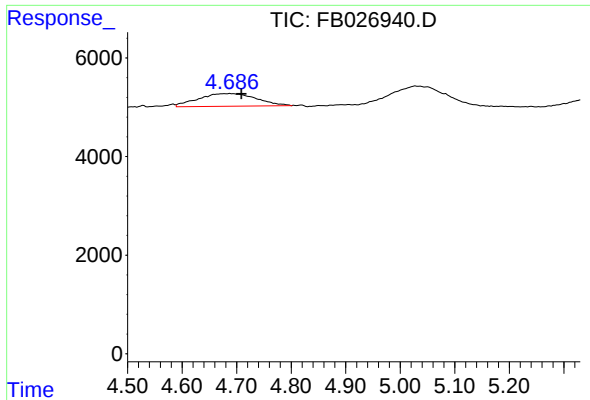

#1 2-Methylpentane


R.T.: 4.688 min
Delta R.T.: -0.021 min
Response: 18833
Conc: 1.00 ng/ml

Instrument :
FID_B
ClientSampleId :

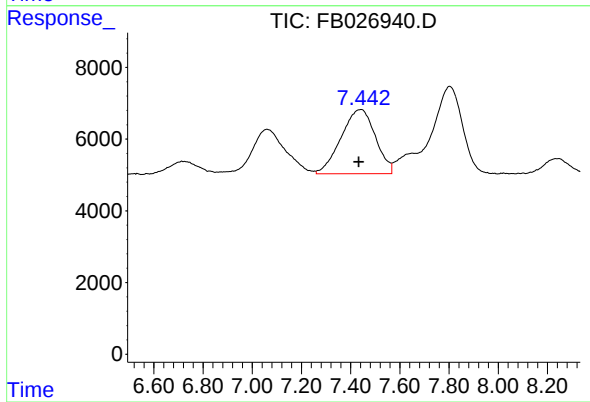


#2 2,2,4-Trimethylpentane

R.T.: 7.443 min
Delta R.T.: 0.010 min
Response: 173868
Conc: 8.69 ng/ml

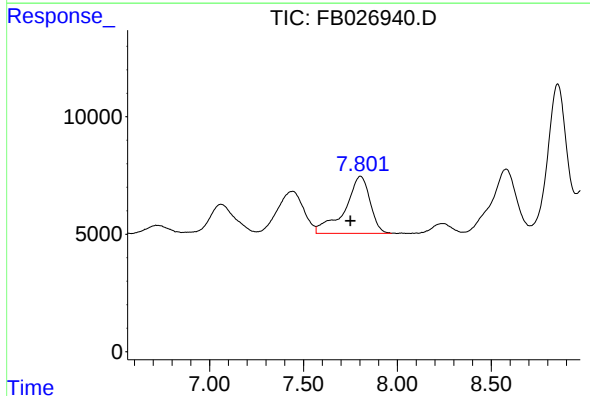


#3 n-Heptane

R.T.: 7.803 min
Delta R.T.: 0.052 min
Response: 226818
Conc: 11.60 ng/ml

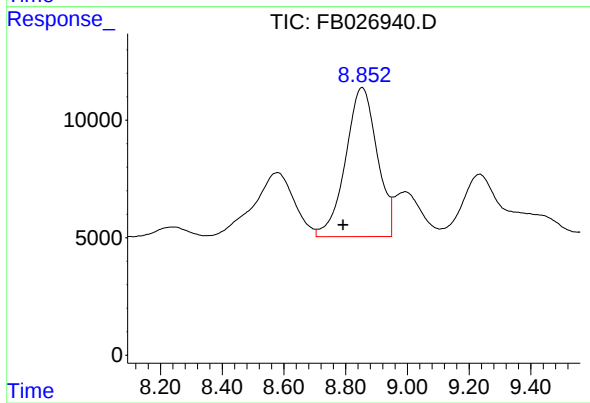

#5 AAA-TFT


R.T.: 8.854 min
Delta R.T.: 0.062 min
Response: 450813
Conc: 39.88 ng/ml

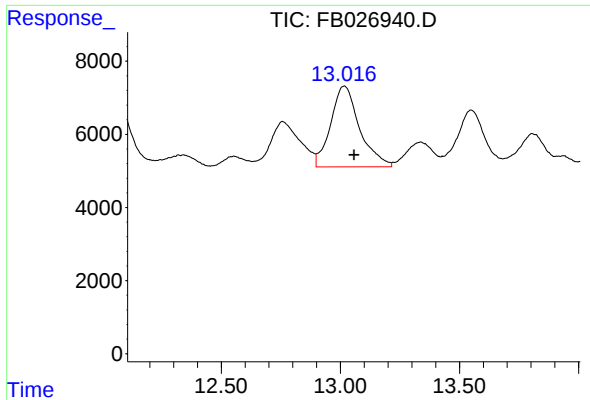

#7 Ethylbenzene

R.T.: 13.016 min
Delta R.T.: -0.042 min
Response: 186791
Conc: 9.78 ng/ml

Instrument :
FID_B
ClientSampleId :

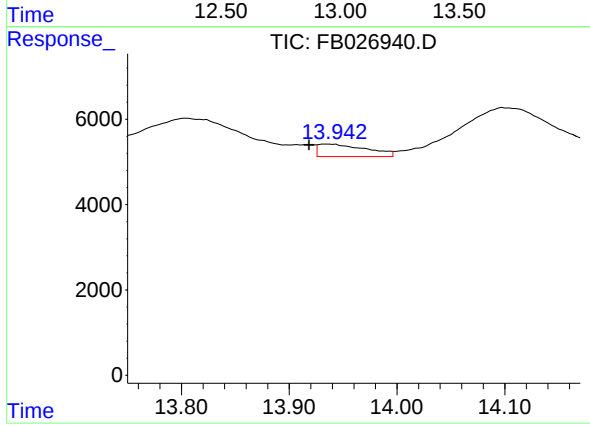

#9 O-Xylene

R.T.: 13.936 min
Delta R.T.: 0.018 min
Response: 9085
Conc: 0.50 ng/ml