

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
 Data File : FB026904.D
 Signal(s) : FID2B.CH
 Acq On : 9 Apr 2022 8:44
 Operator : AJ/MA
 Sample : BSF0409S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0409S1

Integration File: SAMPLE.e
 Quant Time: Apr 09 09:30:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	223053	19.730 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.708	526573	27.974 ng/ml
2) t 2,2,4-Trimethylpentane	7.426	547952	27.390 ng/ml
3) t n-Heptane	7.752	182759	9.343 ng/ml
4) t Benzene	7.889	203832	9.236 ng/ml
6) t Toluene	10.622	581587	28.205 ng/ml
7) t Ethylbenzene	13.059	180469	9.445 ng/ml
8) t m-Xylene	13.192	358763	18.993 ng/ml
9) t O-Xylene	13.919	343987	18.990 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	356463	19.340 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040922\
Data File : FB026904.D
Signal(s) : FID2B.CH
Acq On : 9 Apr 2022 8:44
Operator : AJ/MA
Sample : BSF0409S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0409S1

Integration File: SAMPLE.e
Quant Time: Apr 09 09:30:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

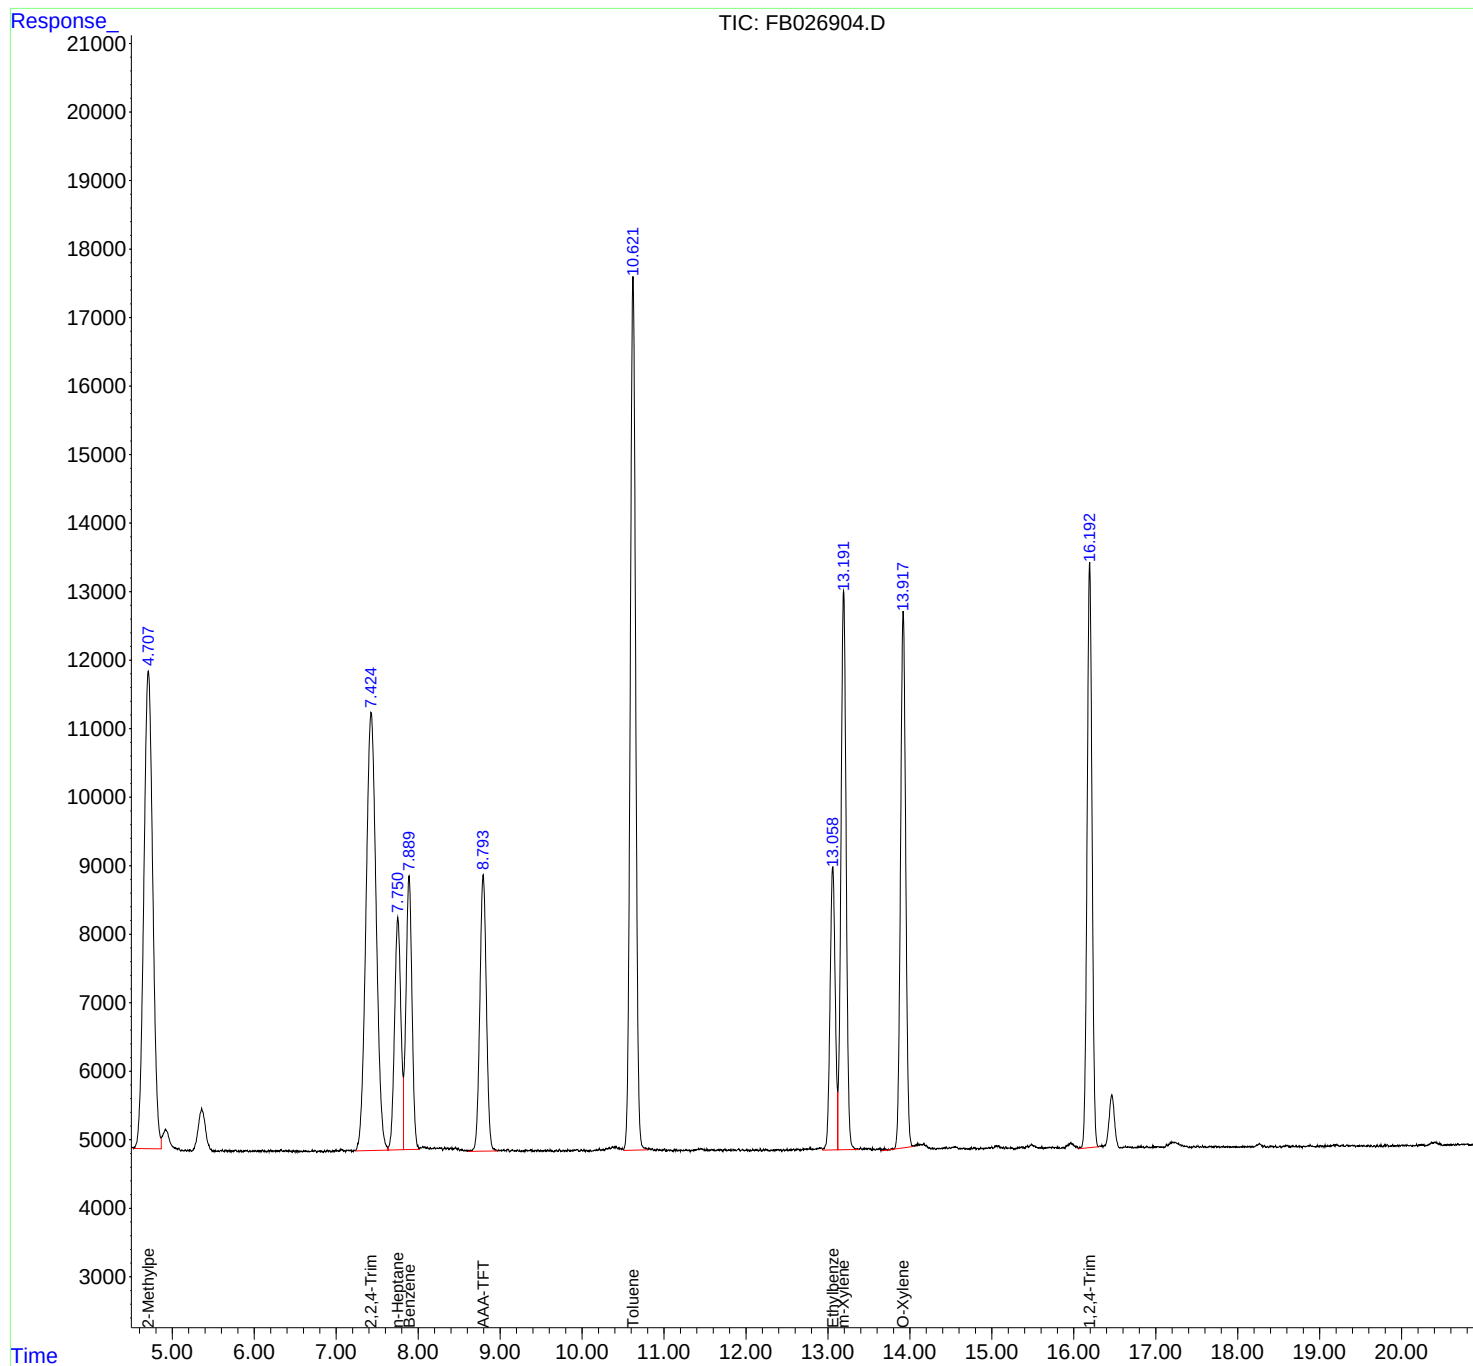


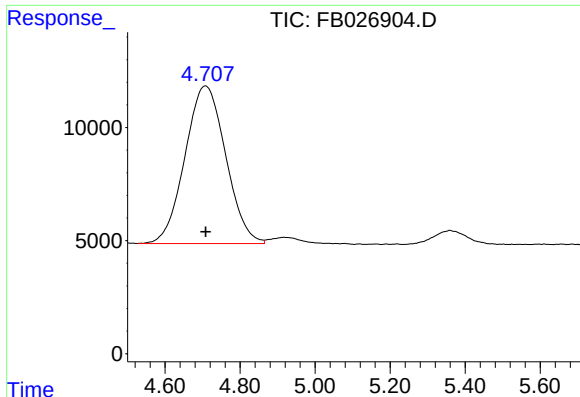

#1 2-Methylpentane


R.T.: 4.708 min
Delta R.T.: 0.000 min
Response: 526573
Conc: 27.97 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0409S1

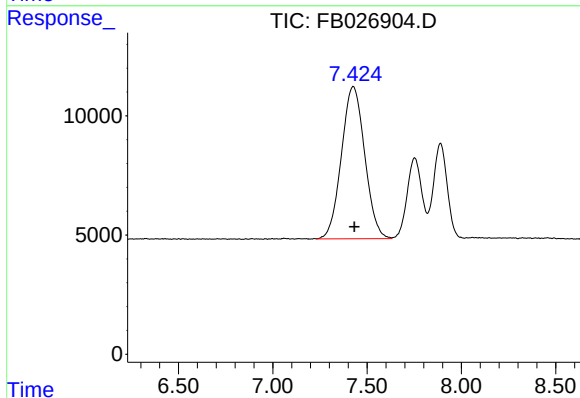


#2 2,2,4-Trimethylpentane

R.T.: 7.426 min
Delta R.T.: -0.007 min
Response: 547952
Conc: 27.39 ng/ml

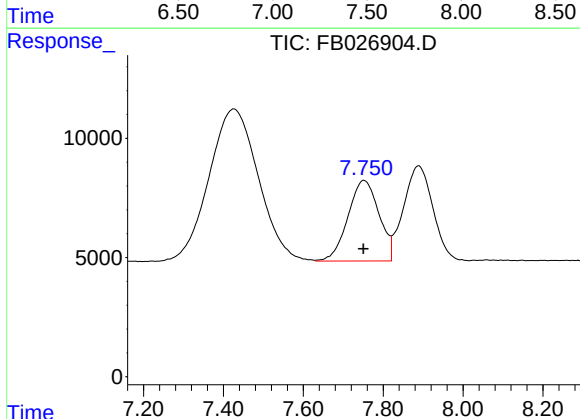


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 182759
Conc: 9.34 ng/ml

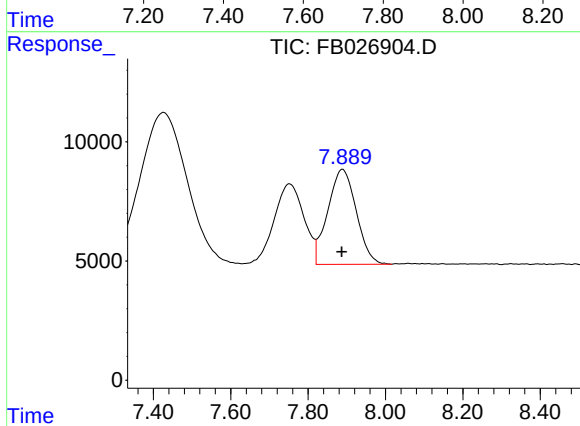

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.002 min
Response: 203832
Conc: 9.24 ng/ml

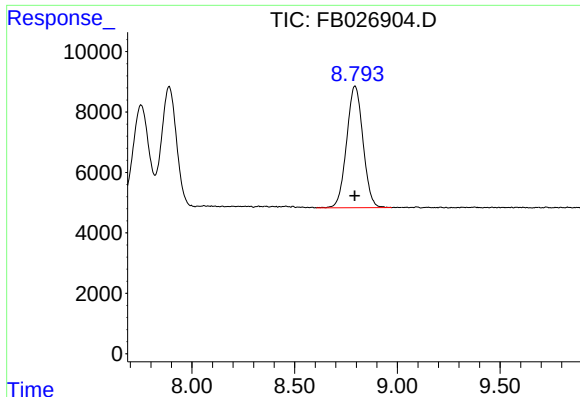

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.002 min
Response: 223053
Conc: 19.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0409S1

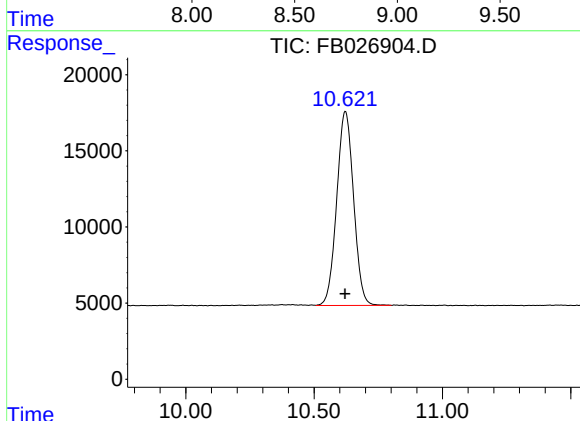


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.001 min
Response: 581587
Conc: 28.21 ng/ml

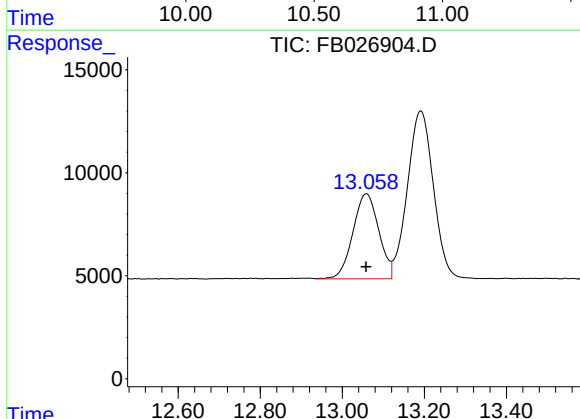


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.001 min
Response: 180469
Conc: 9.45 ng/ml

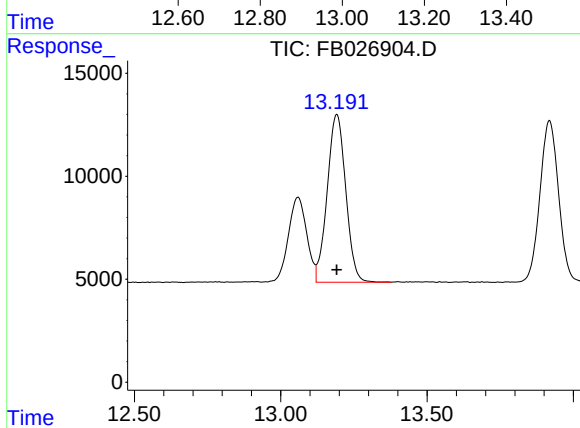

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.000 min
Response: 358763
Conc: 18.99 ng/ml

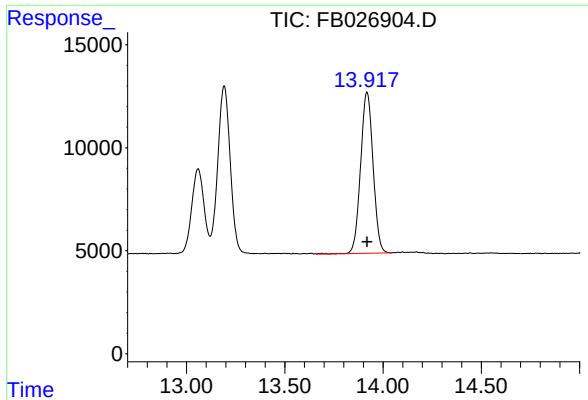

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.000 min
Response: 343987
Conc: 18.99 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0409S1

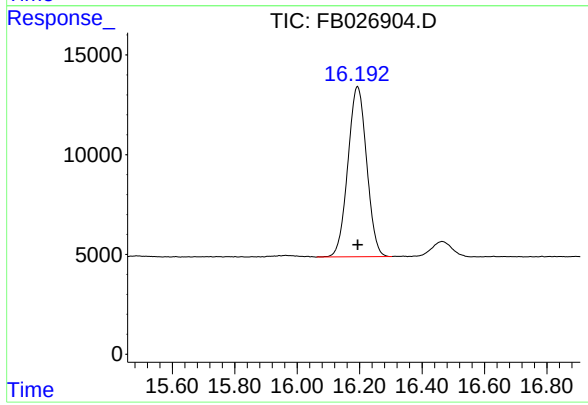

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.000 min
Response: 356463
Conc: 19.34 ng/ml