

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
 Data File : FB024113.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2020 7:53
 Operator : DD/AJ
 Sample : BSF0410S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 11 00:43:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	477808	19.071 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.689	1009552	30.928 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	1088005	31.881 ng/ml
3) t	n-Heptane	7.759	362049	10.727 ng/ml
4) t	Benzene	7.893	423588	10.495 ng/ml
6) t	Toluene	10.632	1201601	30.566 ng/ml
7) t	Ethylbenzene	13.073	370723	10.169 ng/ml
8) t	m-Xylene	13.206	718794	20.534 ng/ml
9) t	O-Xylene	13.933	702557	20.613 ng/ml
10) t	1,2,4-Trimethylbenzene	16.212	595354	20.968 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
Data File : FB024113.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2020 7:53
Operator : DD/AJ
Sample : BSF0410S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 11 00:43:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

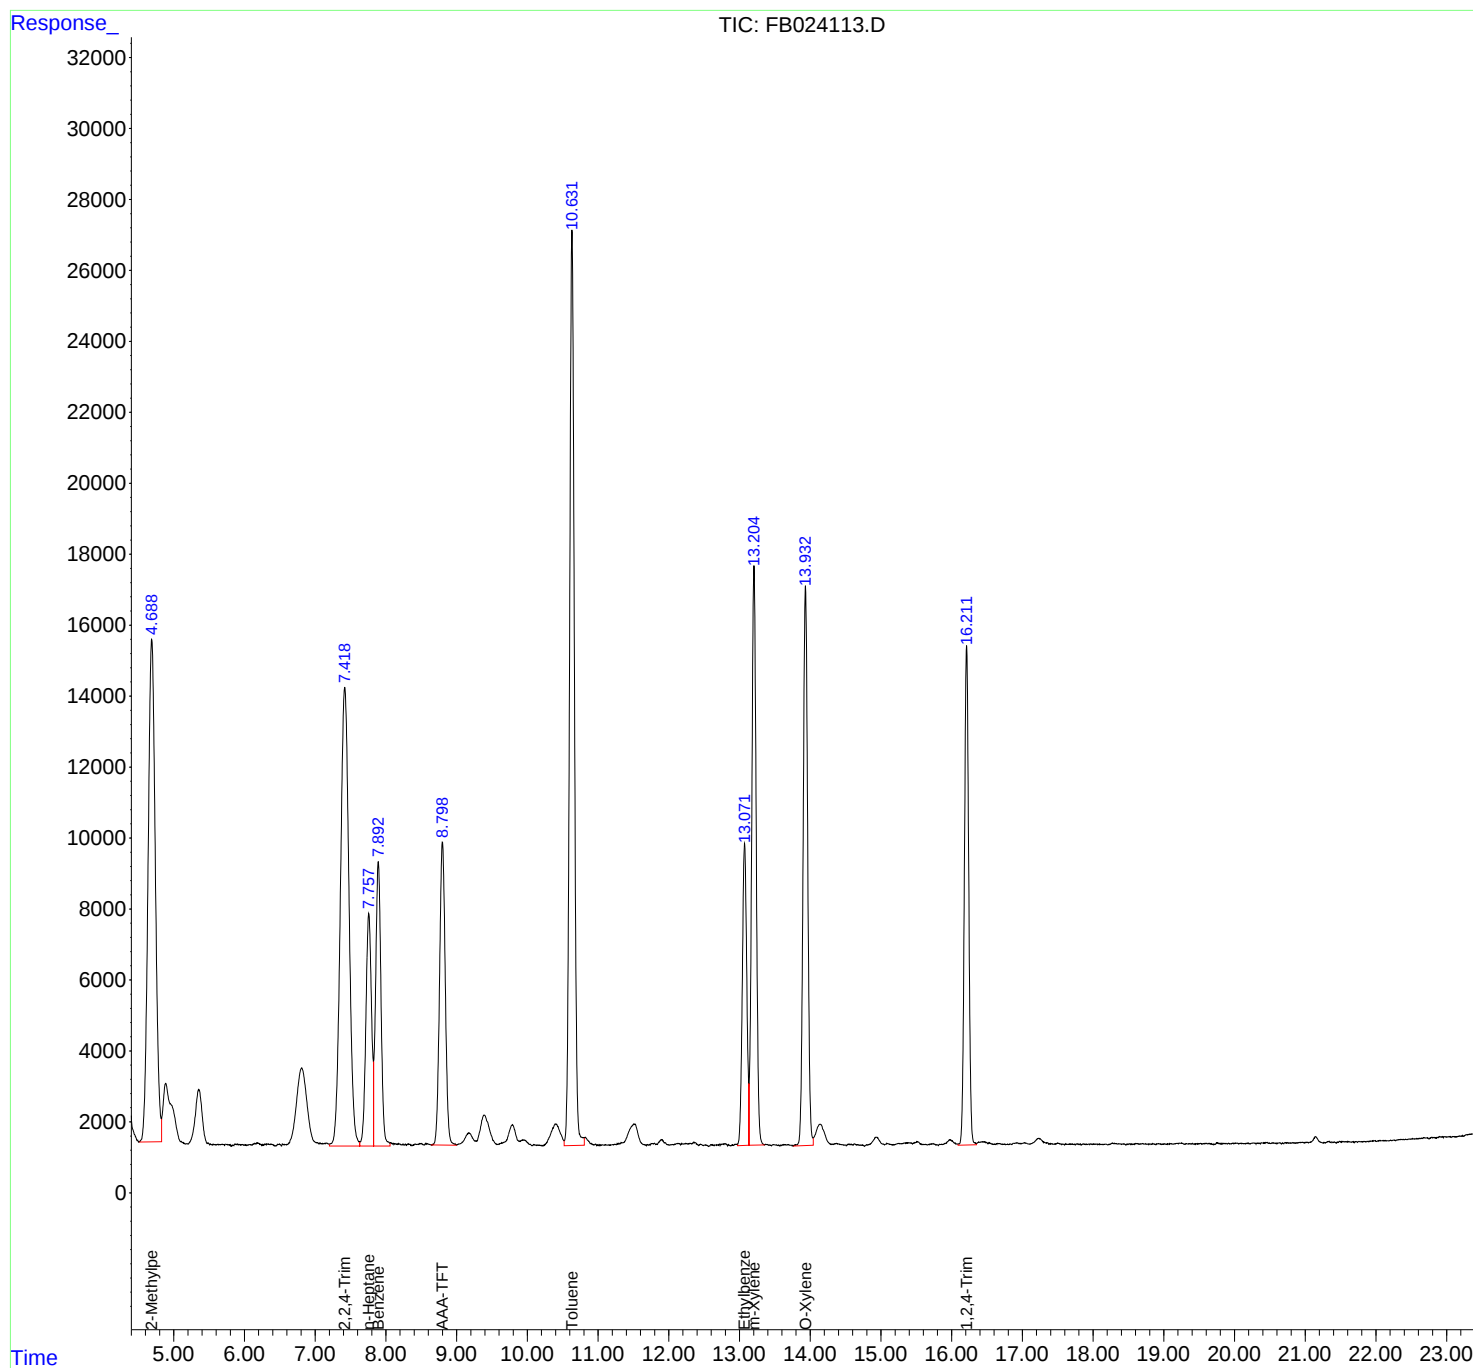

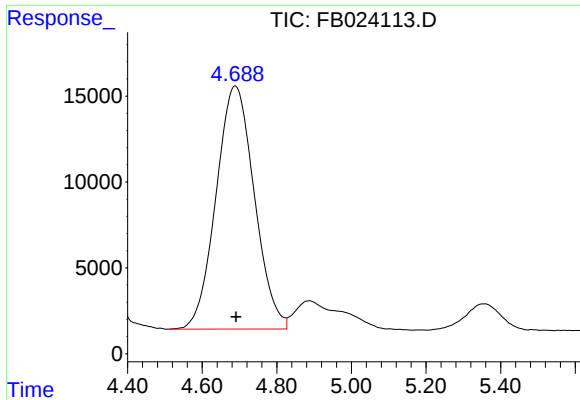


#1 2-Methylpentane

R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 1009552
Conc: 30.93 ng/ml

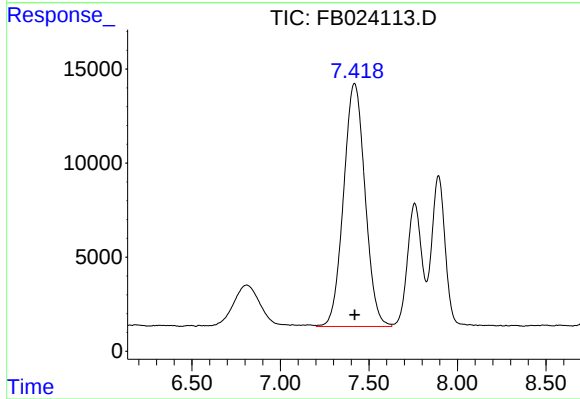


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1088005
Conc: 31.88 ng/ml

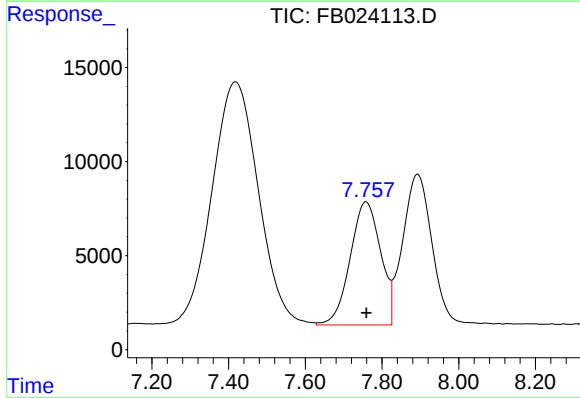


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 362049
Conc: 10.73 ng/ml

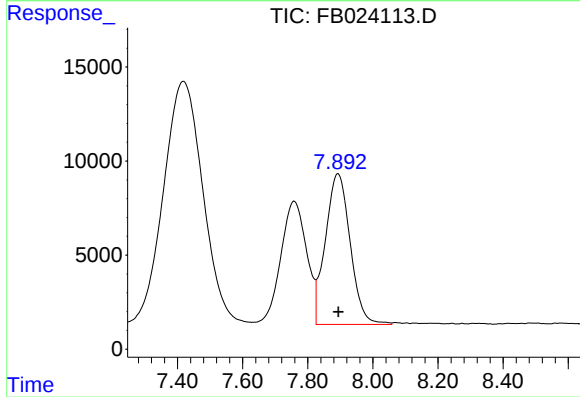


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 423588
Conc: 10.50 ng/ml

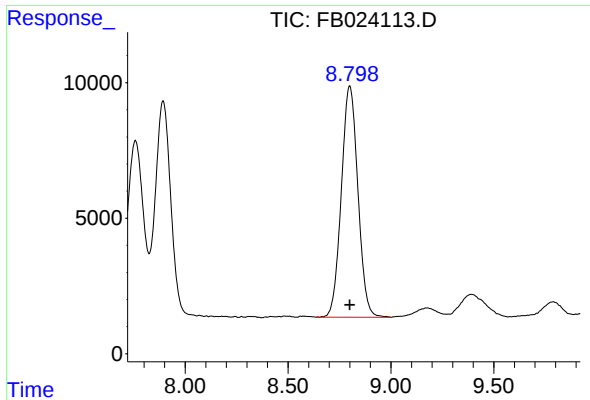


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 477808
Conc: 19.07 ng/ml

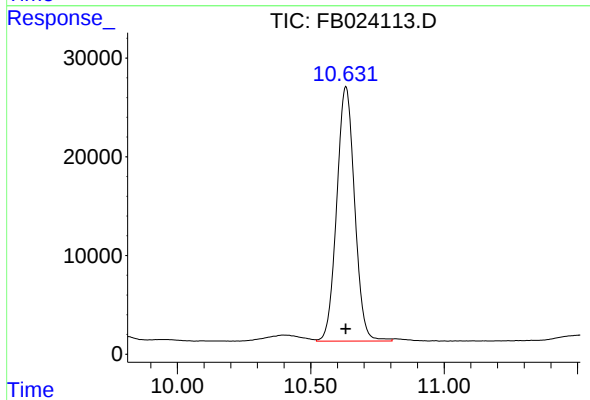


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1201601
Conc: 30.57 ng/ml

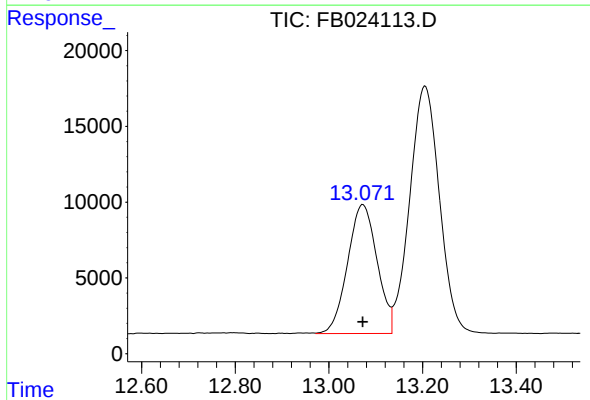


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 370723
Conc: 10.17 ng/ml

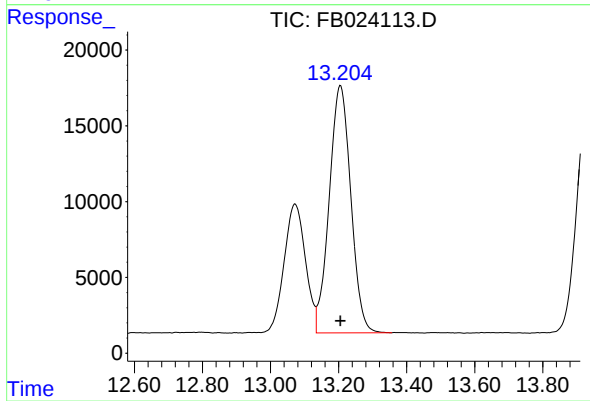


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 718794
Conc: 20.53 ng/ml

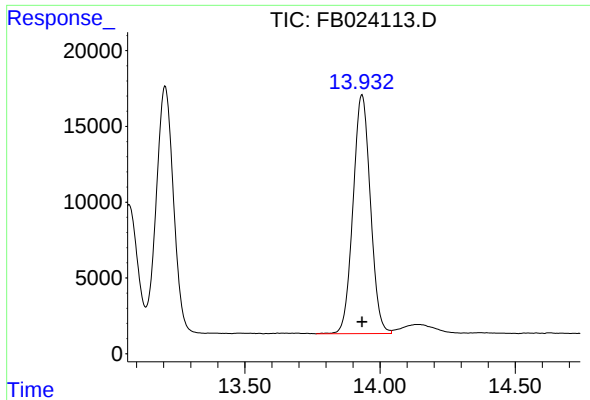

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 702557
Conc: 20.61 ng/ml

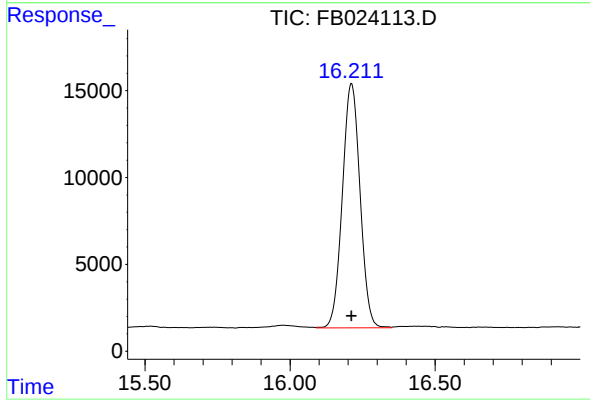

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 595354
Conc: 20.97 ng/ml