

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
 Data File : FB024121.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2020 11:57
 Operator : DD/AJ
 Sample : L2205-18MS
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 11 00:44:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	488660	19.505 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	1004546	30.774 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1067777	31.289 ng/ml
3) t n-Heptane	7.760	352788	10.453 ng/ml
4) t Benzene	7.894	419867	10.403 ng/ml
6) t Toluene	10.633	1196290	30.431 ng/ml
7) t Ethylbenzene	13.073	370175	10.154 ng/ml
8) t m-Xylene	13.206	713894	20.394 ng/ml
9) t O-Xylene	13.934	693058	20.334 ng/ml
10) t 1,2,4-Trimethylbenzene	16.212	583574	20.553 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
Data File : FB024121.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2020 11:57
Operator : DD/AJ
Sample : L2205-18MS
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 11 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 11 00:44:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

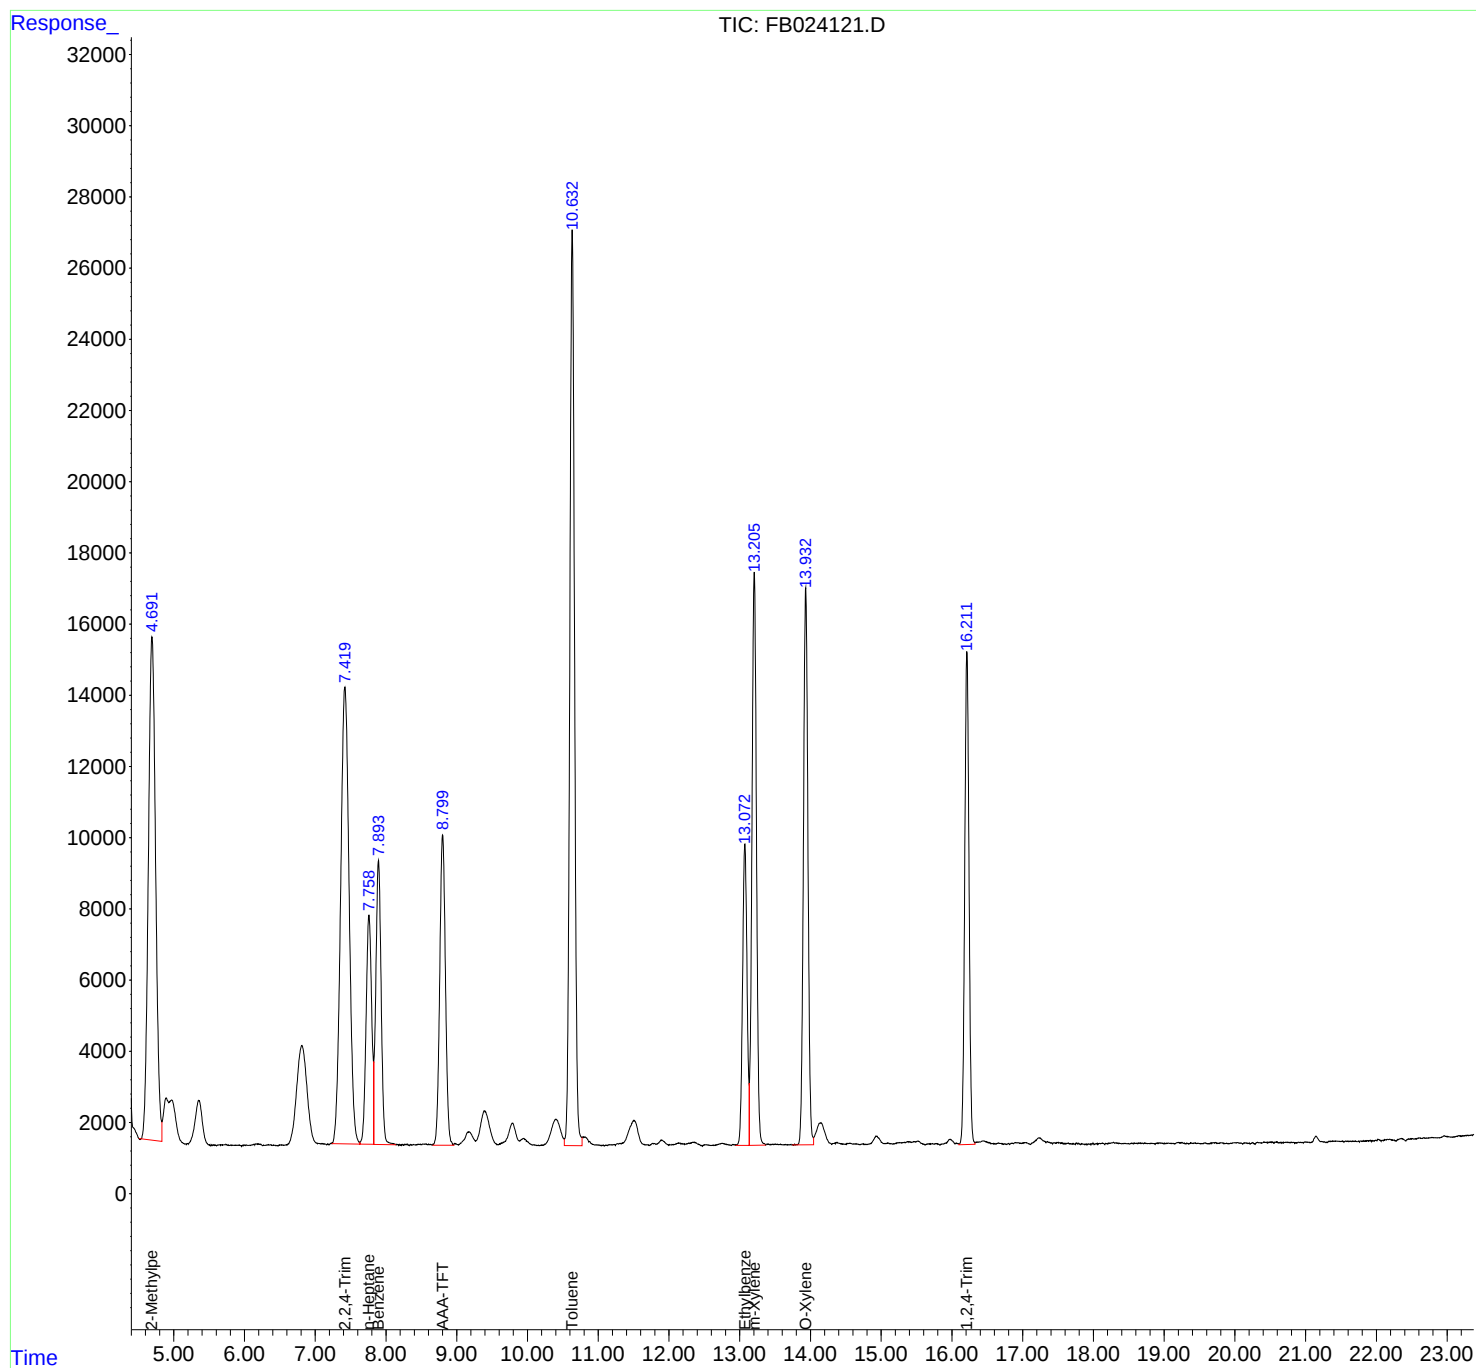

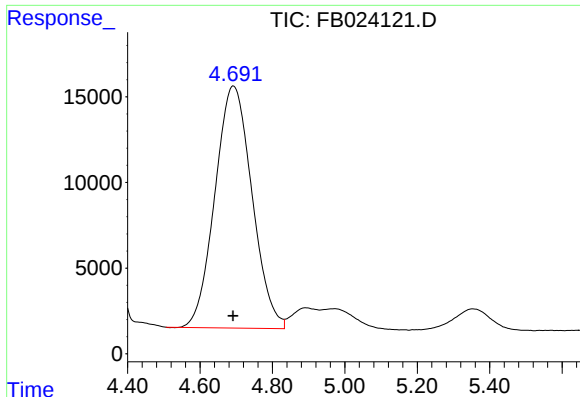


#1 2-Methylpentane

R.T.: 4.692 min
Delta R.T.: 0.001 min
Response: 1004546
Conc: 30.77 ng/ml

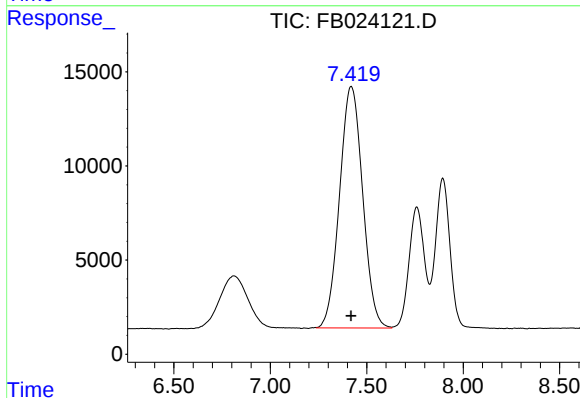


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 1067777
Conc: 31.29 ng/ml

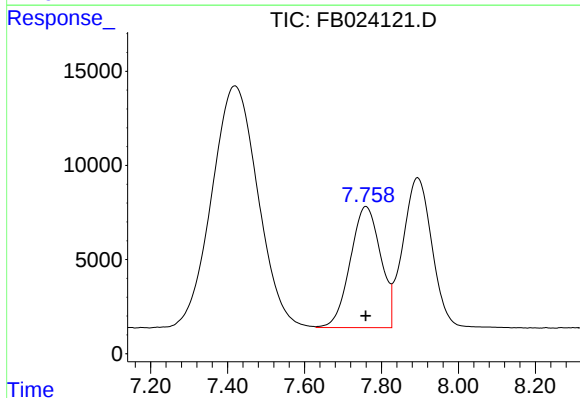


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 352788
Conc: 10.45 ng/ml

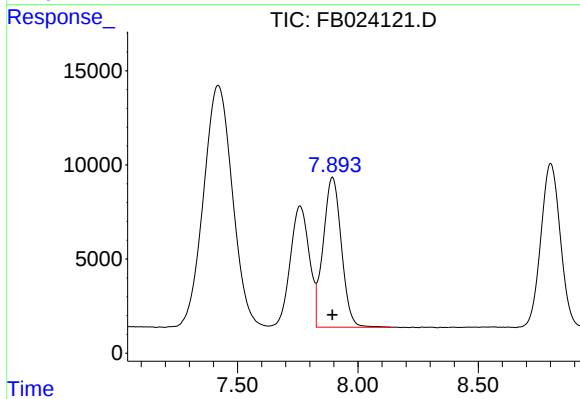


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 419867
Conc: 10.40 ng/ml

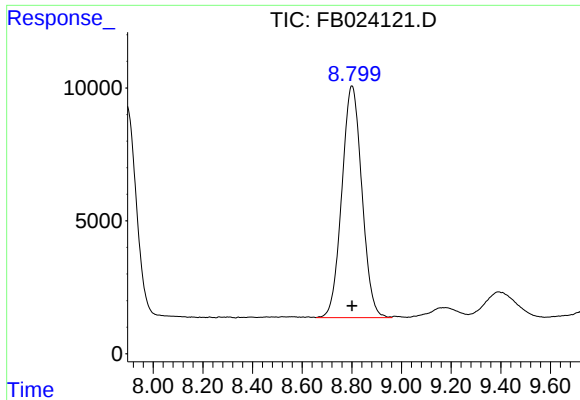


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 488660
Conc: 19.50 ng/ml

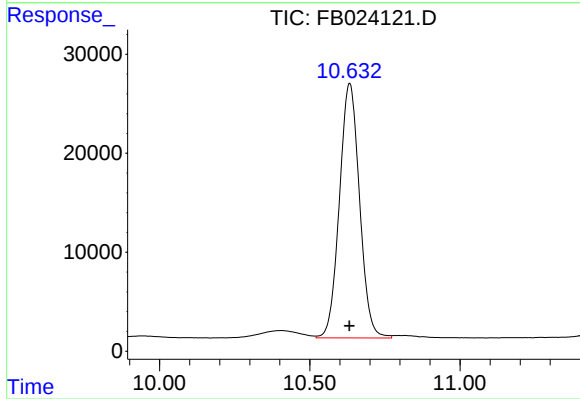


#6 Toluene

R.T.: 10.633 min
Delta R.T.: 0.001 min
Response: 1196290
Conc: 30.43 ng/ml

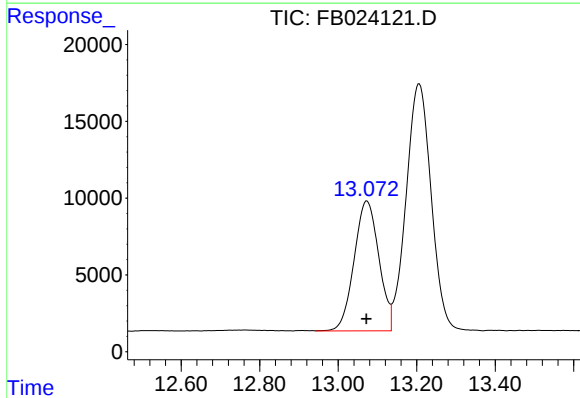


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 370175
Conc: 10.15 ng/ml

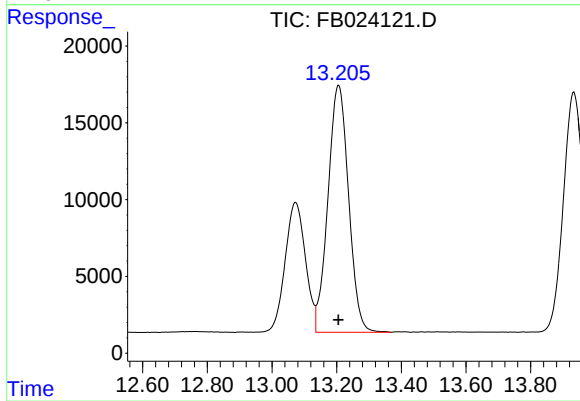


#8 m-Xylene

R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 713894
Conc: 20.39 ng/ml

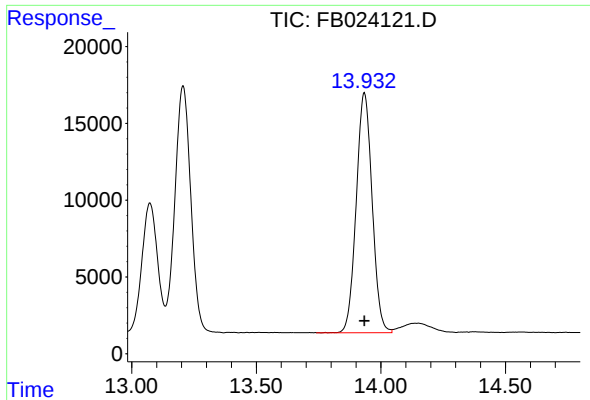

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 693058
Conc: 20.33 ng/ml

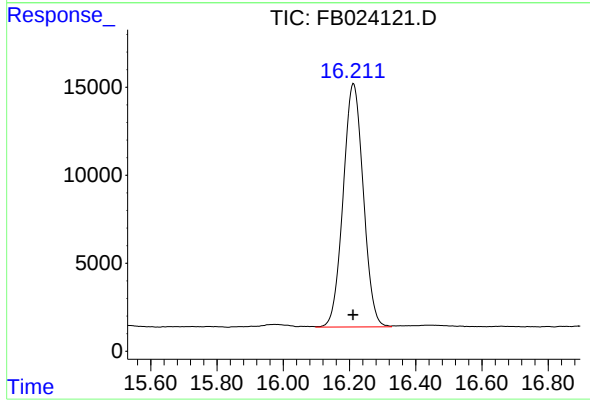

#10 1,2,4-Trimethylbenzene

R.T.: 16.212 min
Delta R.T.: 0.000 min
Response: 583574
Conc: 20.55 ng/ml