

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
 Data File : FB024122.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2020 12:27
 Operator : DD/AJ
 Sample : L2205-18MSD
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 11 00:45:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
 Quant Title :
 QLast Update : Wed Apr 08 10:11:26 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	476828	19.032 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	975853	29.895 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1024741	30.027 ng/ml
3) t n-Heptane	7.759	338281	10.023 ng/ml
4) t Benzene	7.893	417913	10.355 ng/ml
6) t Toluene	10.631	1172495	29.826 ng/ml
7) t Ethylbenzene	13.072	355772	9.759 ng/ml
8) t m-Xylene	13.205	692224	19.775 ng/ml
9) t O-Xylene	13.933	680257	19.959 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	565348	19.911 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041020\
Data File : FB024122.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2020 12:27
Operator : DD/AJ
Sample : L2205-18MSD
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 12 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 11 00:45:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040820.M
Quant Title :
QLast Update : Wed Apr 08 10:11:26 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

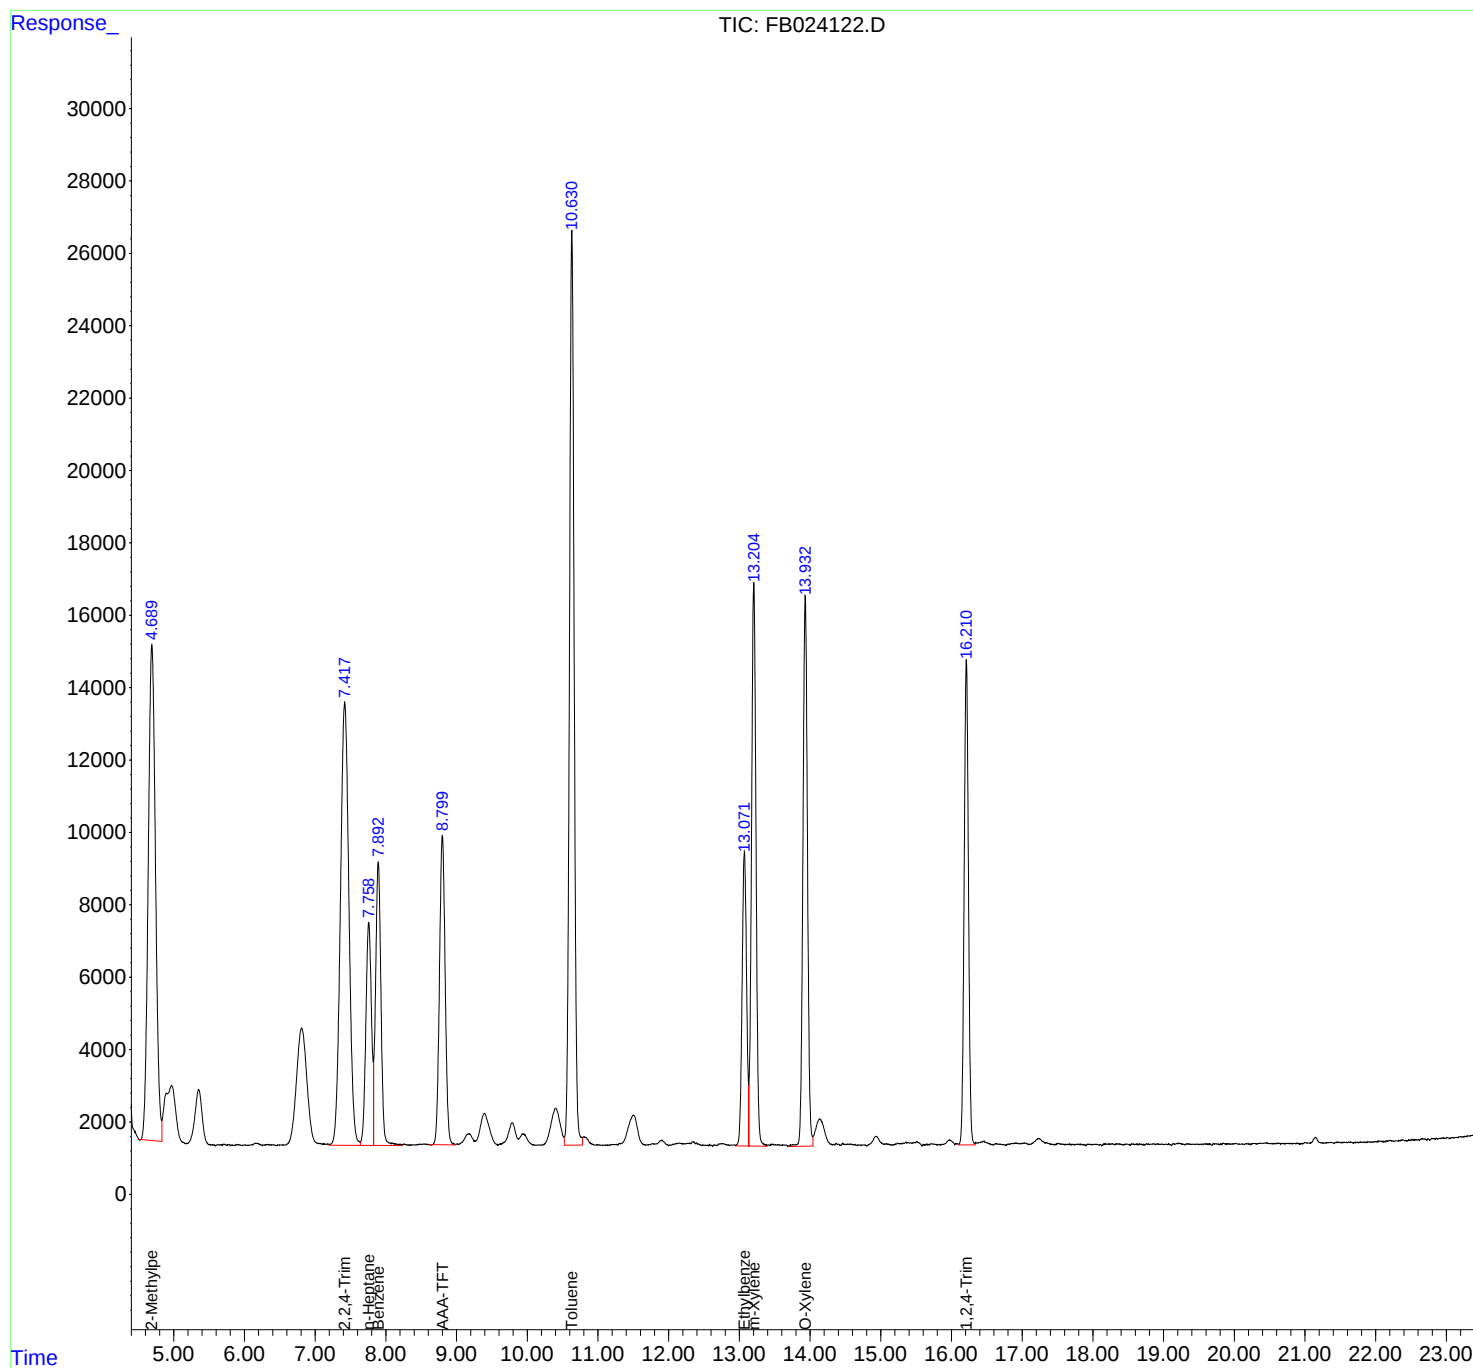

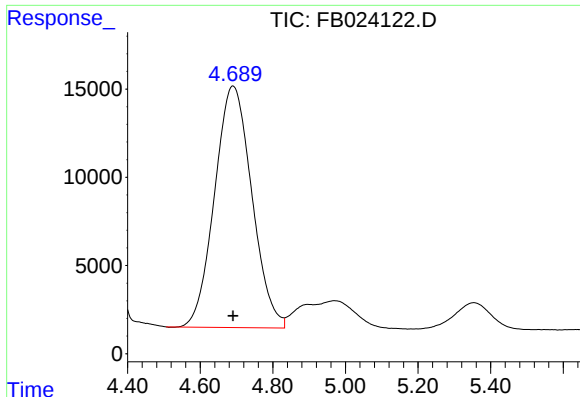


#1 2-Methylpentane

R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 975853
Conc: 29.90 ng/ml

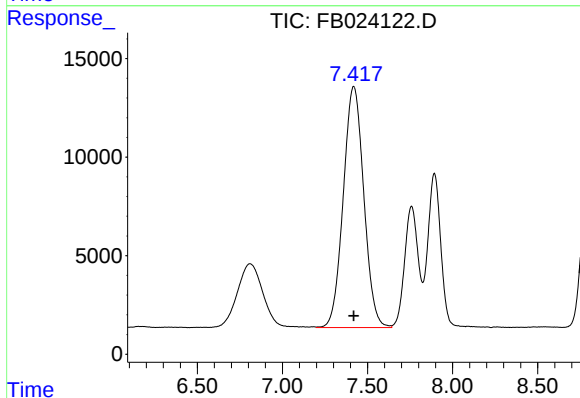


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1024741
Conc: 30.03 ng/ml

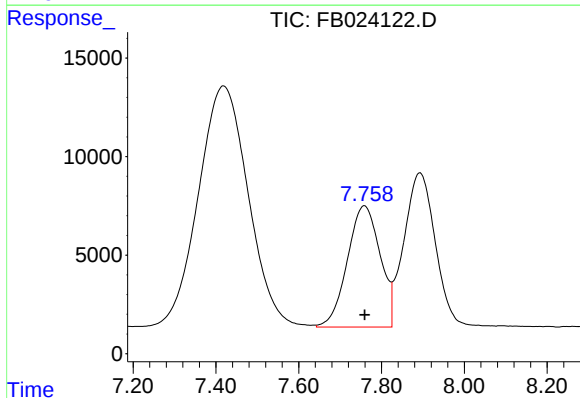


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 338281
Conc: 10.02 ng/ml

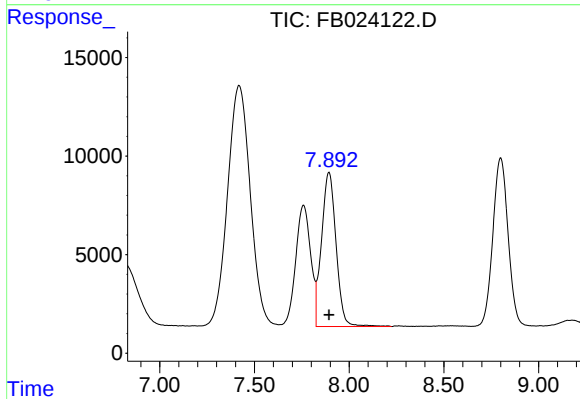


#4 Benzene

R.T.: 7.893 min
Delta R.T.: 0.000 min
Response: 417913
Conc: 10.35 ng/ml

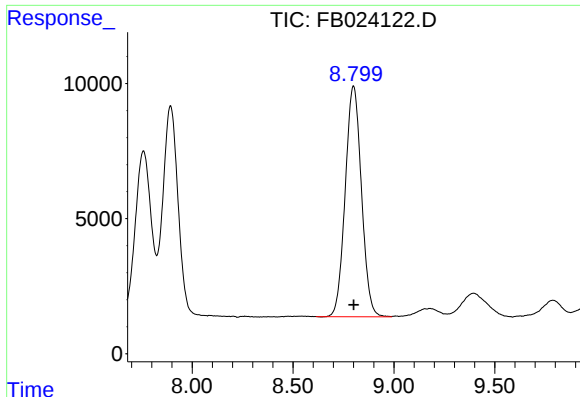


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 476828
Conc: 19.03 ng/ml

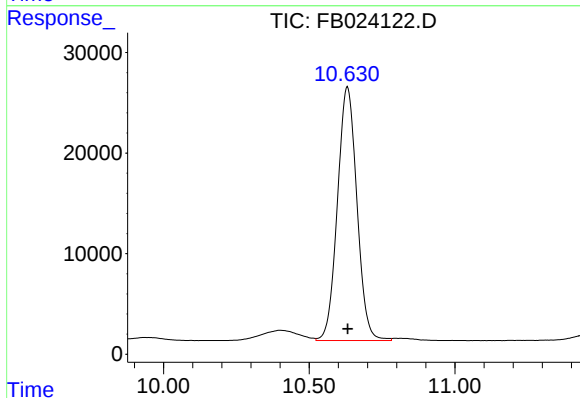


#6 Toluene

R.T.: 10.631 min
Delta R.T.: 0.000 min
Response: 1172495
Conc: 29.83 ng/ml

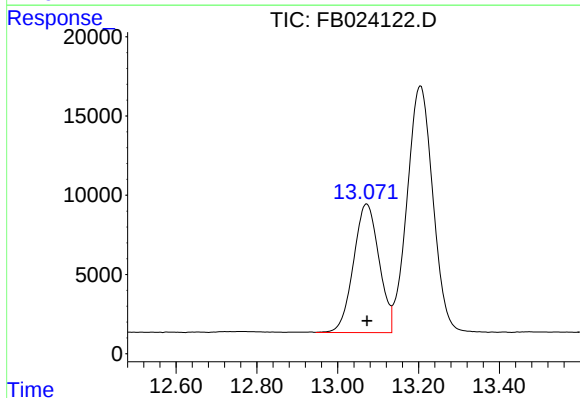


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 355772
Conc: 9.76 ng/ml

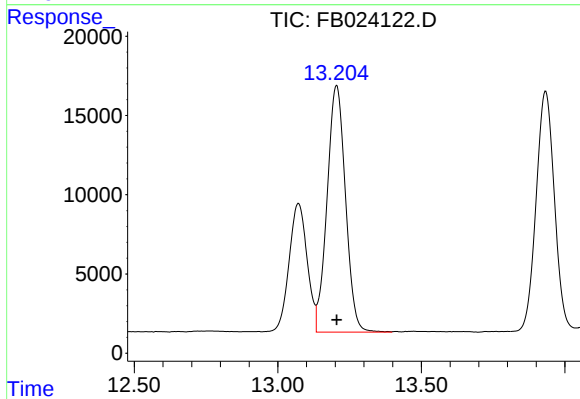


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 692224
Conc: 19.77 ng/ml

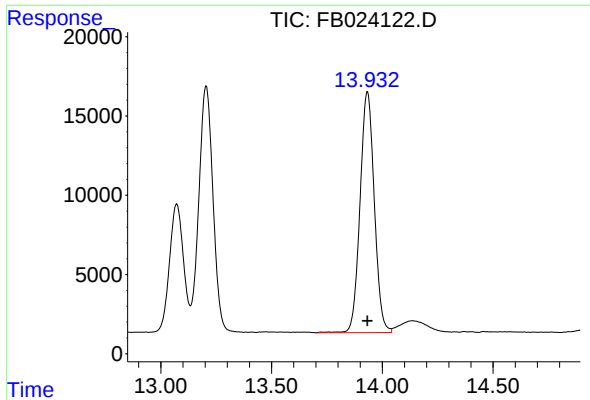

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 680257
Conc: 19.96 ng/ml

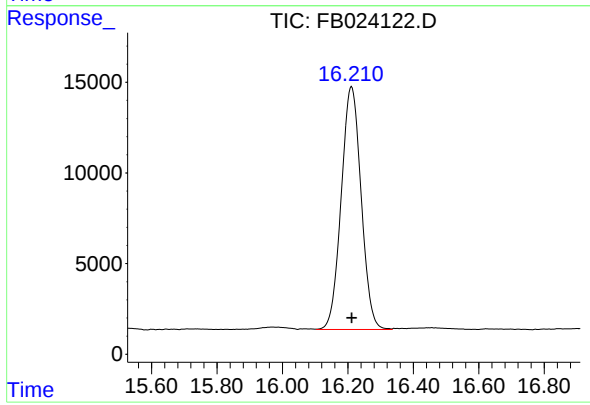

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 565348
Conc: 19.91 ng/ml