

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB041023\  
 Data File : FB029609.D  
 Signal(s) : FID2B.CH  
 Acq On : 10 Apr 2023 12:05  
 Operator : YP/AJ  
 Sample : 02262-07  
 Misc : 8.08G/5.00 ML DI WATER  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 FID\_B  
 ClientSampleId :

Integration File: Calibration.e  
 Quant Time: Apr 10 18:06:51 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB032323.M  
 Quant Title :  
 QLast Update : Thu Mar 23 11:44:29 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 5 g/ml  
 Signal Phase : RTX-502.2  
 Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.791  | 216066   | 15.159 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.615 | 4970     | 0.225 ng/ml  |
| 8) t m-Xylene                | 13.183 | 7366     | 0.360 ng/ml  |
| 9) t O-Xylene                | 13.912 | 7399     | 0.373 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.188 | 20229    | 1.060 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB041023\  
Data File : FB029609.D  
Signal(s) : FID2B.CH  
Acq On : 10 Apr 2023 12:05  
Operator : YP/AJ  
Sample : 02262-07  
Misc : 8.08G/5.00 ML DI WATER  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
FID\_B  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Apr 10 18:06:51 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB032323.M  
Quant Title :  
QLast Update : Thu Mar 23 11:44:29 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

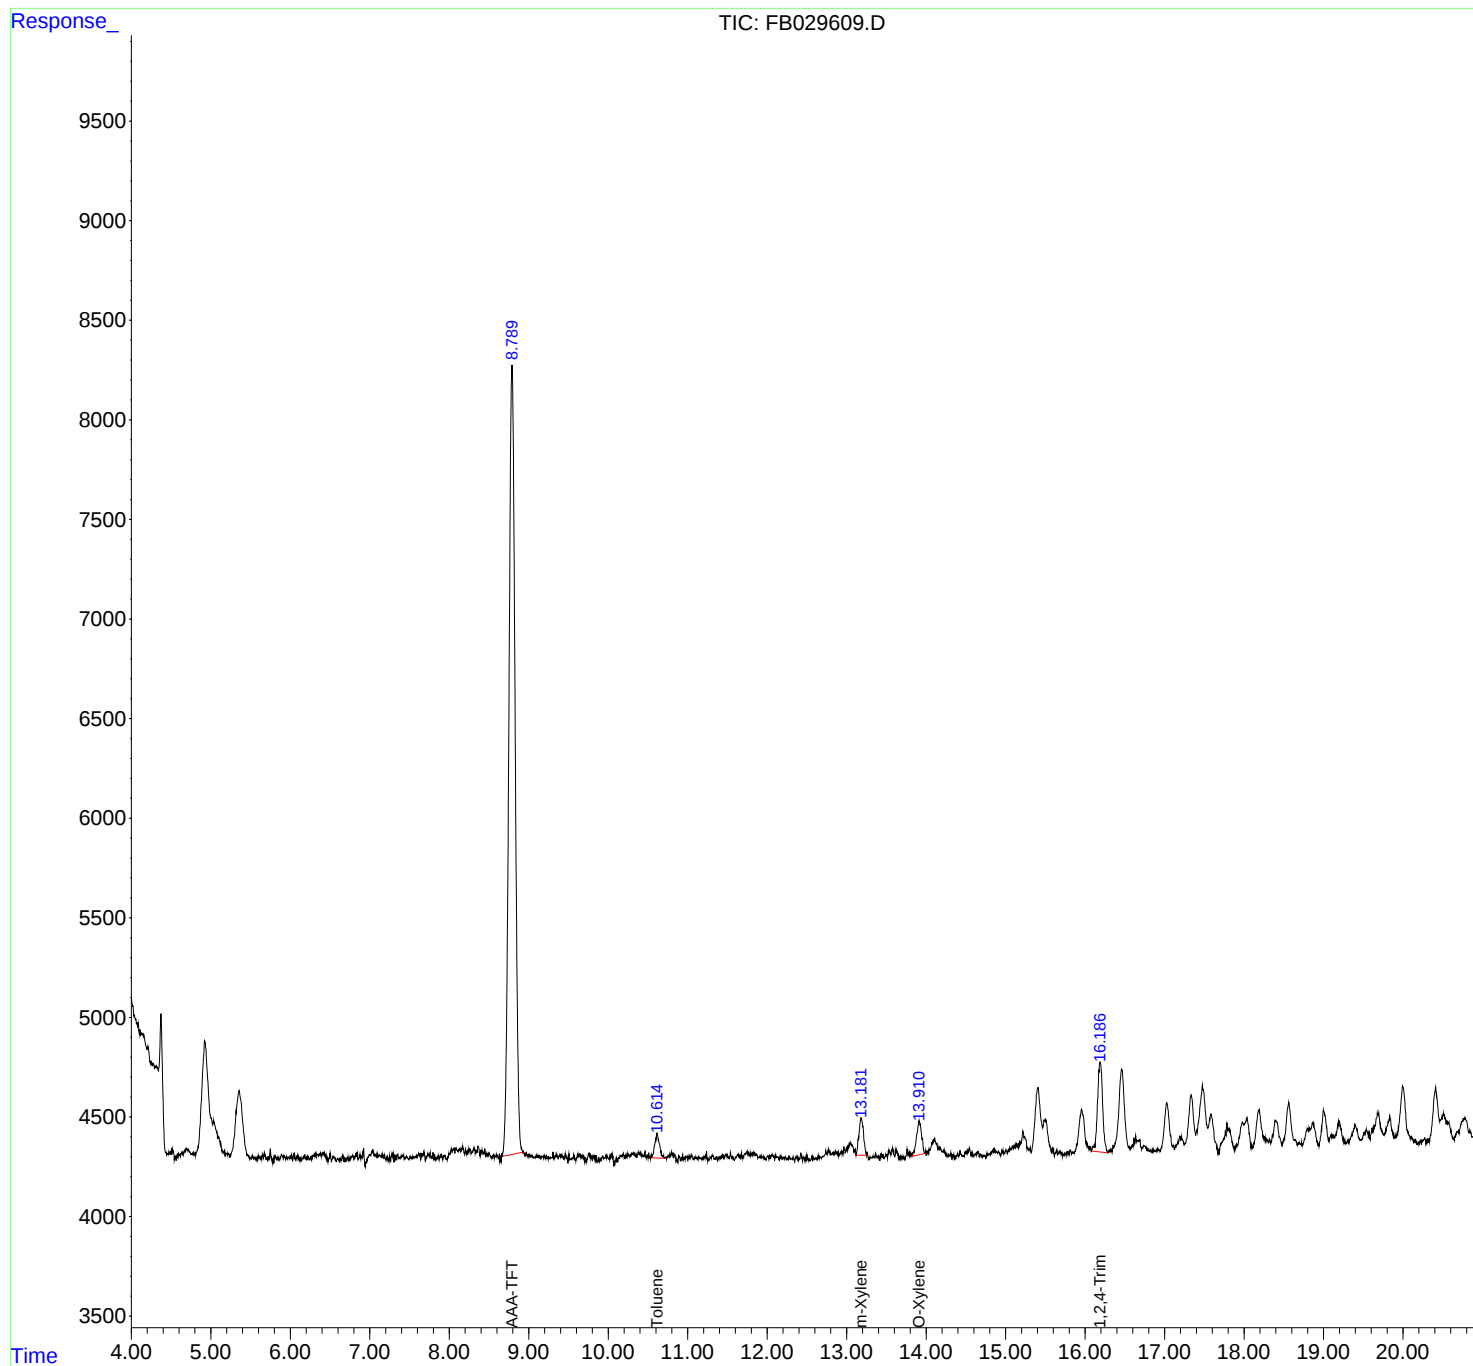


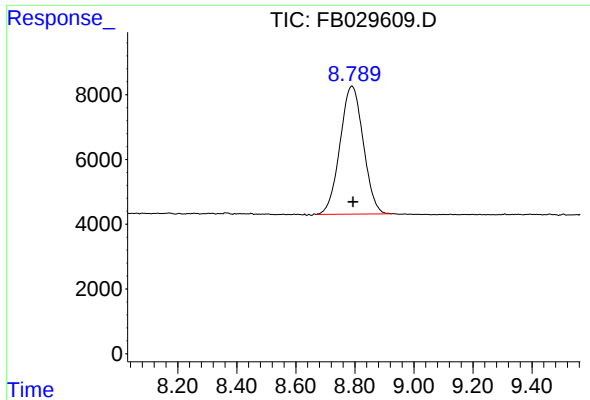

#5 AAA-TFT


R.T.: 8.791 min  
Delta R.T.: -0.003 min  
Response: 216066  
Conc: 15.16 ng/ml

Instrument :  
FID\_B  
ClientSampleId :

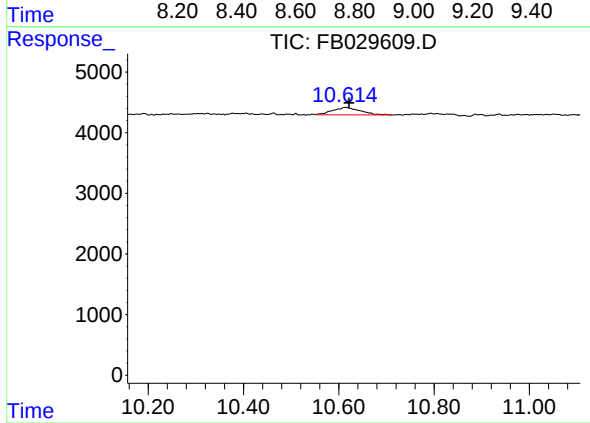


#6 Toluene

R.T.: 10.615 min  
Delta R.T.: -0.006 min  
Response: 4970  
Conc: 0.23 ng/ml

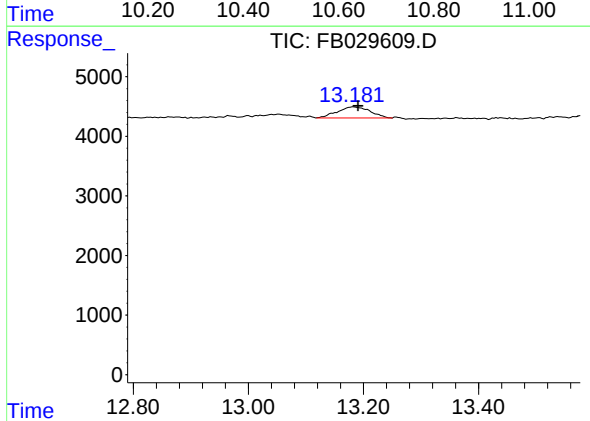


#8 m-Xylene

R.T.: 13.183 min  
Delta R.T.: -0.008 min  
Response: 7366  
Conc: 0.36 ng/ml

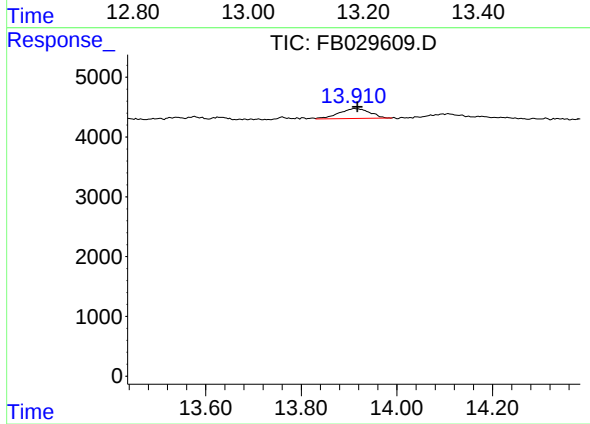

#9 O-Xylene

R.T.: 13.912 min  
Delta R.T.: -0.006 min  
Response: 7399  
Conc: 0.37 ng/ml

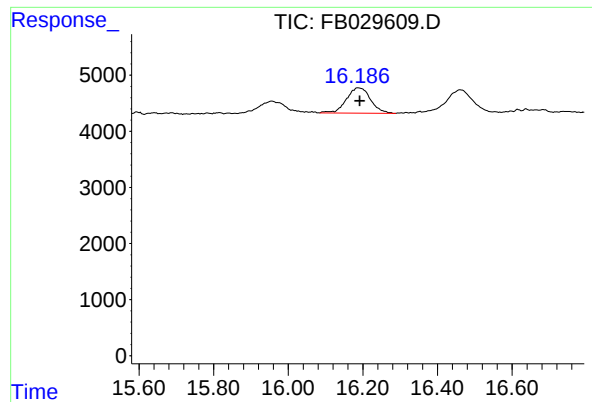

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min  
Delta R.T.: -0.004 min  
Response: 20229  
Conc: 1.06 ng/ml

Instrument :

FID\_B

ClientSampleId :