

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041023\
 Data File : FB029610.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2023 12:43
 Operator : YP/AJ
 Sample : 02262-11
 Misc : 7.65G/5.00 ML DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 10 18:06:58 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	172875	12.129 ng/ml
Target Compounds			
8) t m-Xylene	13.193	9570	0.468 ng/ml
9) t O-Xylene	13.914	8720	0.440 ng/ml
10) t 1,2,4-Trimethylbenzene	16.187	21989	1.152 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041023\
Data File : FB029610.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2023 12:43
Operator : YP/AJ
Sample : 02262-11
Misc : 7.65G/5.00 ML DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 10 18:06:58 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

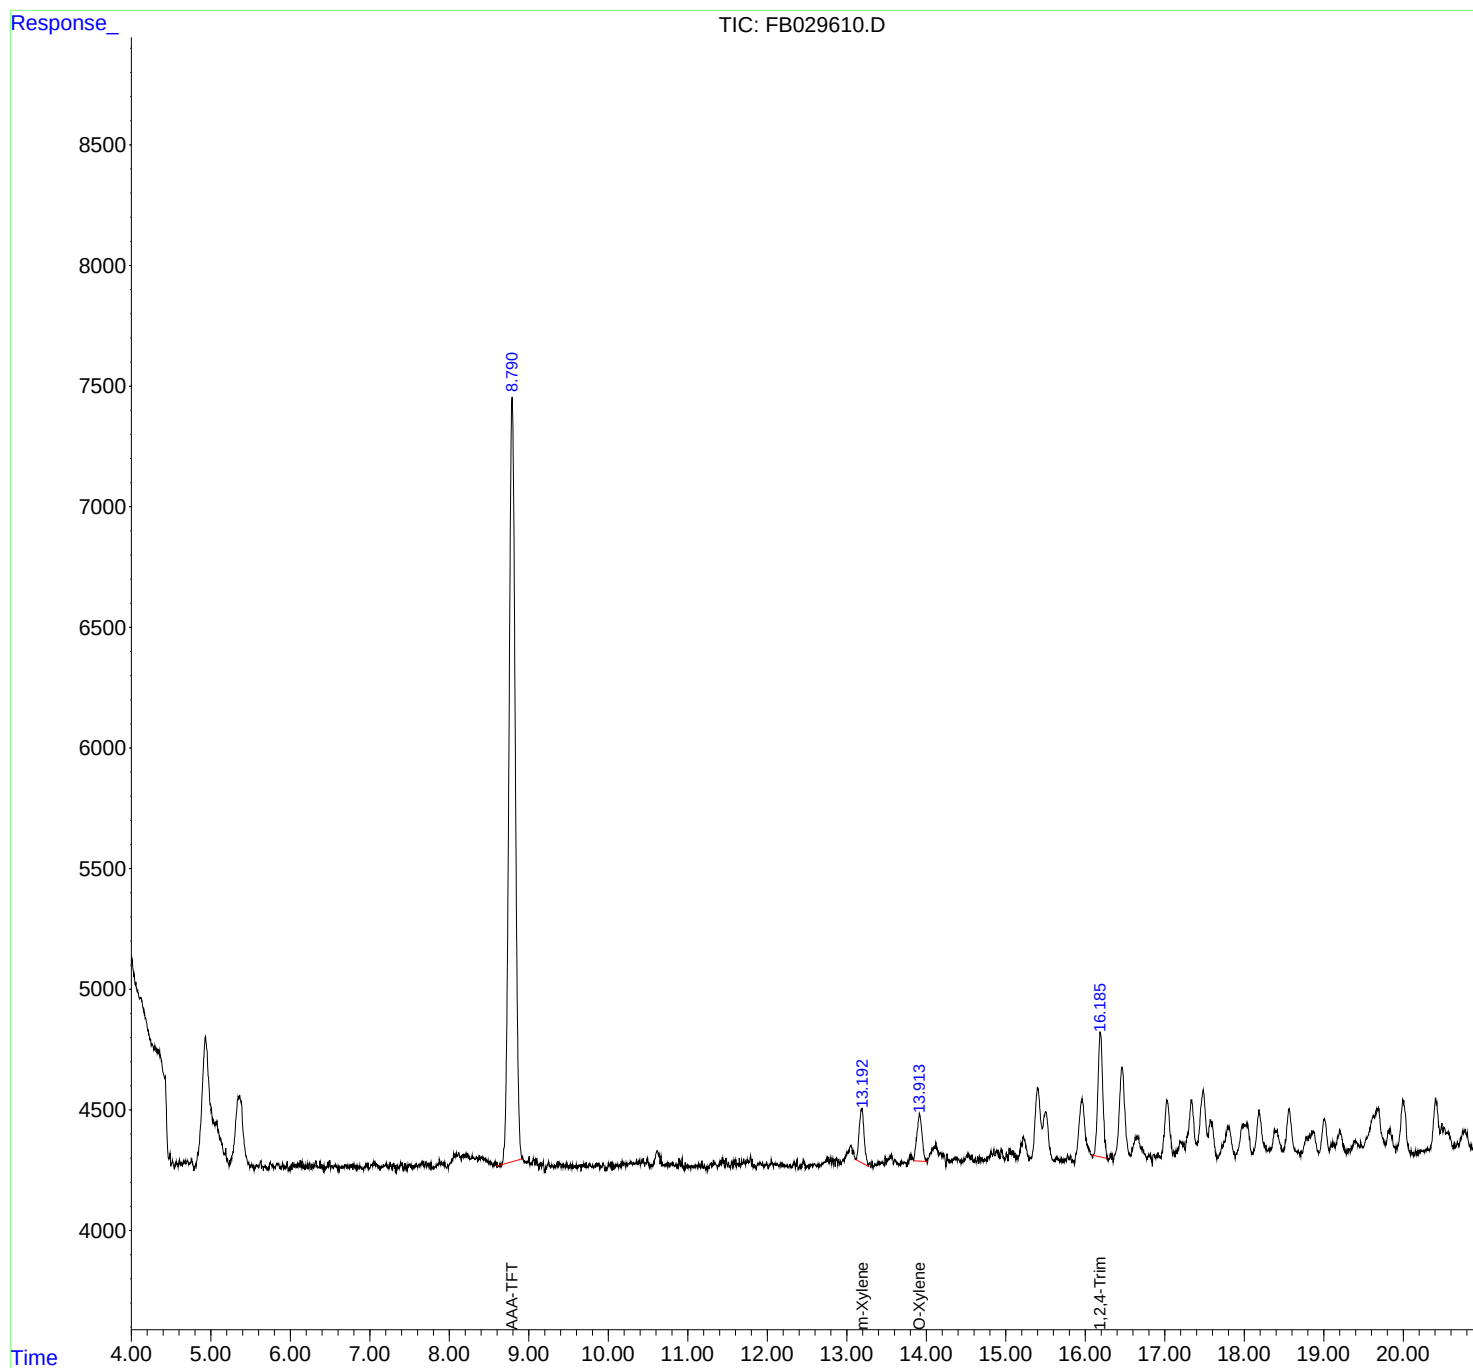


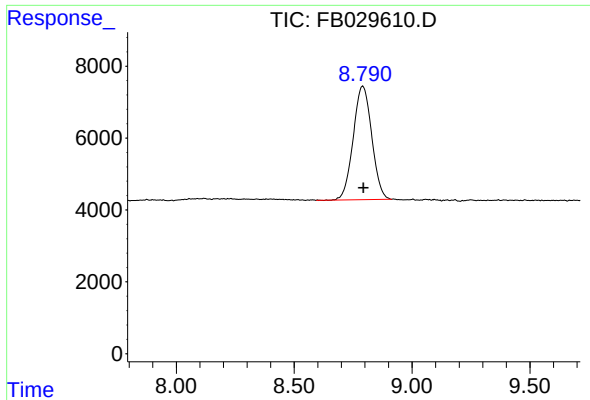

#5 AAA-TFT


R.T.: 8.791 min
Delta R.T.: -0.003 min
Response: 172875
Conc: 12.13 ng/ml

Instrument :
FID_B
ClientSampleId :

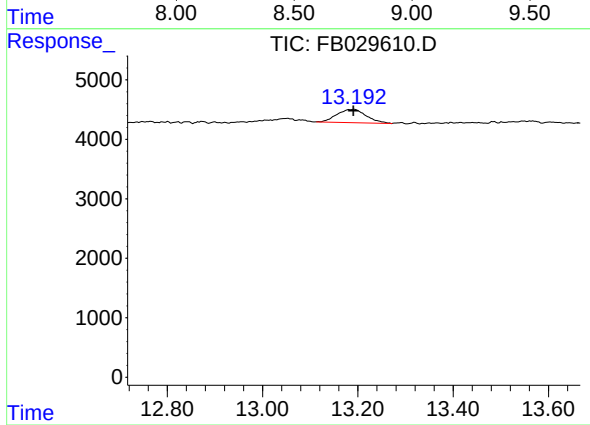


#8 m-Xylene

R.T.: 13.193 min
Delta R.T.: 0.003 min
Response: 9570
Conc: 0.47 ng/ml

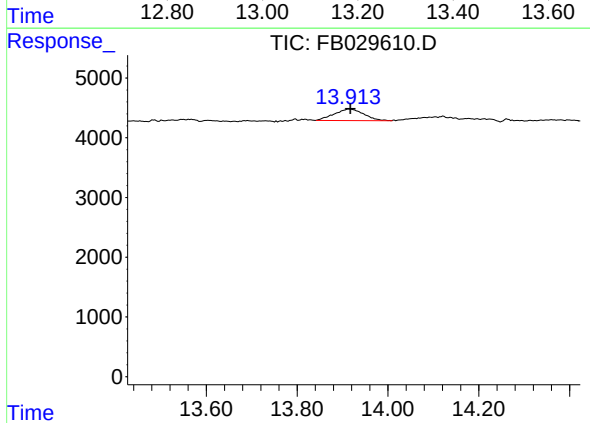

#9 o-Xylene

R.T.: 13.914 min
Delta R.T.: -0.003 min
Response: 8720
Conc: 0.44 ng/ml

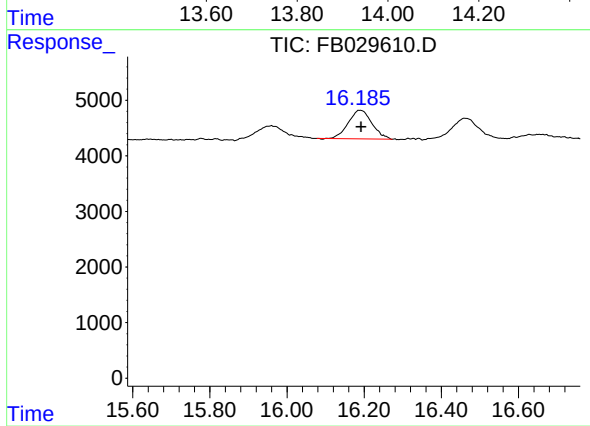

#10 1,2,4-Trimethylbenzene

R.T.: 16.187 min
Delta R.T.: -0.005 min
Response: 21989
Conc: 1.15 ng/ml