

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041023\
 Data File : FB029611.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2023 13:21
 Operator : YP/AJ
 Sample : BSF0410S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0410S2

Integration File: SAMPLE.e
 Quant Time: Apr 10 18:07:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	309388	21.706 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	498155	29.672 ng/ml
2) t 2,2,4-Trimethylpentane	7.422	570739	31.002 ng/ml
3) t n-Heptane	7.751	192907	9.903 ng/ml
4) t Benzene	7.886	240559	10.647 ng/ml
6) t Toluene	10.619	691397	31.363 ng/ml
7) t Ethylbenzene	13.056	218079	10.550 ng/ml
8) t m-Xylene	13.188	431027	21.065 ng/ml
9) t O-Xylene	13.915	420105	21.206 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	392761	20.573 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041023\
Data File : FB029611.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2023 13:21
Operator : YP/AJ
Sample : BSF0410S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0410S2

Integration File: SAMPLE.e
Quant Time: Apr 10 18:07:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

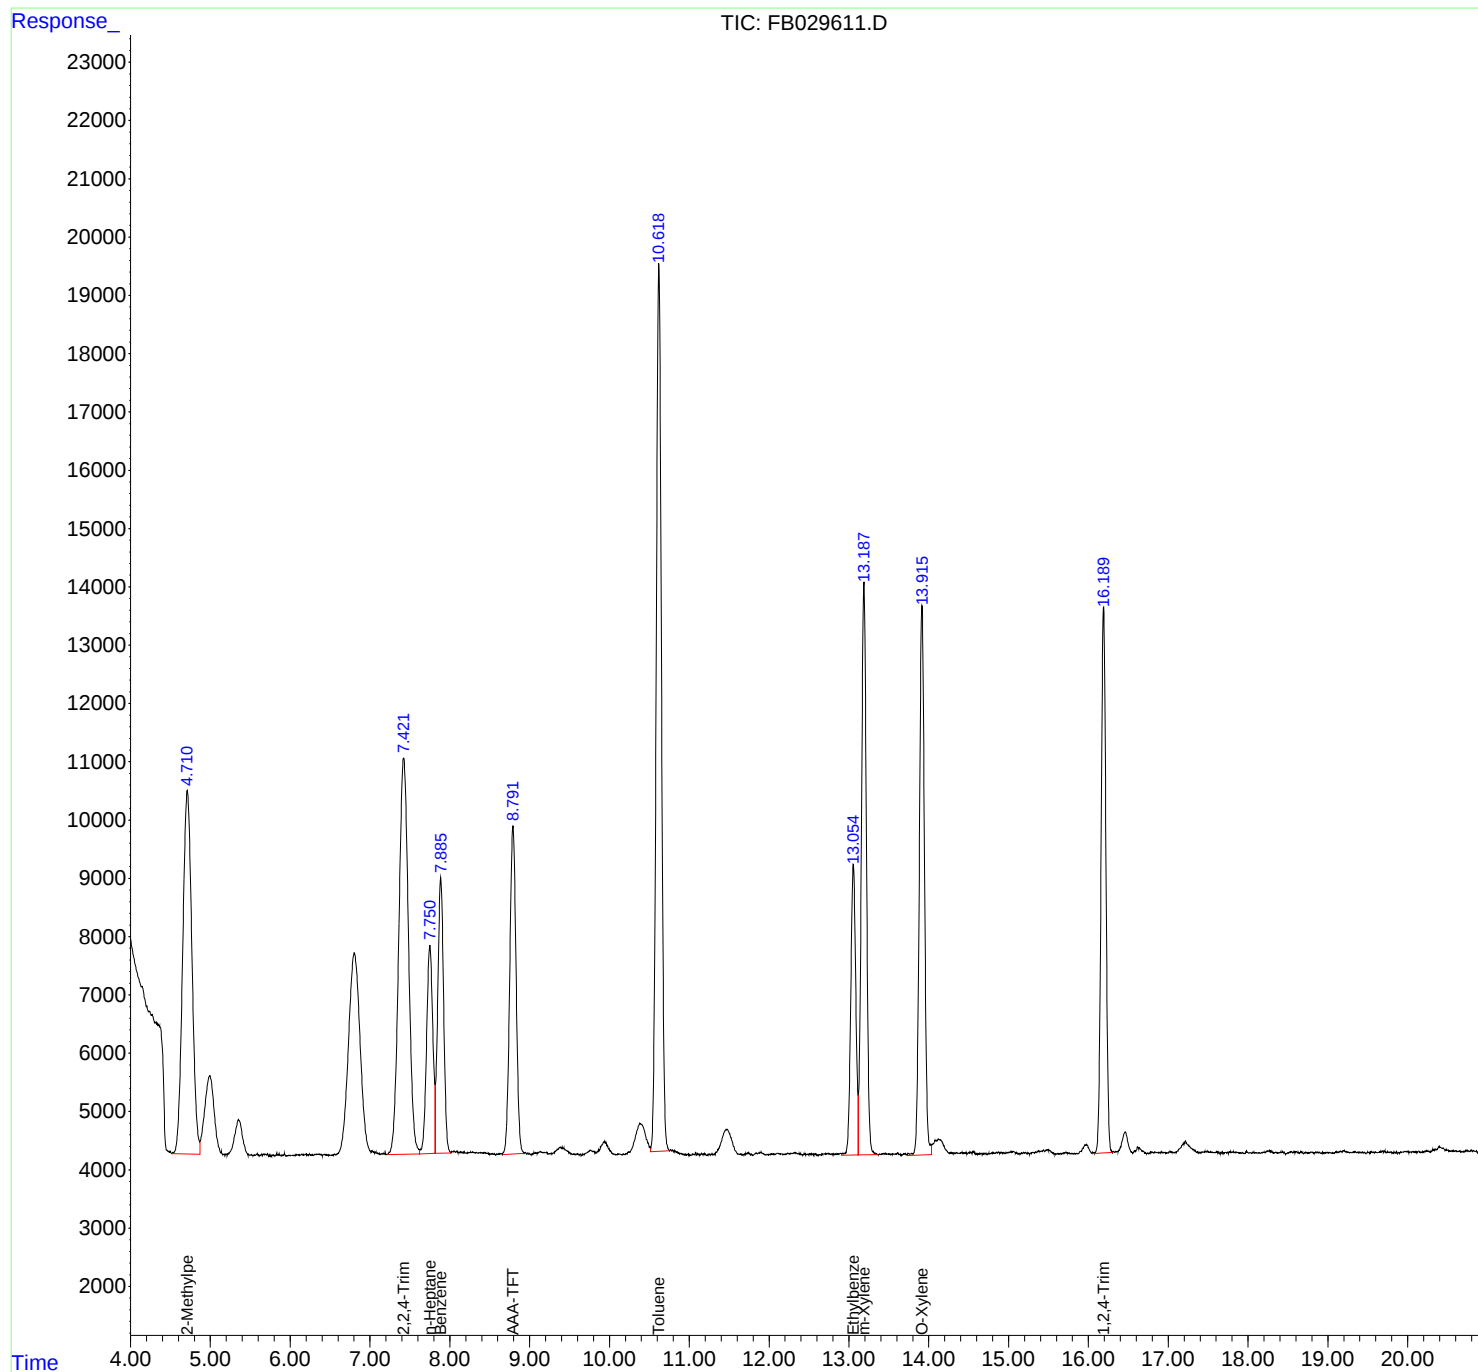


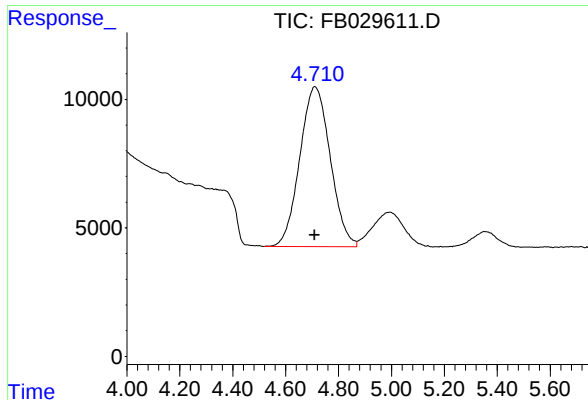

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.001 min
Response: 498155
Conc: 29.67 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0410S2

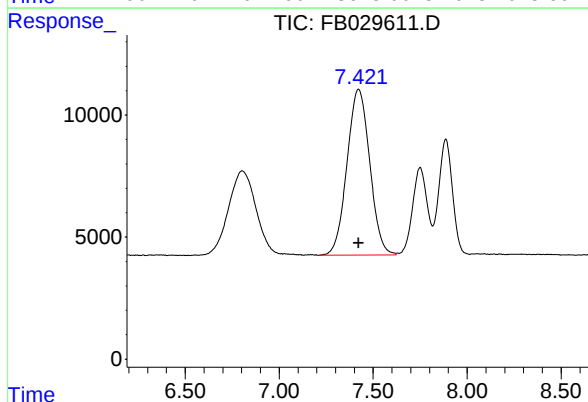


#2 2,2,4-Trimethylpentane

R.T.: 7.422 min
Delta R.T.: 0.000 min
Response: 570739
Conc: 31.00 ng/ml

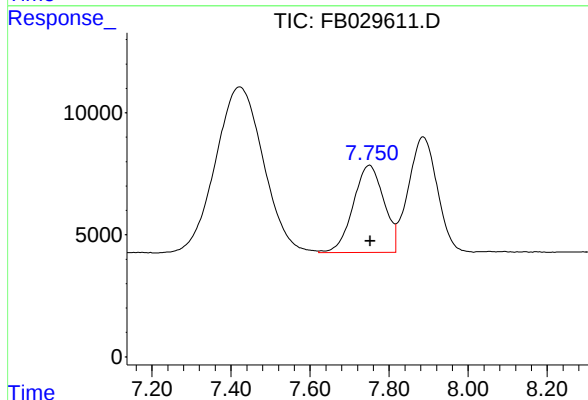


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.002 min
Response: 192907
Conc: 9.90 ng/ml

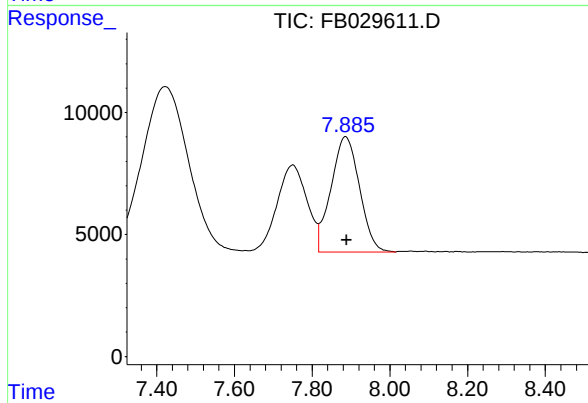

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 240559
Conc: 10.65 ng/ml

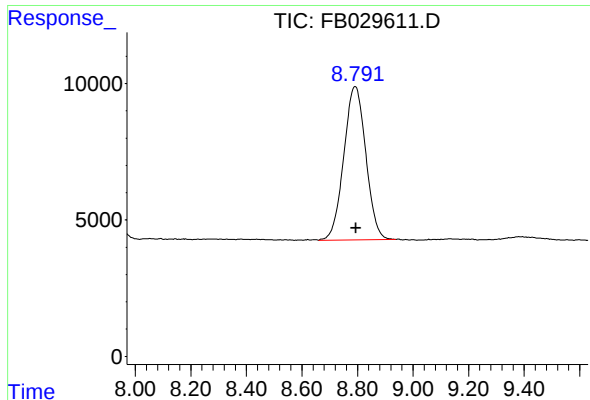

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.002 min
Response: 309388
Conc: 21.71 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0410S2

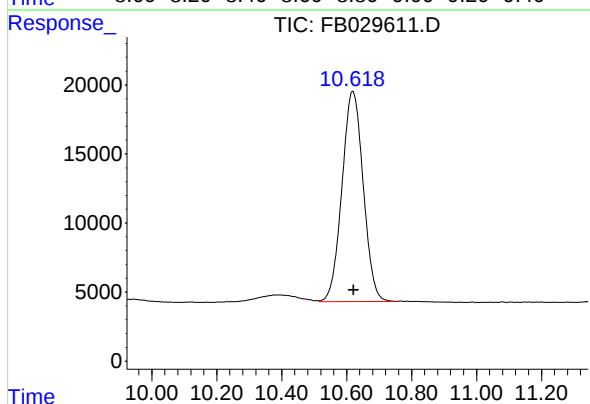


#6 Toluene

R.T.: 10.619 min
Delta R.T.: -0.002 min
Response: 691397
Conc: 31.36 ng/ml

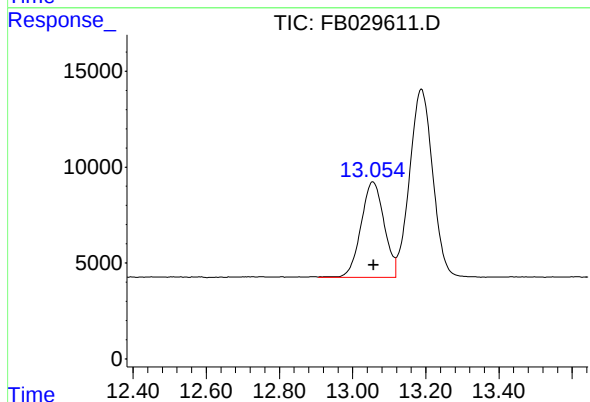


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 218079
Conc: 10.55 ng/ml

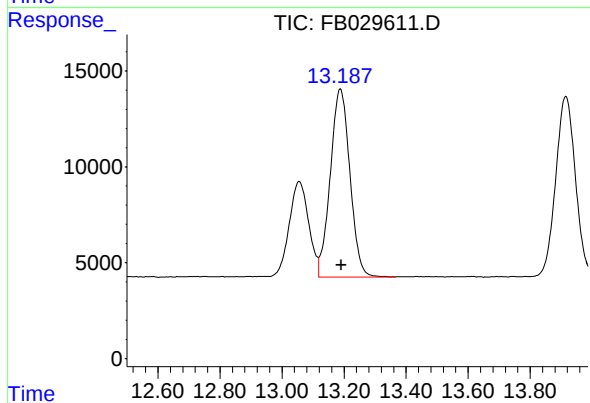

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.002 min
Response: 431027
Conc: 21.07 ng/ml

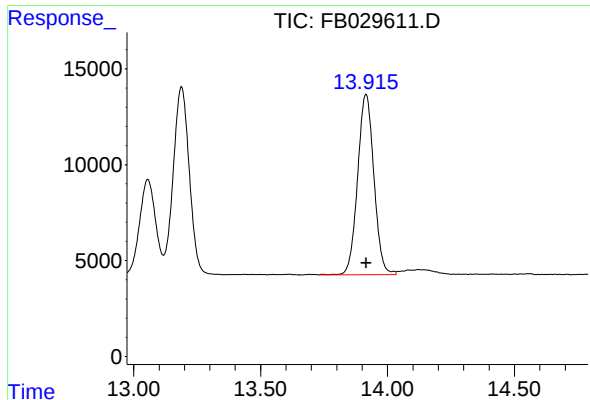

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.002 min
Response: 420105
Conc: 21.21 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0410S2

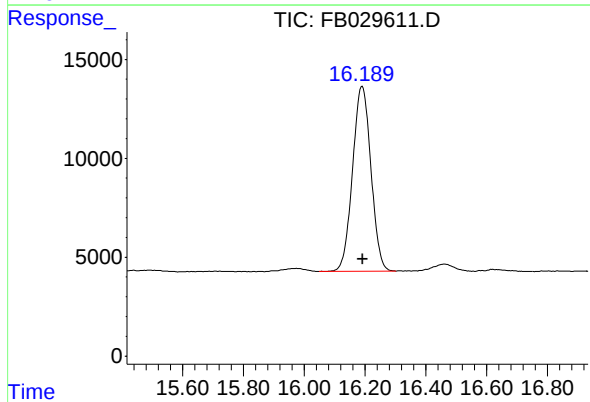

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.001 min
Response: 392761
Conc: 20.57 ng/ml