

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041024\
 Data File : FB030672.D
 Signal(s) : FID2B.CH
 Acq On : 10 Apr 2024 10:21
 Operator : YP/AJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 10 10:21:44 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
 Quant Title :
 QLast Update : Wed Apr 10 10:21:26 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.786	266061	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	479493	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.411	510633	30.000 ng/ml
3) t n-Heptane	7.745	164220	10.000 ng/ml
4) t Benzene	7.882	195971	10.000 ng/ml
6) t Toluene	10.614	573448	30.000 ng/ml
7) t Ethylbenzene	13.050	182172	10.000 ng/ml
8) t m-Xylene	13.183	367422	20.000 ng/ml
9) t O-Xylene	13.910	362287	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.185	374548	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041024\
Data File : FB030672.D
Signal(s) : FID2B.CH
Acq On : 10 Apr 2024 10:21
Operator : YP/AJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 10 10:21:44 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB041024.M
Quant Title :
QLast Update : Wed Apr 10 10:21:26 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

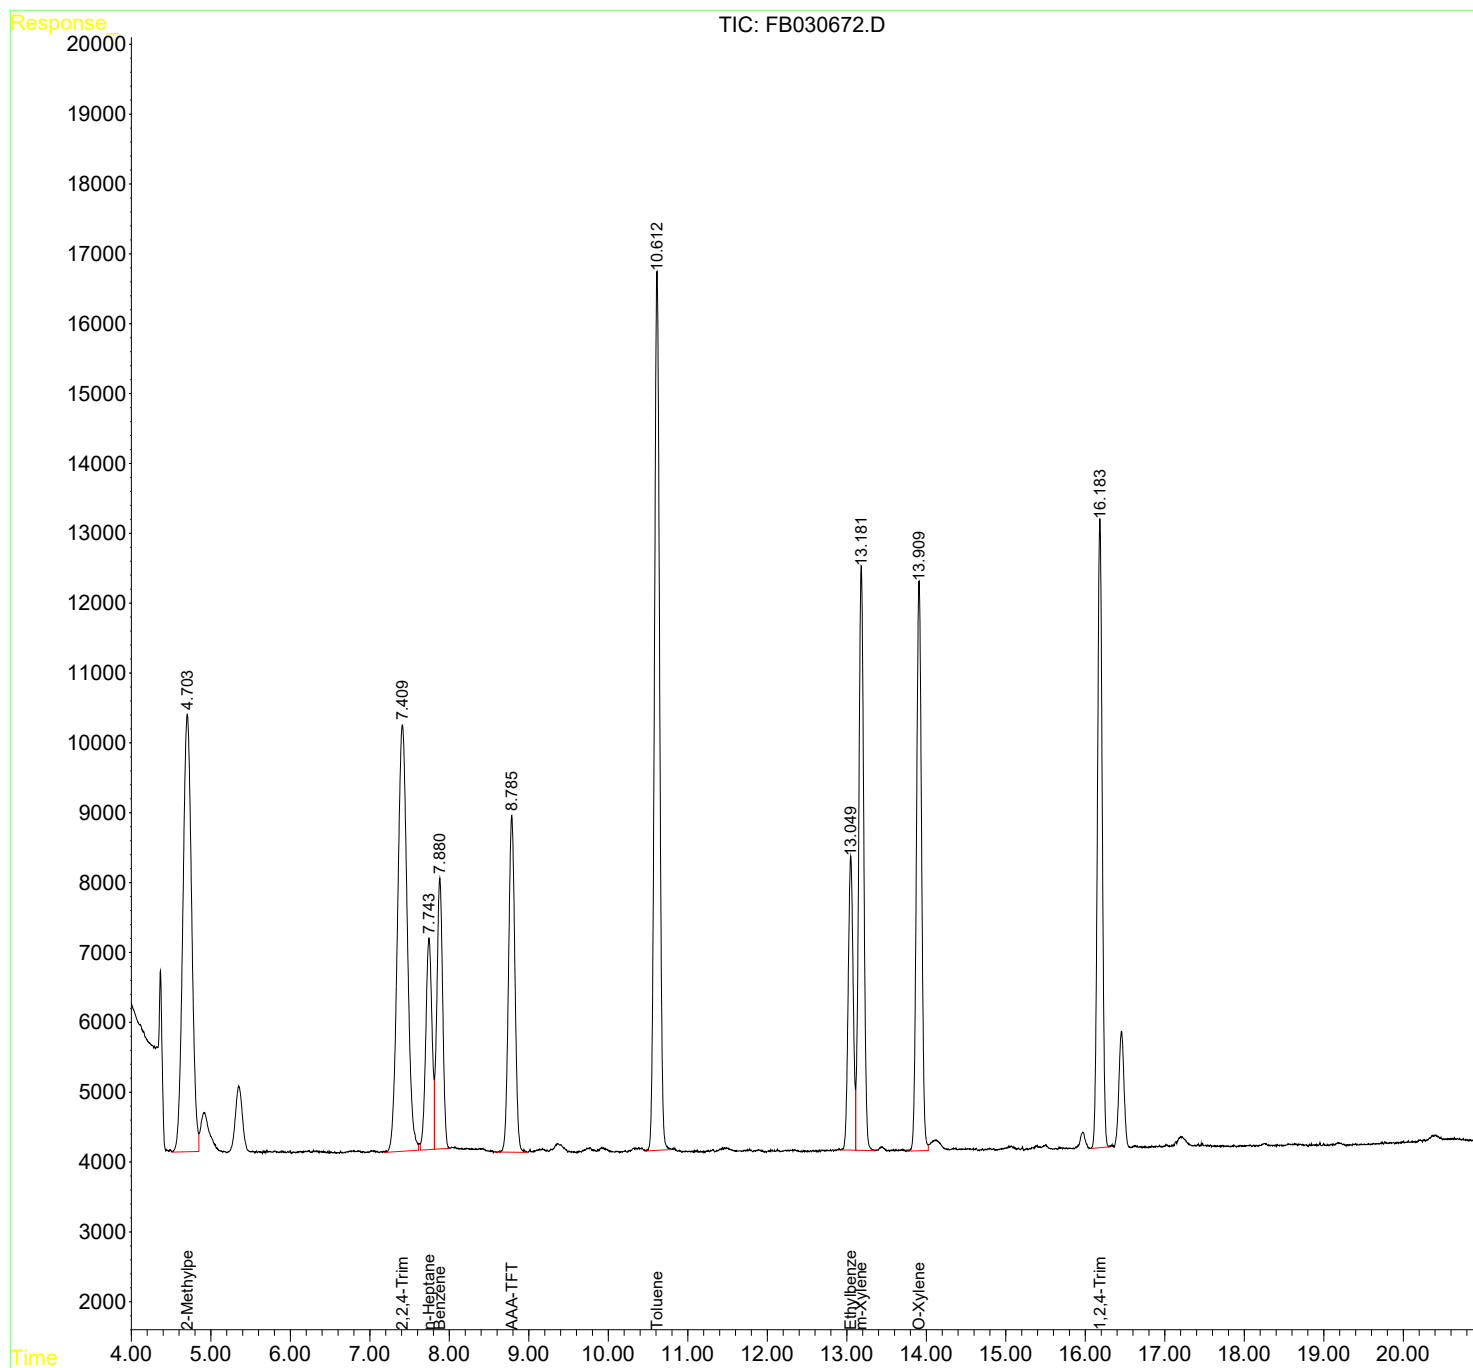


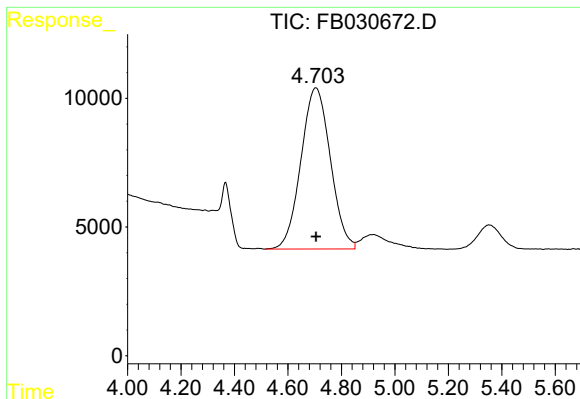

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: 0.000 min
Response: 479493
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :

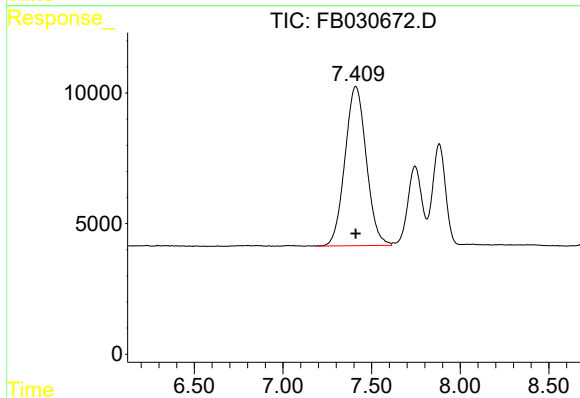


#2 2,2,4-Trimethylpentane

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 510633
Conc: 30.00 ng/ml

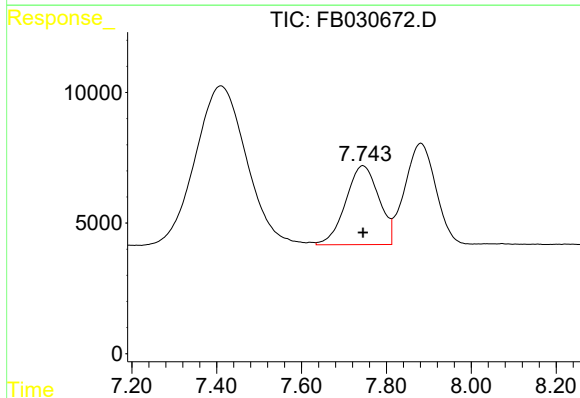


#3 n-Heptane

R.T.: 7.745 min
Delta R.T.: 0.000 min
Response: 164220
Conc: 10.00 ng/ml

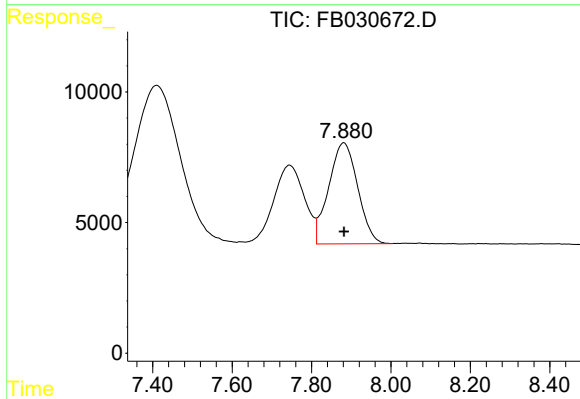

#4 Benzene


R.T.: 7.882 min
Delta R.T.: 0.000 min
Response: 195971
Conc: 10.00 ng/ml

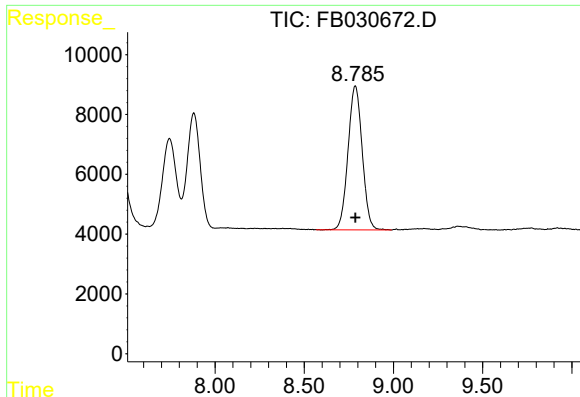

#5 AAA-TFT


R.T.: 8.786 min
Delta R.T.: 0.000 min
Response: 266061
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

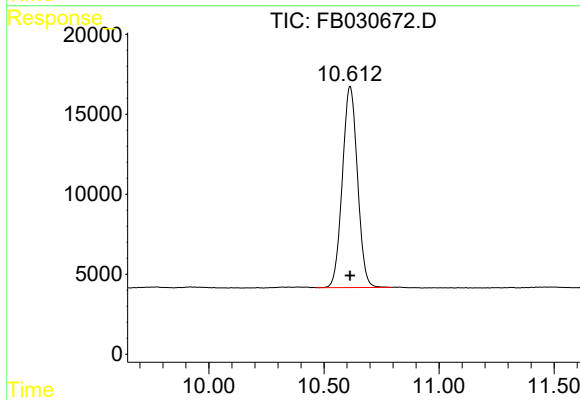


#6 Toluene

R.T.: 10.614 min
Delta R.T.: 0.000 min
Response: 573448
Conc: 30.00 ng/ml

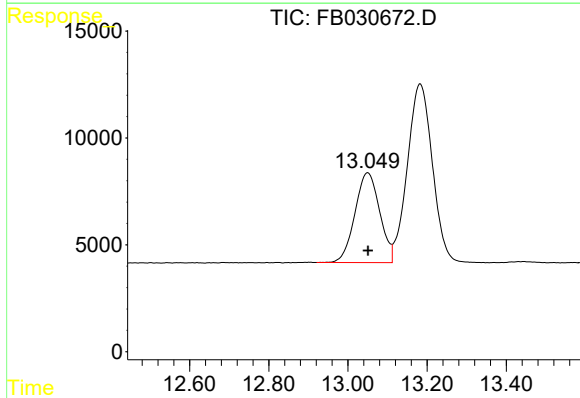


#7 Ethylbenzene

R.T.: 13.050 min
Delta R.T.: 0.000 min
Response: 182172
Conc: 10.00 ng/ml

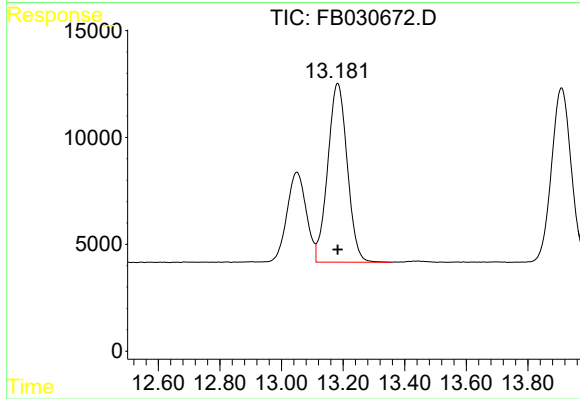

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: 0.000 min
Response: 367422
Conc: 20.00 ng/ml

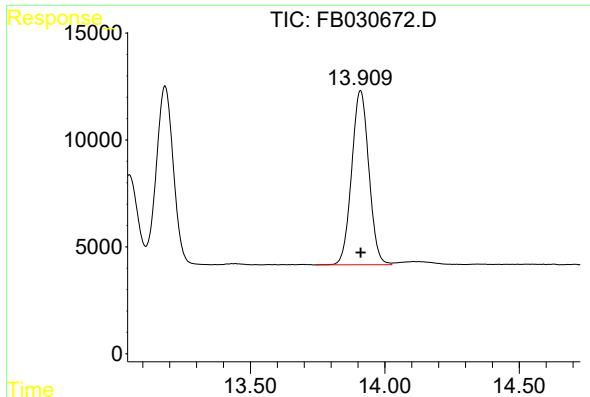

#9 O-Xylene

R.T.: 13.910 min
Delta R.T.: 0.000 min
Response: 362287
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :

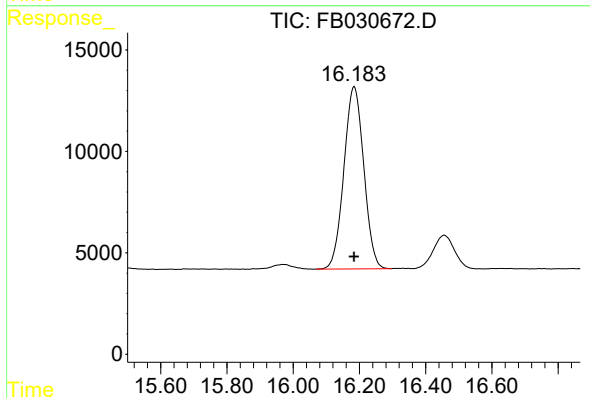

#10 1,2,4-Trimethylbenzene

R.T.: 16.185 min
Delta R.T.: 0.000 min
Response: 374548
Conc: 20.00 ng/ml