

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041119\
 Data File : FB020637.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2019 10:38
 Operator : MJ/SJ
 Sample : BSF0411S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 12 07:25:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	428313	23.222 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.864	1207112	34.289 ng/ml
2) t 2,2,4-Trimethylpentane	7.620	1067836	35.817 ng/ml
3) t n-Heptane	7.950	445971	11.361 ng/ml
4) t Benzene	8.087	458232	11.156 ng/ml
6) t Toluene	10.837	1007425	33.341 ng/ml
7) t Ethylbenzene	13.287	298046	11.651 ng/ml
8) t m-Xylene	13.420	619658	23.446 ng/ml
9) t O-Xylene	14.151	637785	23.559 ng/ml
10) t 1,2,4-Trimethylbenzene	16.436	626202	23.968 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041119\
Data File : FB020637.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2019 10:38
Operator : MJ/SJ
Sample : BSF0411S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 12 07:25:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

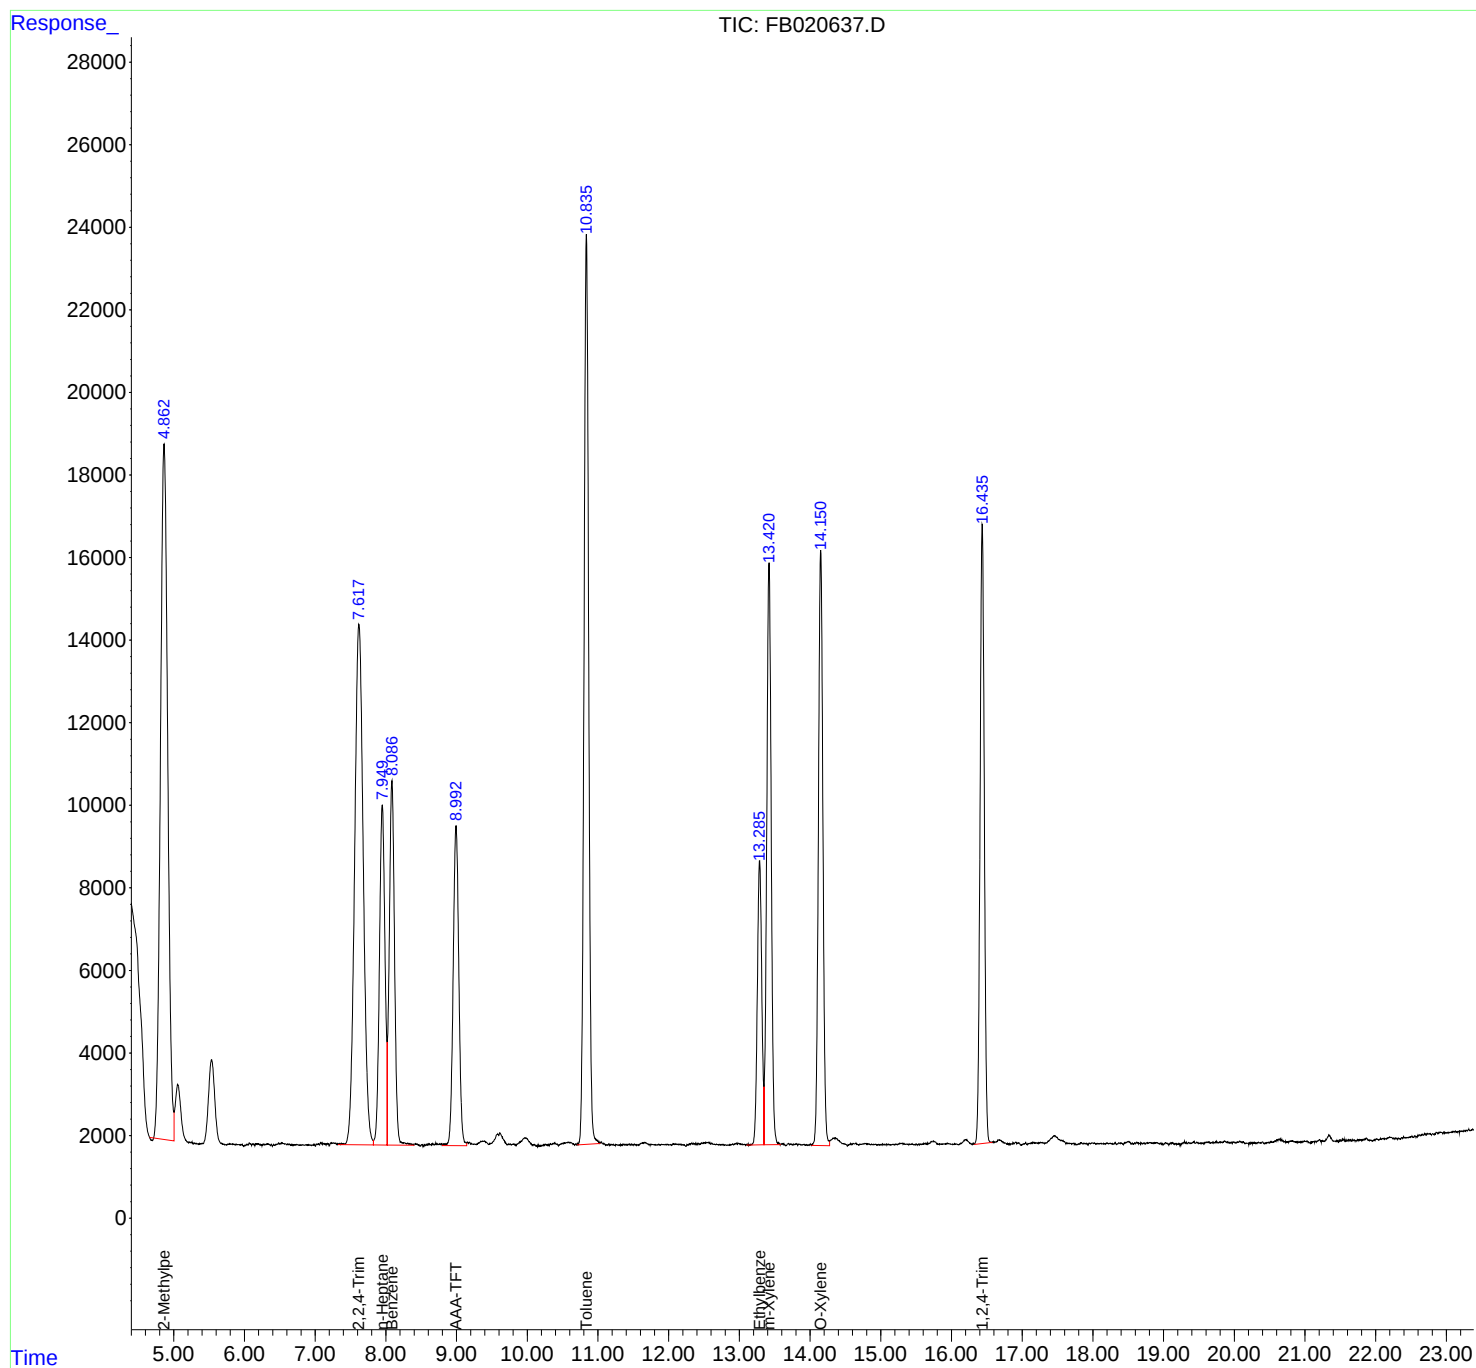

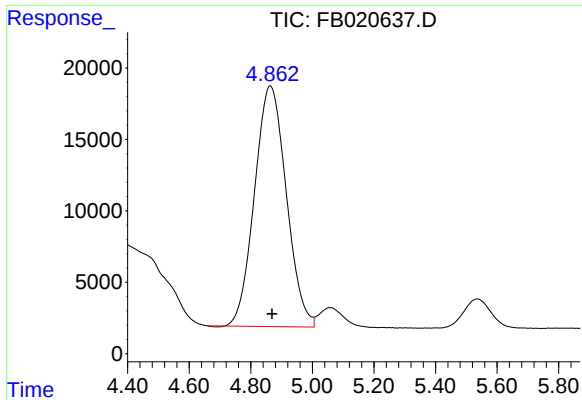


#1 2-Methylpentane

R.T.: 4.864 min
Delta R.T.: -0.005 min
Response: 1207112
Conc: 34.29 ng/ml

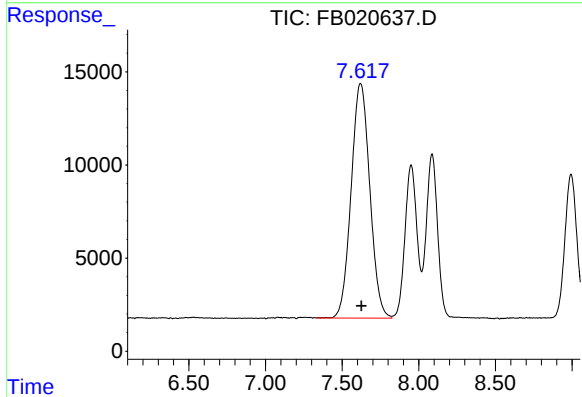


#2 2,2,4-Trimethylpentane

R.T.: 7.620 min
Delta R.T.: -0.007 min
Response: 1067836
Conc: 35.82 ng/ml

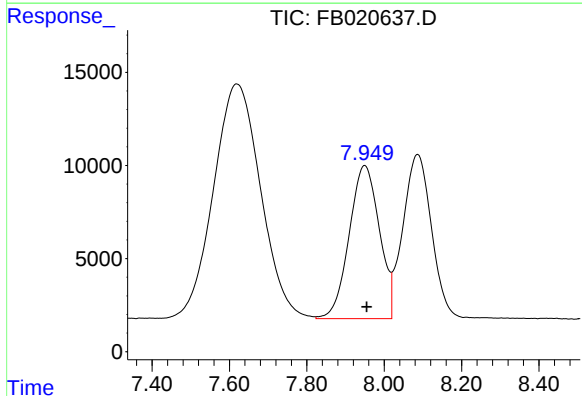


#3 n-Heptane

R.T.: 7.950 min
Delta R.T.: -0.005 min
Response: 445971
Conc: 11.36 ng/ml

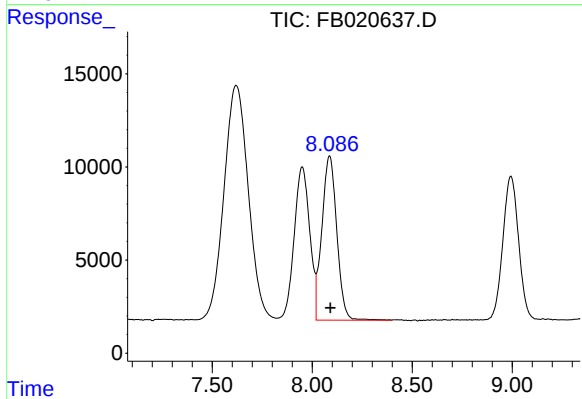


#4 Benzene

R.T.: 8.087 min
Delta R.T.: -0.004 min
Response: 458232
Conc: 11.16 ng/ml

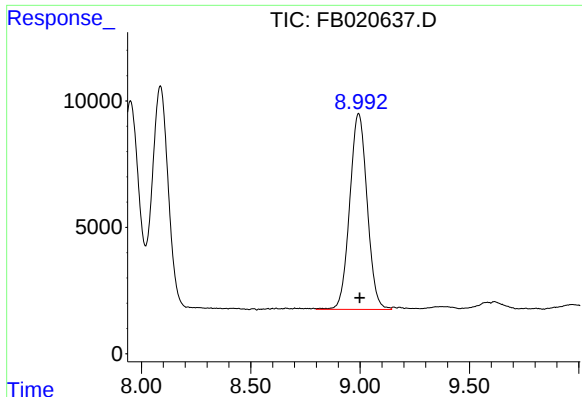


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.005 min
Response: 428313
Conc: 23.22 ng/ml

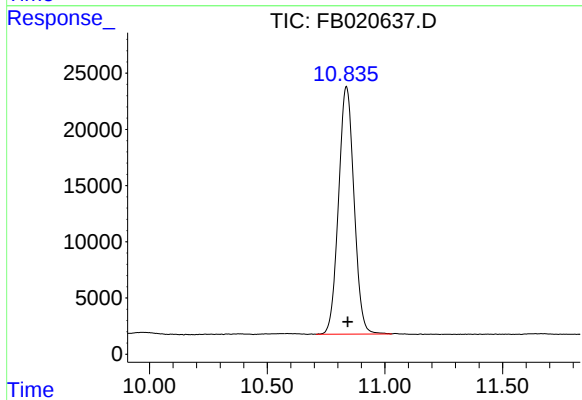


#6 Toluene

R.T.: 10.837 min
Delta R.T.: -0.005 min
Response: 1007425
Conc: 33.34 ng/ml

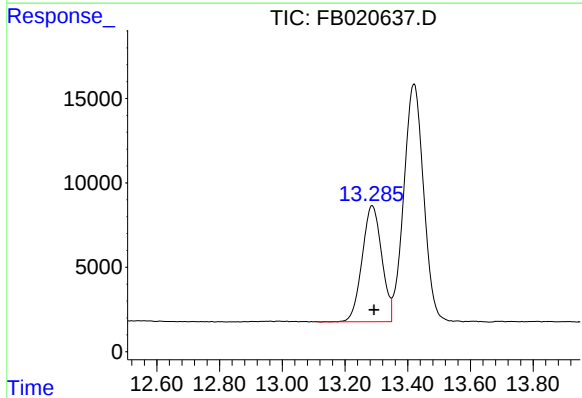


#7 Ethylbenzene

R.T.: 13.287 min
Delta R.T.: -0.005 min
Response: 298046
Conc: 11.65 ng/ml

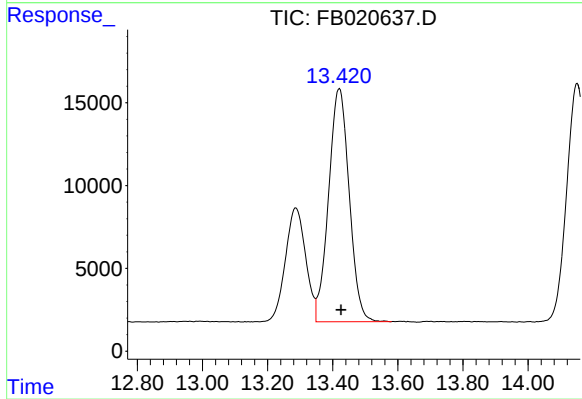


#8 m-Xylene

R.T.: 13.420 min
Delta R.T.: -0.005 min
Response: 619658
Conc: 23.45 ng/ml

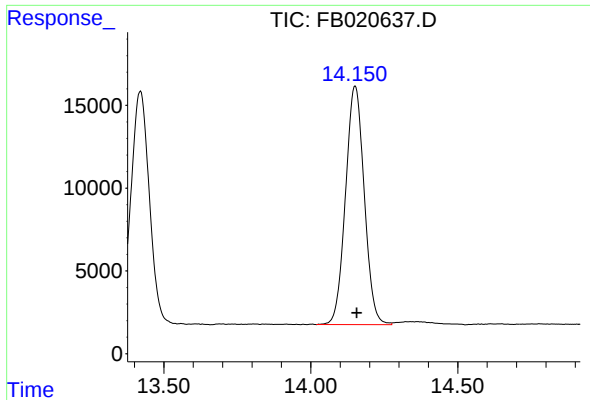

#9 O-Xylene

R.T.: 14.151 min
Delta R.T.: -0.005 min
Response: 637785
Conc: 23.56 ng/ml

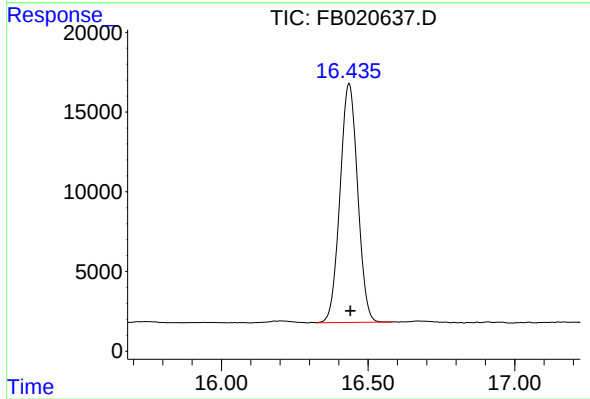

#10 1,2,4-Trimethylbenzene

R.T.: 16.436 min
Delta R.T.: -0.005 min
Response: 626202
Conc: 23.97 ng/ml