

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041119\
 Data File : FB020640.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2019 13:02
 Operator : MJ/SJ
 Sample : K2357-01MSD
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 12 07:25:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.995	412069	22.341 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.867	1068850	30.362 ng/ml
2) t 2,2,4-Trimethylpentane	7.622	909126	30.494 ng/ml
3) t n-Heptane	7.951	376327	9.586 ng/ml
4) t Benzene	8.088	414797	10.099 ng/ml
6) t Toluene	10.838	925320	30.623 ng/ml
7) t Ethylbenzene	13.288	286101	11.184 ng/ml
8) t m-Xylene	13.421	597937	22.624 ng/ml
9) t O-Xylene	14.152	610828	22.563 ng/ml
10) t 1,2,4-Trimethylbenzene	16.437	596048	22.813 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041119\
Data File : FB020640.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2019 13:02
Operator : MJ/SJ
Sample : K2357-01MSD
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 6 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 12 07:25:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

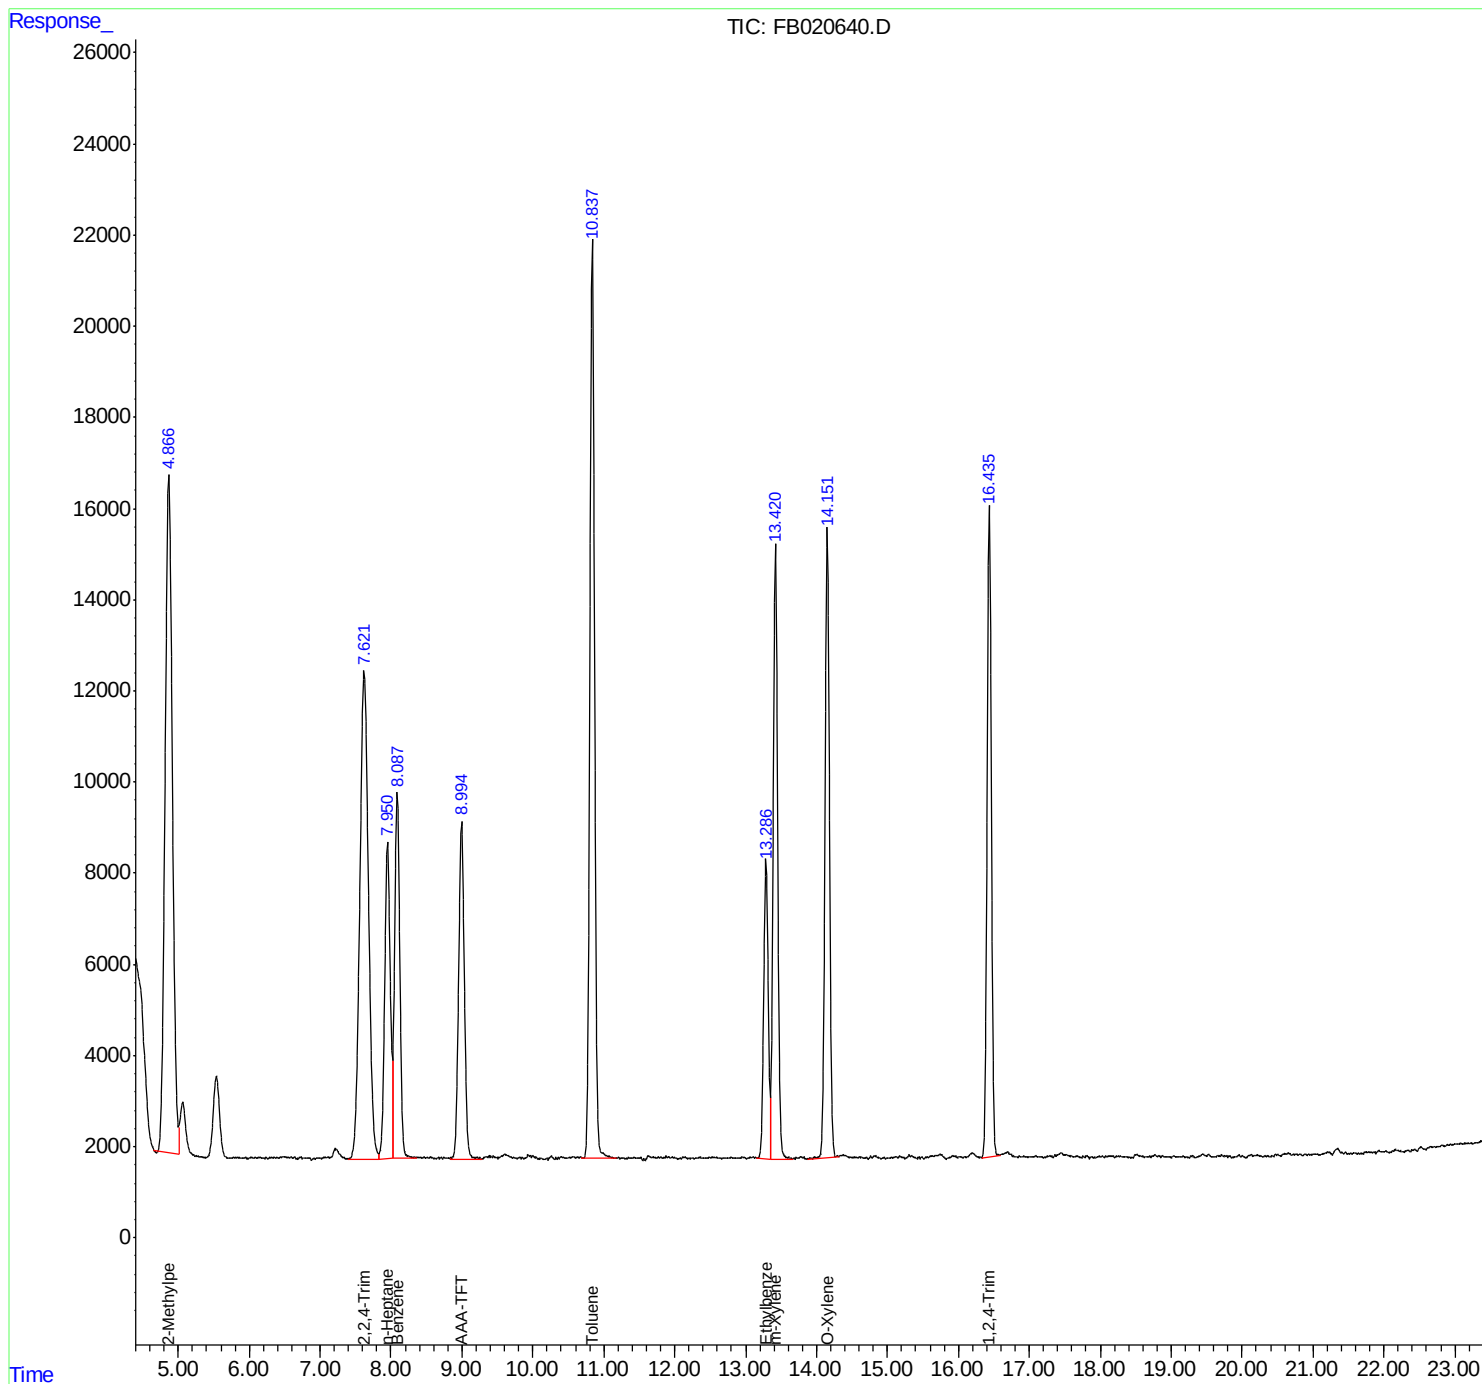

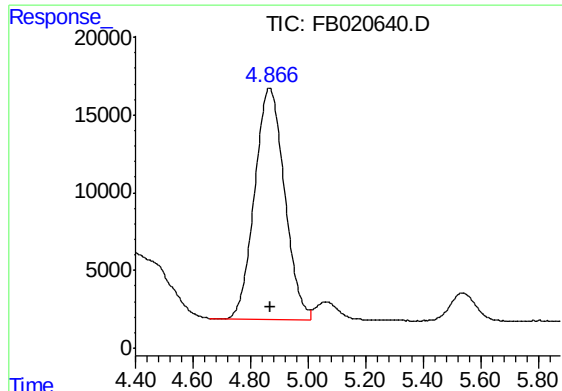


#1 2-Methylpentane

R.T.: 4.867 min
Delta R.T.: -0.002 min
Response: 1068850
Conc: 30.36 ng/ml

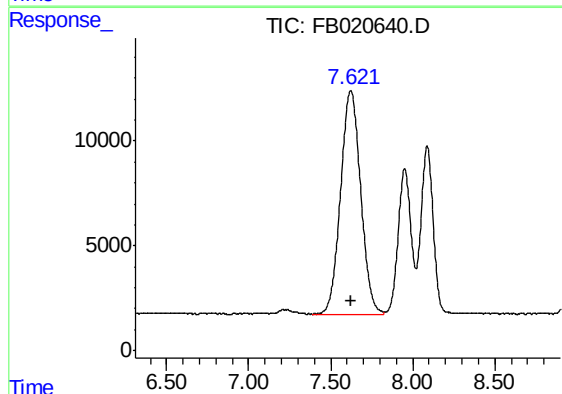


#2 2,2,4-Trimethylpentane

R.T.: 7.622 min
Delta R.T.: -0.005 min
Response: 909126
Conc: 30.49 ng/ml

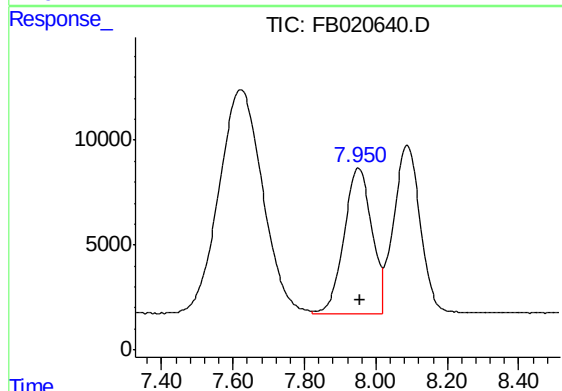


#3 n-Heptane

R.T.: 7.951 min
Delta R.T.: -0.004 min
Response: 376327
Conc: 9.59 ng/ml

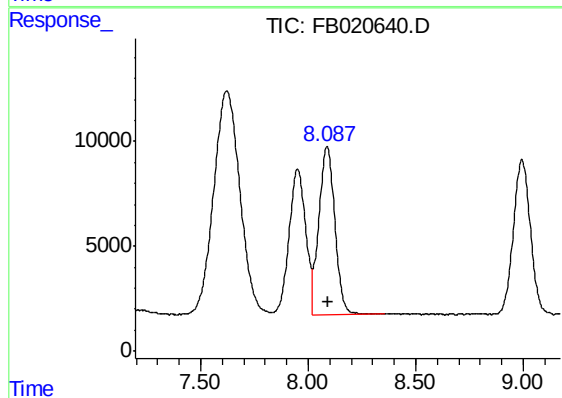


#4 Benzene

R.T.: 8.088 min
Delta R.T.: -0.003 min
Response: 414797
Conc: 10.10 ng/ml

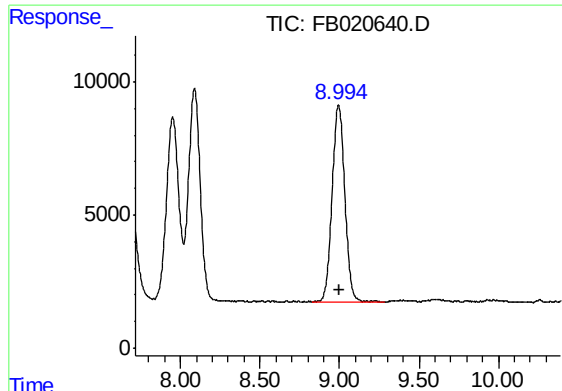


#5 AAA-TFT

R.T.: 8.995 min
Delta R.T.: -0.004 min
Response: 412069
Conc: 22.34 ng/ml

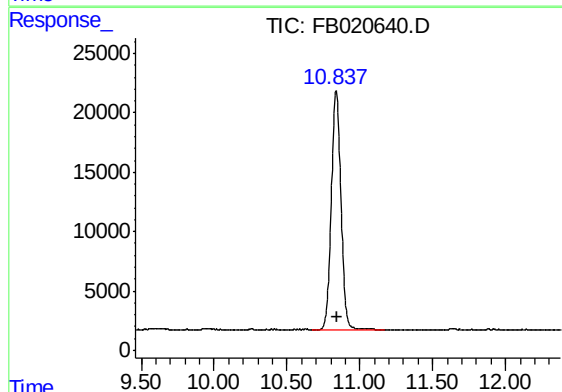


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.004 min
Response: 925320
Conc: 30.62 ng/ml

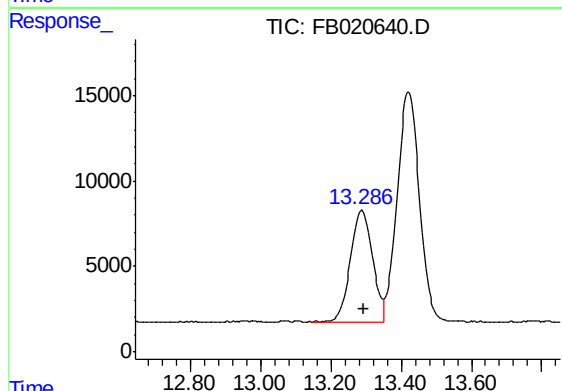


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: -0.004 min
Response: 286101
Conc: 11.18 ng/ml

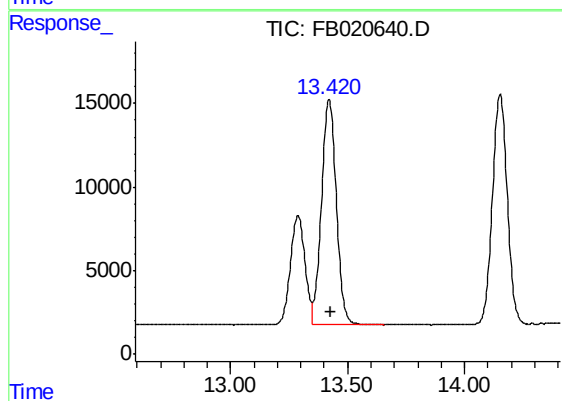


#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.004 min
Response: 597937
Conc: 22.62 ng/ml

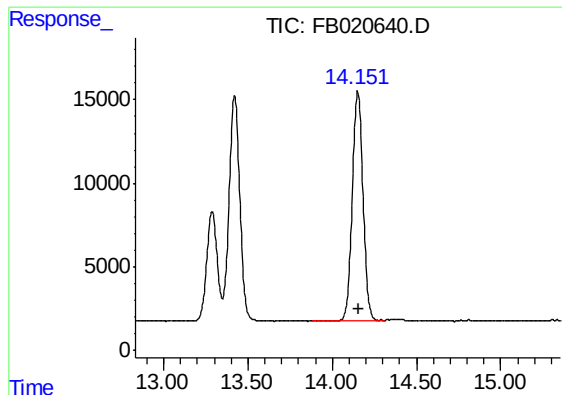

#9 O-Xylene

R.T.: 14.152 min
Delta R.T.: -0.004 min
Response: 610828
Conc: 22.56 ng/ml

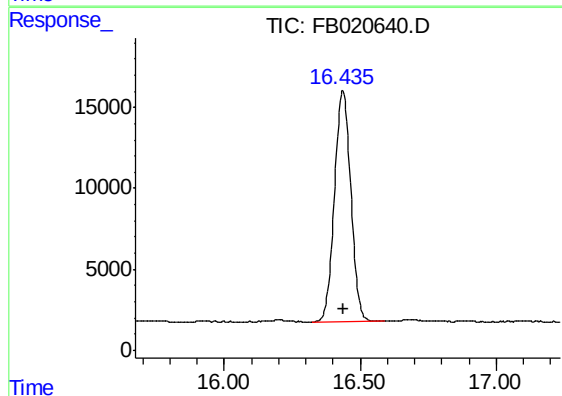

#10 1,2,4-Trimethylbenzene

R.T.: 16.437 min
Delta R.T.: -0.004 min
Response: 596048
Conc: 22.81 ng/ml