

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
 Data File : FB026957.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2022 15:02
 Operator : AJ/MA
 Sample : BSF0411S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 11 17:01:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	297652	26.328 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	539261	28.648 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	563996	28.192 ng/ml
3) t n-Heptane	7.749	194773	9.957 ng/ml
4) t Benzene	7.885	216624	9.816 ng/ml
6) t Toluene	10.618	630071	30.556 ng/ml
7) t Ethylbenzene	13.054	195007	10.206 ng/ml
8) t m-Xylene	13.187	384860	20.374 ng/ml
9) t O-Xylene	13.914	370638	20.462 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	377655	20.489 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
Data File : FB026957.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2022 15:02
Operator : AJ/MA
Sample : BSF0411S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 11 17:01:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

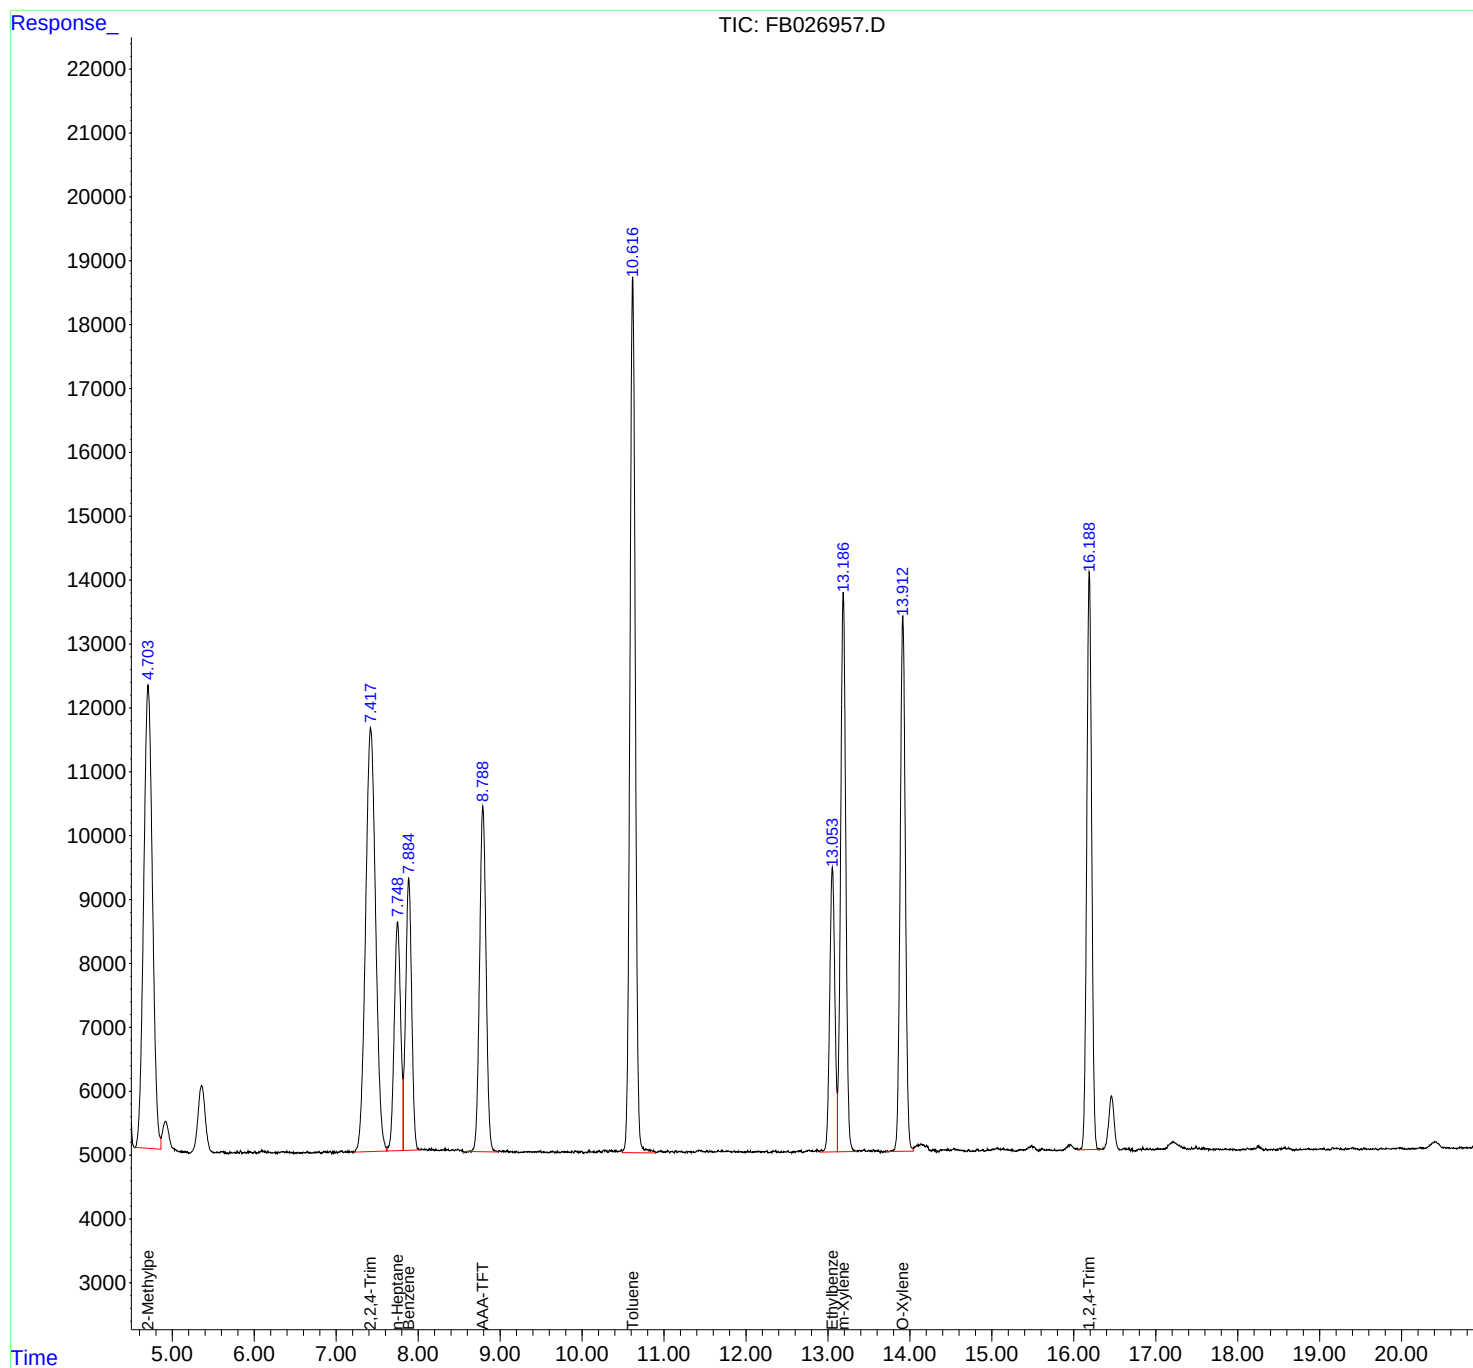


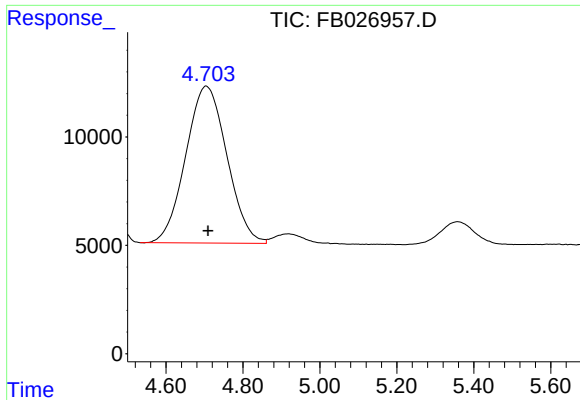

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.004 min
Response: 539261
Conc: 28.65 ng/ml

Instrument :
FID_B
ClientSampleId :

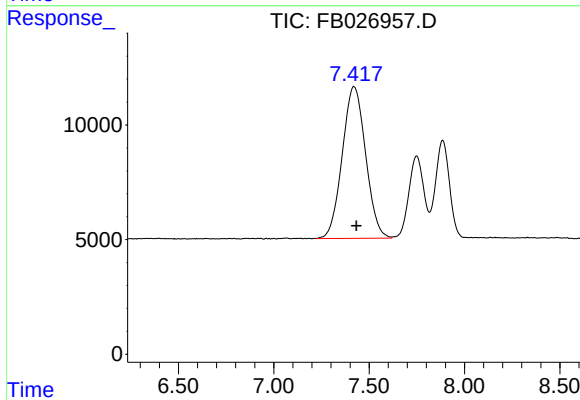


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: -0.014 min
Response: 563996
Conc: 28.19 ng/ml

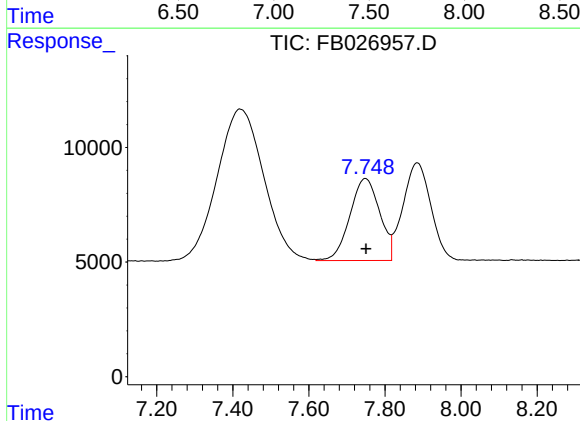


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: -0.002 min
Response: 194773
Conc: 9.96 ng/ml

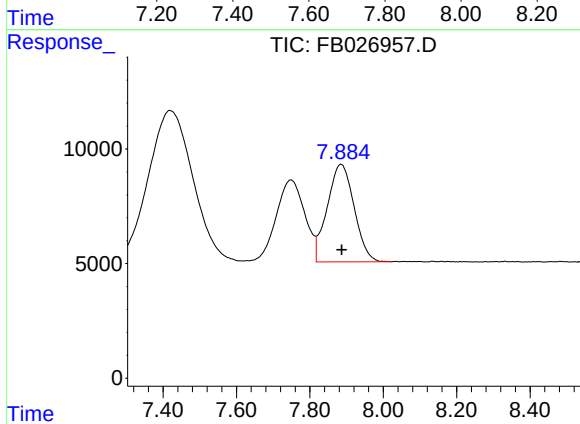

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 216624
Conc: 9.82 ng/ml

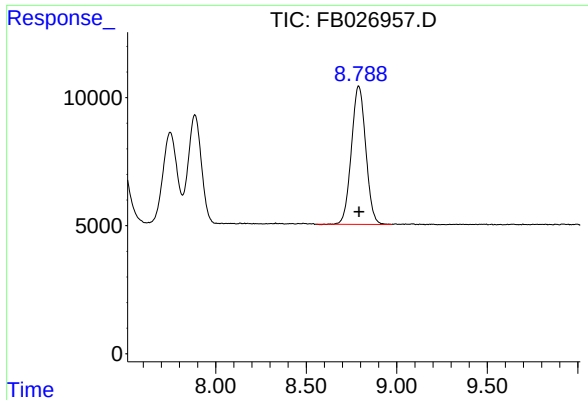

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 297652
Conc: 26.33 ng/ml

Instrument :
FID_B
ClientSampleId :

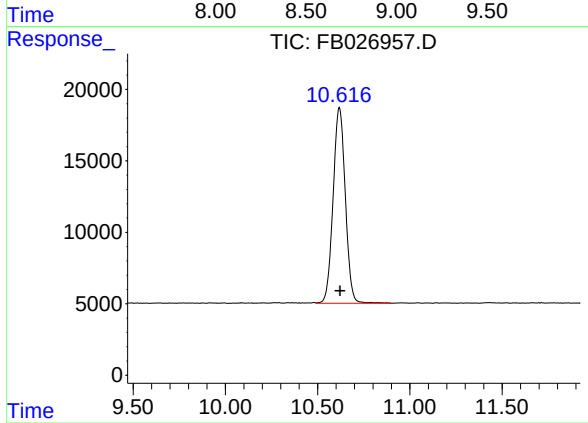


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 630071
Conc: 30.56 ng/ml

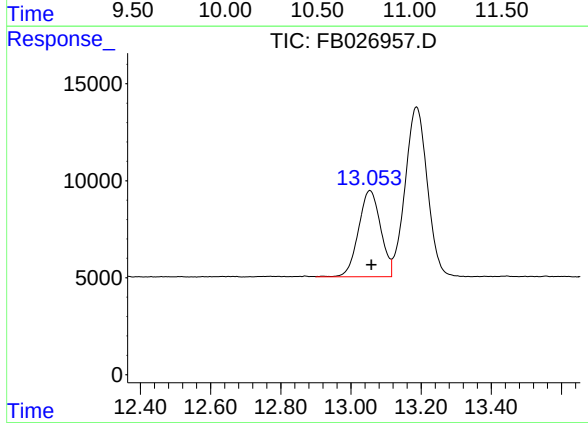


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 195007
Conc: 10.21 ng/ml

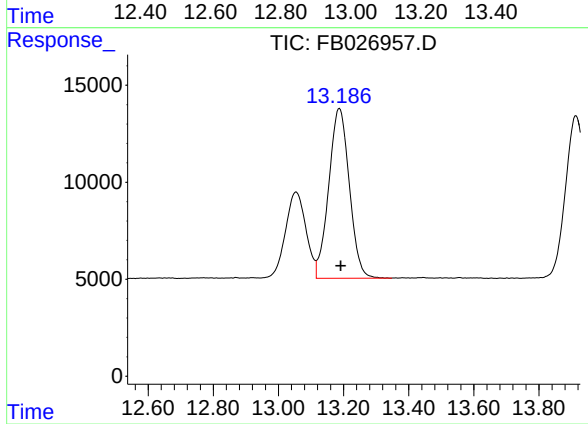

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 384860
Conc: 20.37 ng/ml

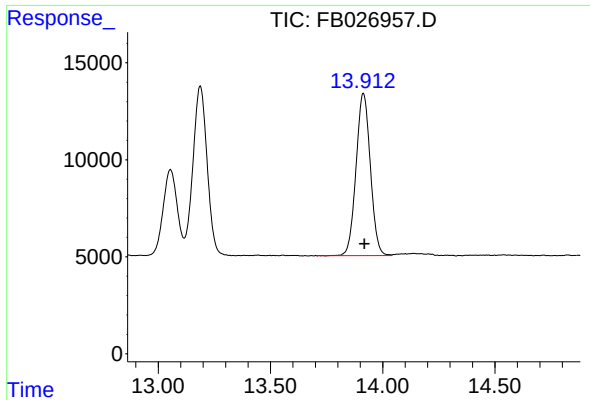

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 370638
Conc: 20.46 ng/ml

Instrument :
FID_B
ClientSampleId :

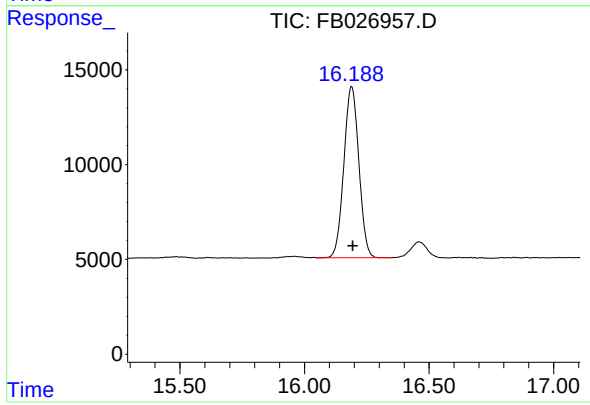

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 377655
Conc: 20.49 ng/ml