

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
 Data File : FB026966.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2022 20:26
 Operator : AJ/MA
 Sample : N2301-08 500X
 Misc : 5.01G/5.00 ML MEOH
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 11 20:52:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	283774	25.101 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.676	580	0.031 ng/ml
2) t 2,2,4-Trimethylpentane	7.466	77694	3.884 ng/ml
3) t n-Heptane	7.730	10109	0.517 ng/ml
7) t Ethylbenzene	13.015	772096	40.409 ng/ml
9) t O-Xylene	13.934	116430	6.428 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	20228	1.097 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
Data File : FB026966.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2022 20:26
Operator : AJ/MA
Sample : N2301-08 500X
Misc : 5.01G/5.00 ML MEOH
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 11 20:52:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

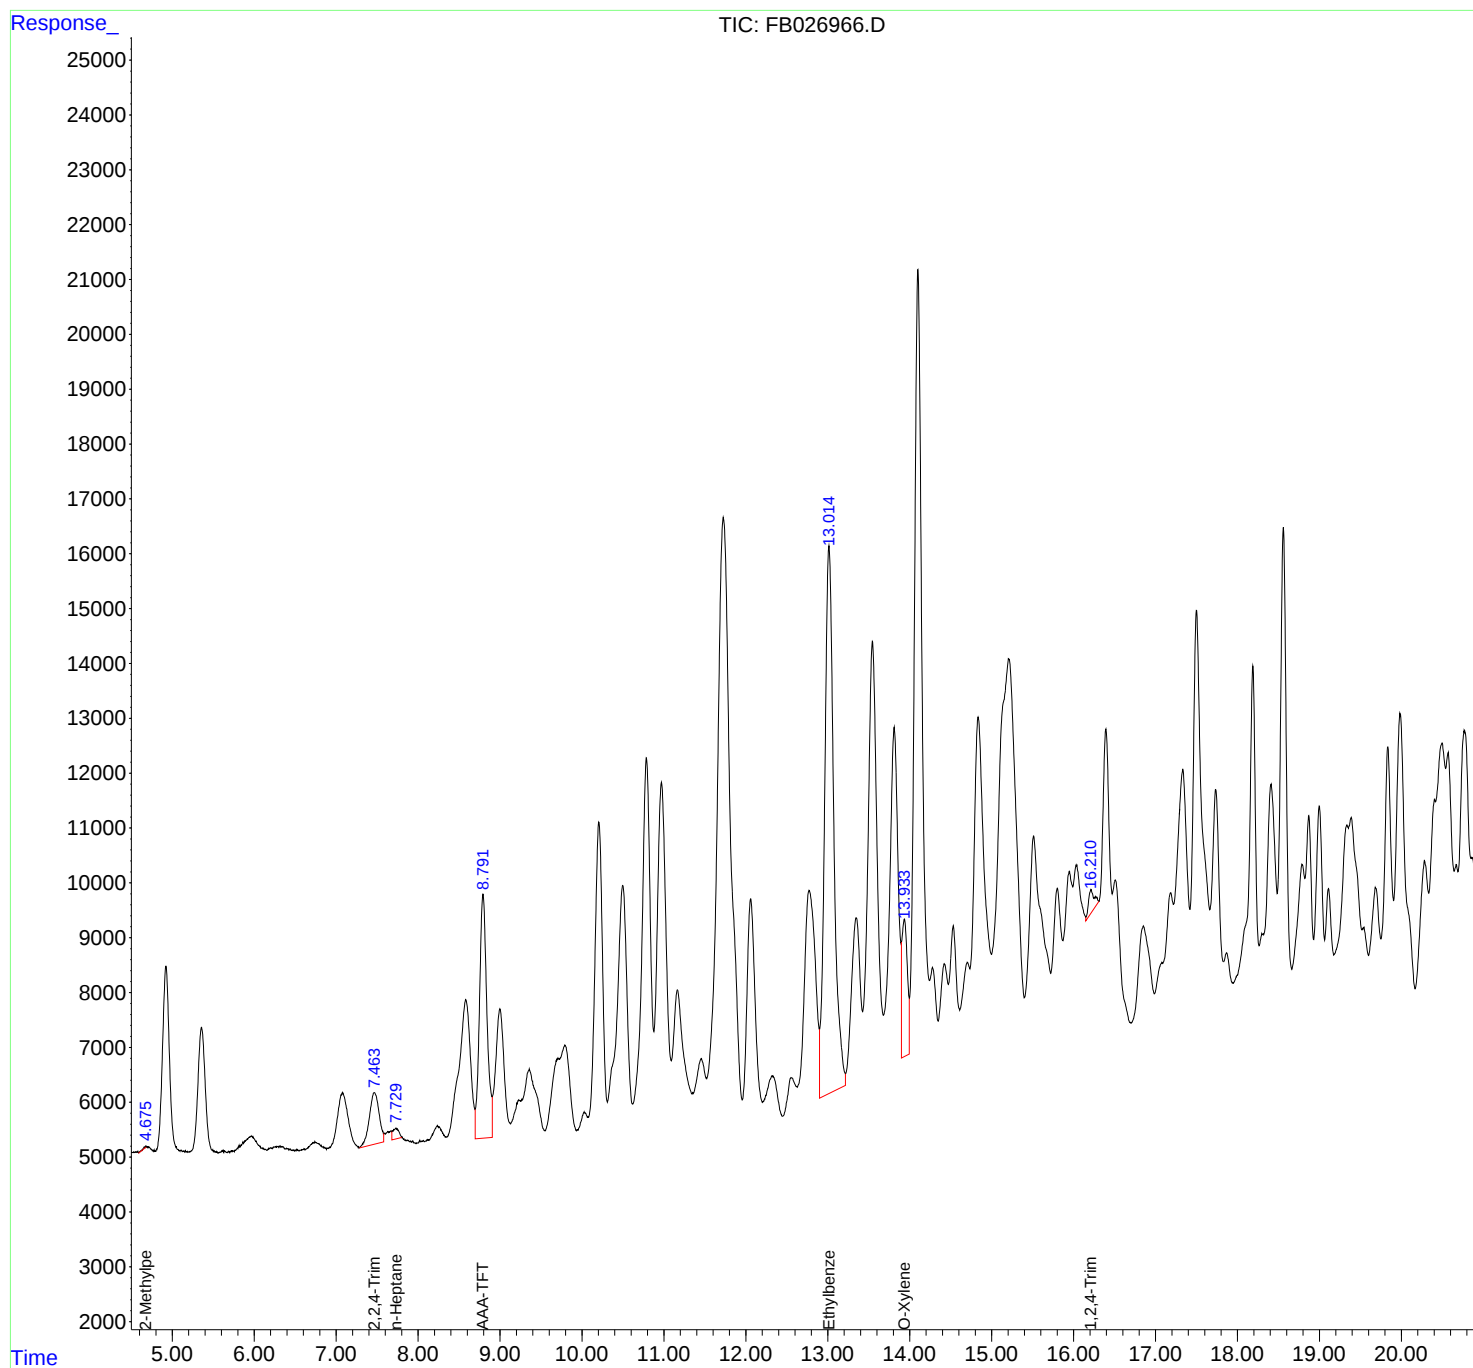


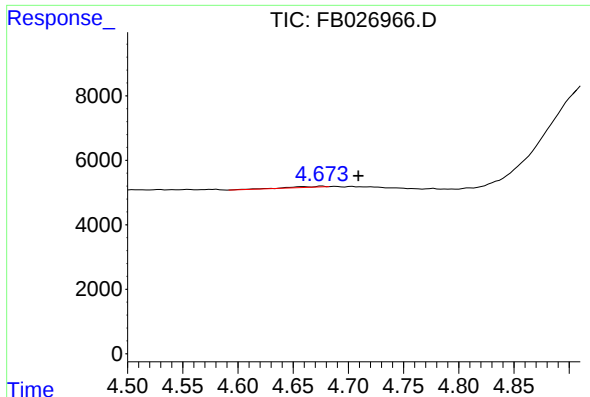

#1 2-Methylpentane


R.T.: 4.676 min
Delta R.T.: -0.033 min
Response: 580
Conc: 0.03 ng/ml

Instrument :
FID_B
ClientSampleId :

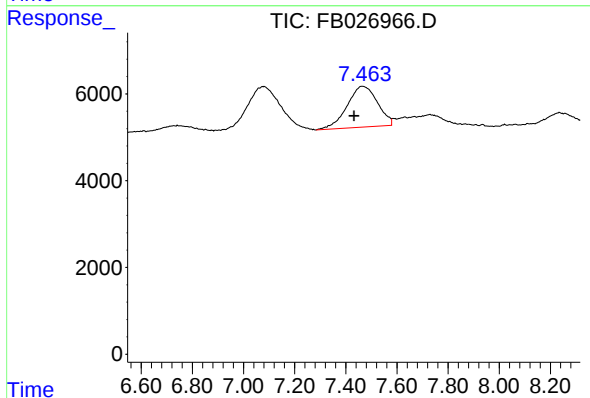


#2 2,2,4-Trimethylpentane

R.T.: 7.466 min
Delta R.T.: 0.033 min
Response: 77694
Conc: 3.88 ng/ml

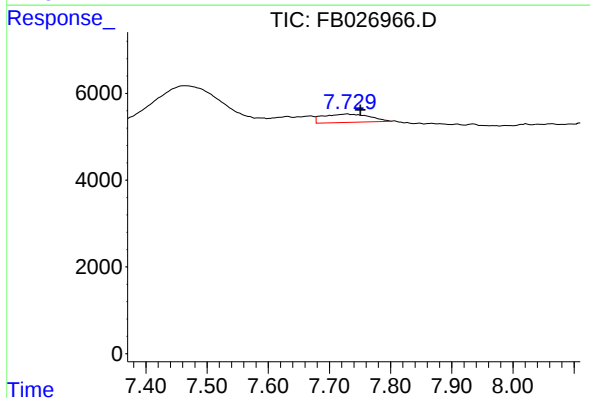


#3 n-Heptane

R.T.: 7.730 min
Delta R.T.: -0.020 min
Response: 10109
Conc: 0.52 ng/ml

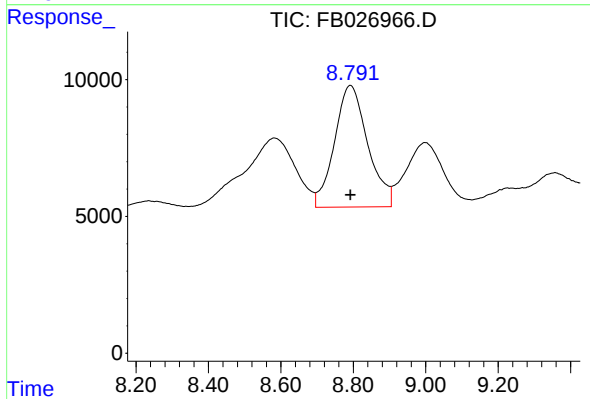

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 283774
Conc: 25.10 ng/ml

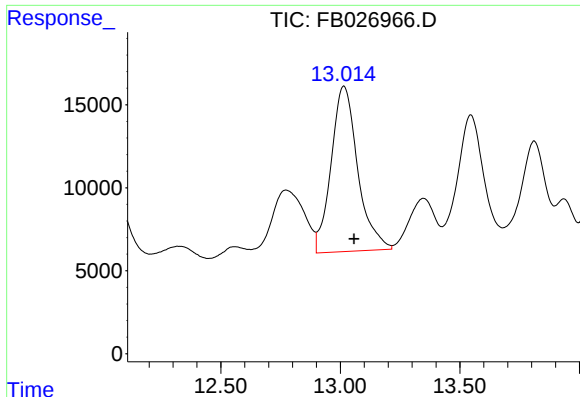

#7 Ethylbenzene


R.T.: 13.015 min
Delta R.T.: -0.044 min
Response: 772096
Conc: 40.41 ng/ml

Instrument :
FID_B
ClientSampleId :

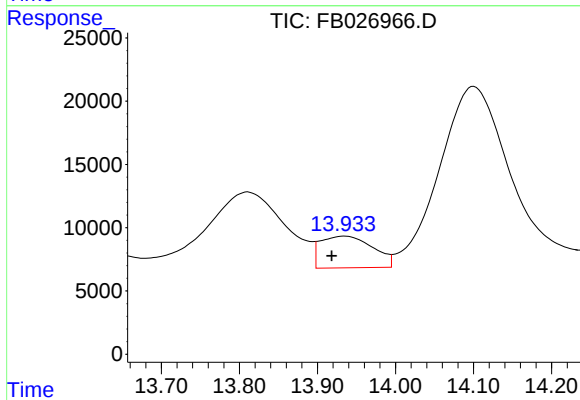

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.016 min
Response: 116430
Conc: 6.43 ng/ml

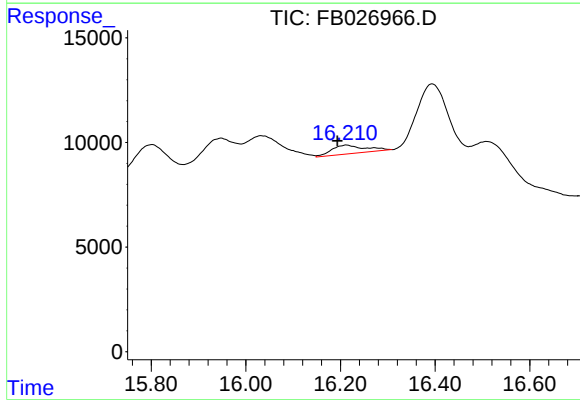

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.019 min
Response: 20228
Conc: 1.10 ng/ml