

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
 Data File : FB026951.D
 Signal(s) : FID2B.CH
 Acq On : 11 Apr 2022 11:07
 Operator : AJ/MA
 Sample : BSF0411S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0411S1

Integration File: Calibration.e
 Quant Time: Apr 11 13:38:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	81264	7.188 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.698	211562	11.239 ng/ml
2) t 2,2,4-Trimethylpentane	7.413	216814	10.838 ng/ml
3) t n-Heptane	7.748	65501	3.348 ng/ml
4) t Benzene	7.883	63530	2.879 ng/ml
6) t Toluene	10.615	185574	9.000 ng/ml
7) t Ethylbenzene	13.053	62920	3.293 ng/ml
8) t m-Xylene	13.186	124987	6.617 ng/ml
9) t O-Xylene	13.912	117164	6.468 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	126501	6.863 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041122\
Data File : FB026951.D
Signal(s) : FID2B.CH
Acq On : 11 Apr 2022 11:07
Operator : AJ/MA
Sample : BSF0411S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0411S1

Integration File: Calibration.e
Quant Time: Apr 11 13:38:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

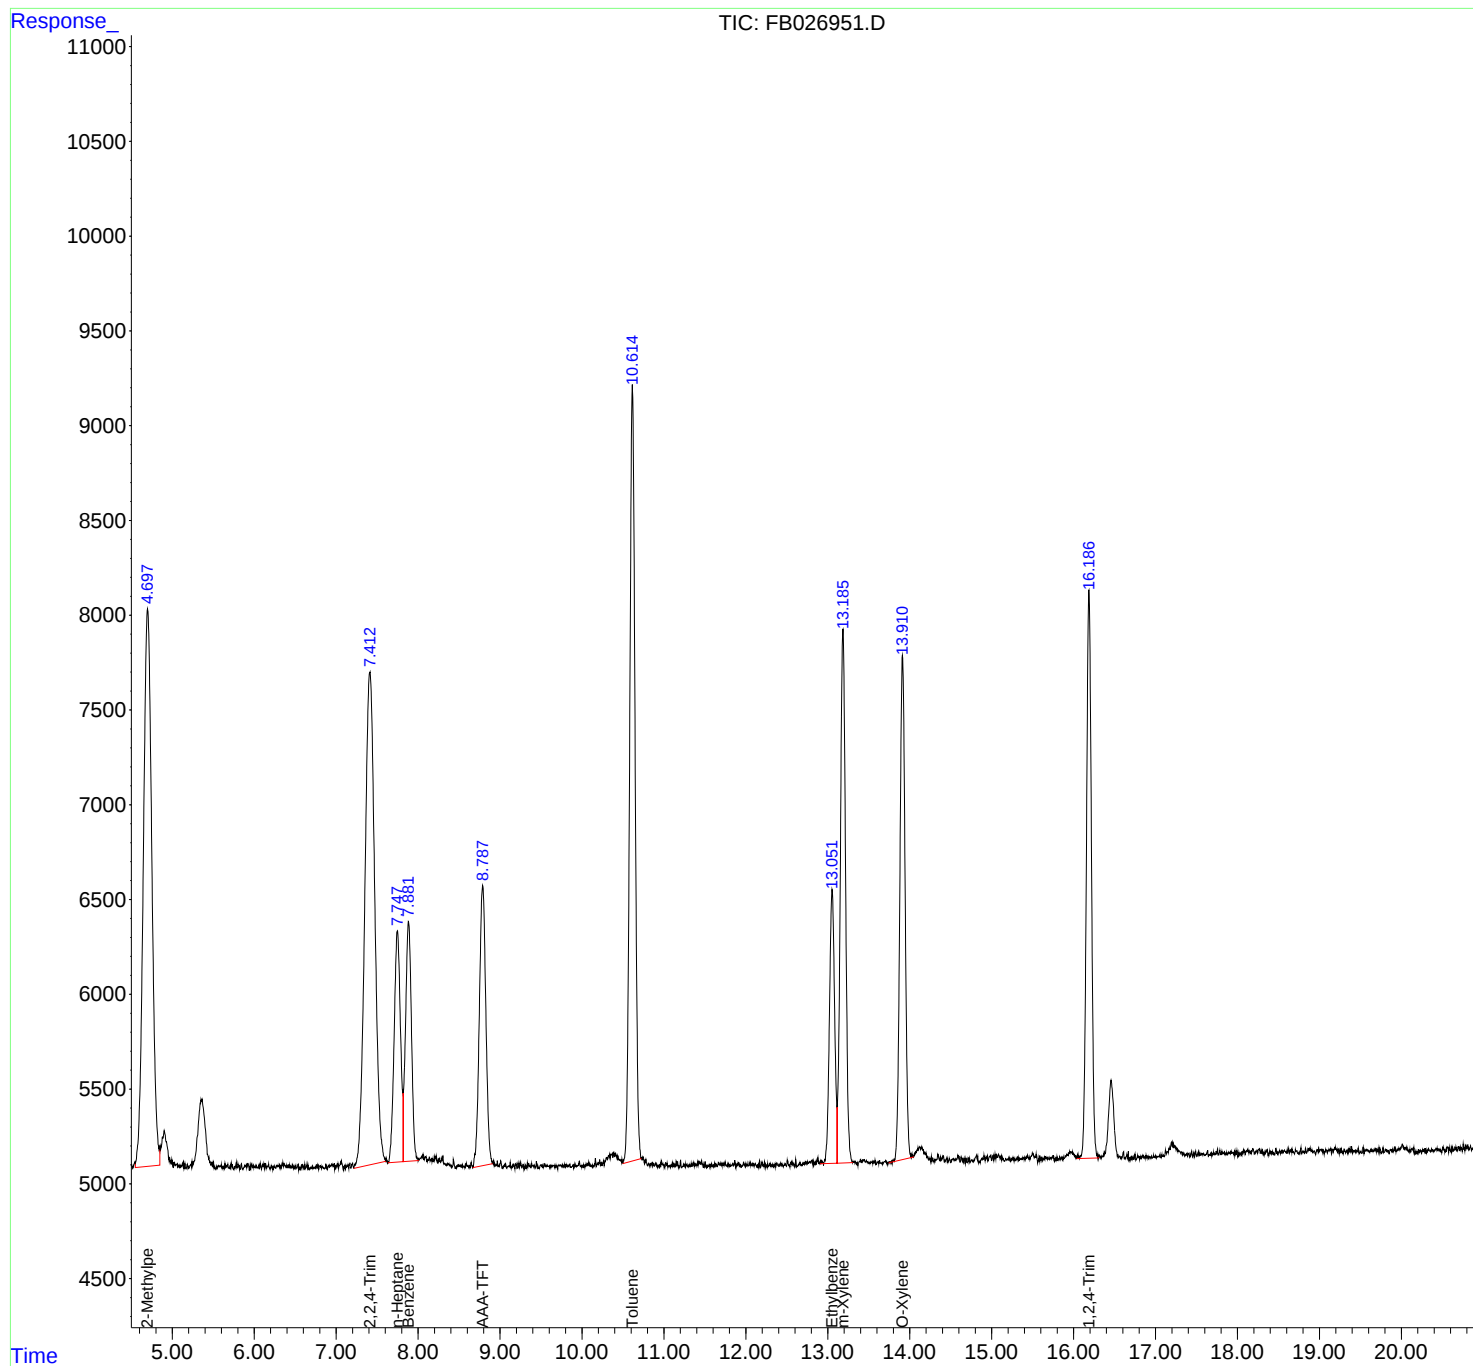


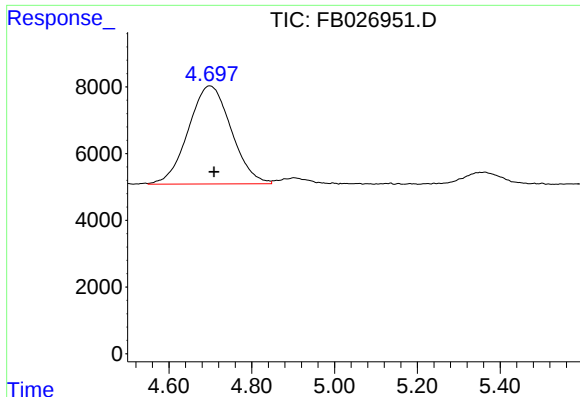

#1 2-Methylpentane


R.T.: 4.698 min
Delta R.T.: -0.011 min
Response: 211562
Conc: 11.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0411S1

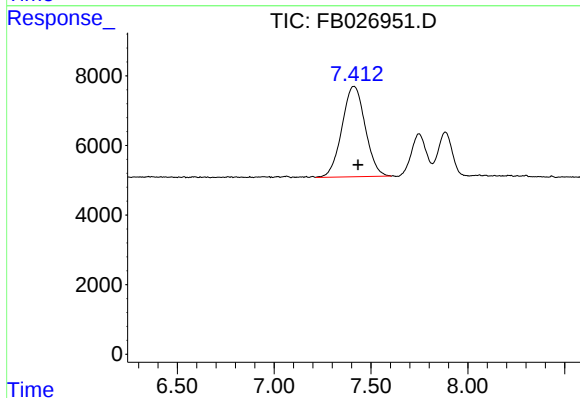


#2 2,2,4-Trimethylpentane

R.T.: 7.413 min
Delta R.T.: -0.020 min
Response: 216814
Conc: 10.84 ng/ml

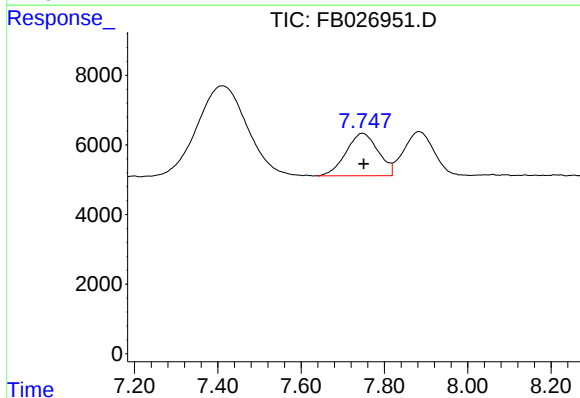


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.002 min
Response: 65501
Conc: 3.35 ng/ml

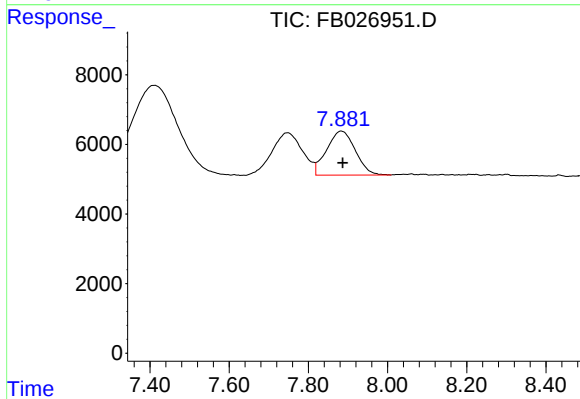

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.004 min
Response: 63530
Conc: 2.88 ng/ml

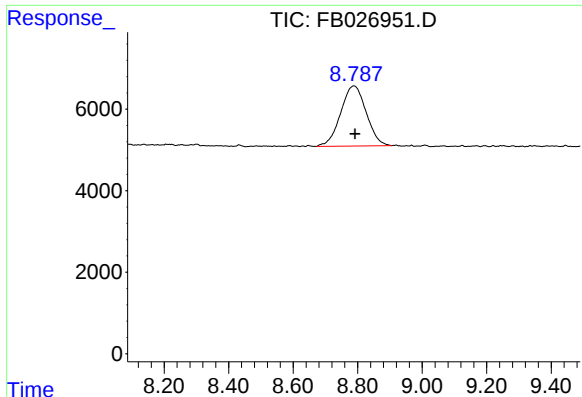

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 81264
Conc: 7.19 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0411S1

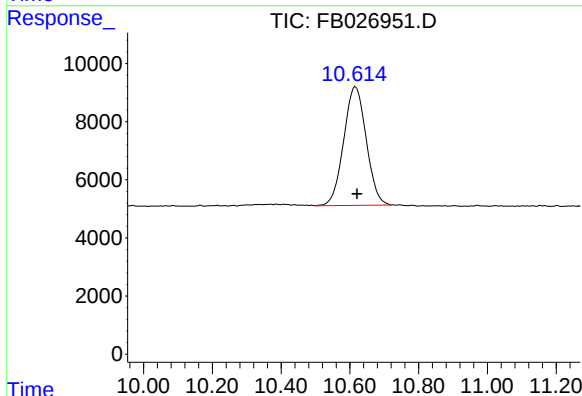


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.006 min
Response: 185574
Conc: 9.00 ng/ml

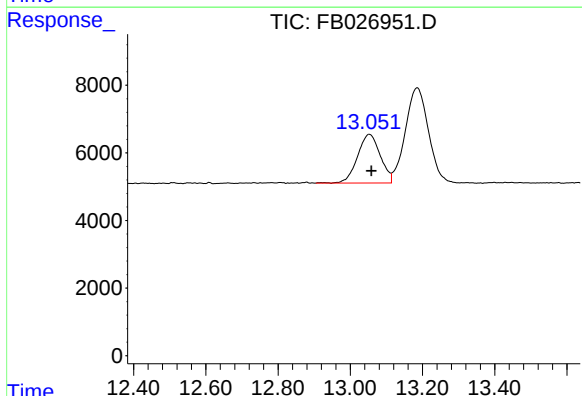


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 62920
Conc: 3.29 ng/ml

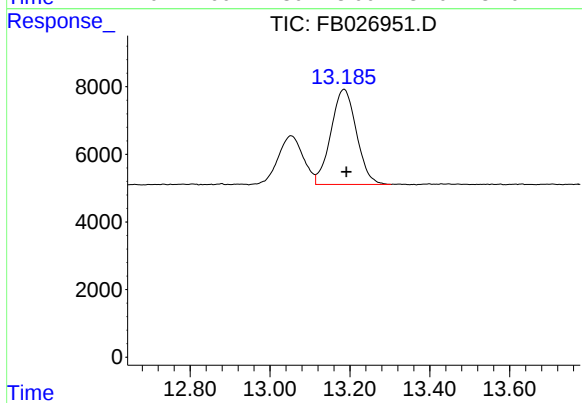

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.005 min
Response: 124987
Conc: 6.62 ng/ml

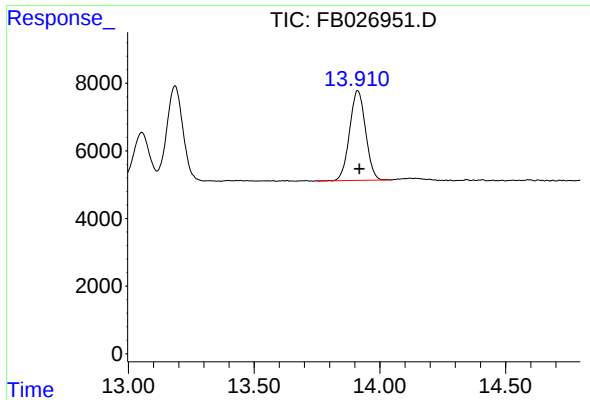

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.007 min
Response: 117164
Conc: 6.47 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0411S1

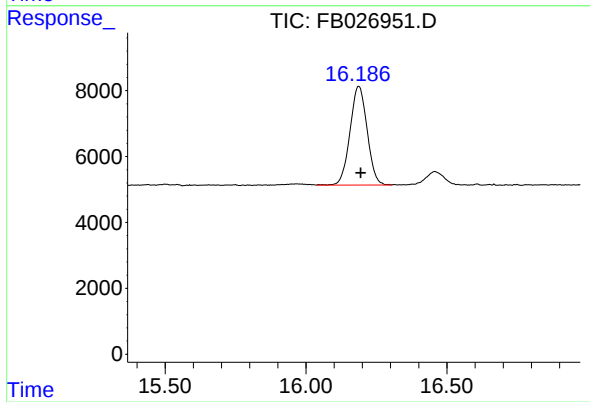

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.006 min
Response: 126501
Conc: 6.86 ng/ml