

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041219\
 Data File : FB020661.D
 Signal(s) : FID2B.CH
 Acq On : 12 Apr 2019 9:23
 Operator : MJ/SJ
 Sample : BSF0412S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 13 00:07:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
 Quant Title :
 QLast Update : Thu Apr 04 17:27:15 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.994	395623	21.450 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.866	1174171	33.354 ng/ml
2) t 2,2,4-Trimethylpentane	7.620	1040312	34.894 ng/ml
3) t n-Heptane	7.951	422353	10.759 ng/ml
4) t Benzene	8.087	428403	10.430 ng/ml
6) t Toluene	10.838	973475	32.217 ng/ml
7) t Ethylbenzene	13.288	293904	11.489 ng/ml
8) t m-Xylene	13.421	613237	23.203 ng/ml
9) t O-Xylene	14.151	626520	23.143 ng/ml
10) t 1,2,4-Trimethylbenzene	16.435	614113	23.505 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041219\
Data File : FB020661.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2019 9:23
Operator : MJ/SJ
Sample : BSF0412S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 13 00:07:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040419.M
Quant Title :
QLast Update : Thu Apr 04 17:27:15 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

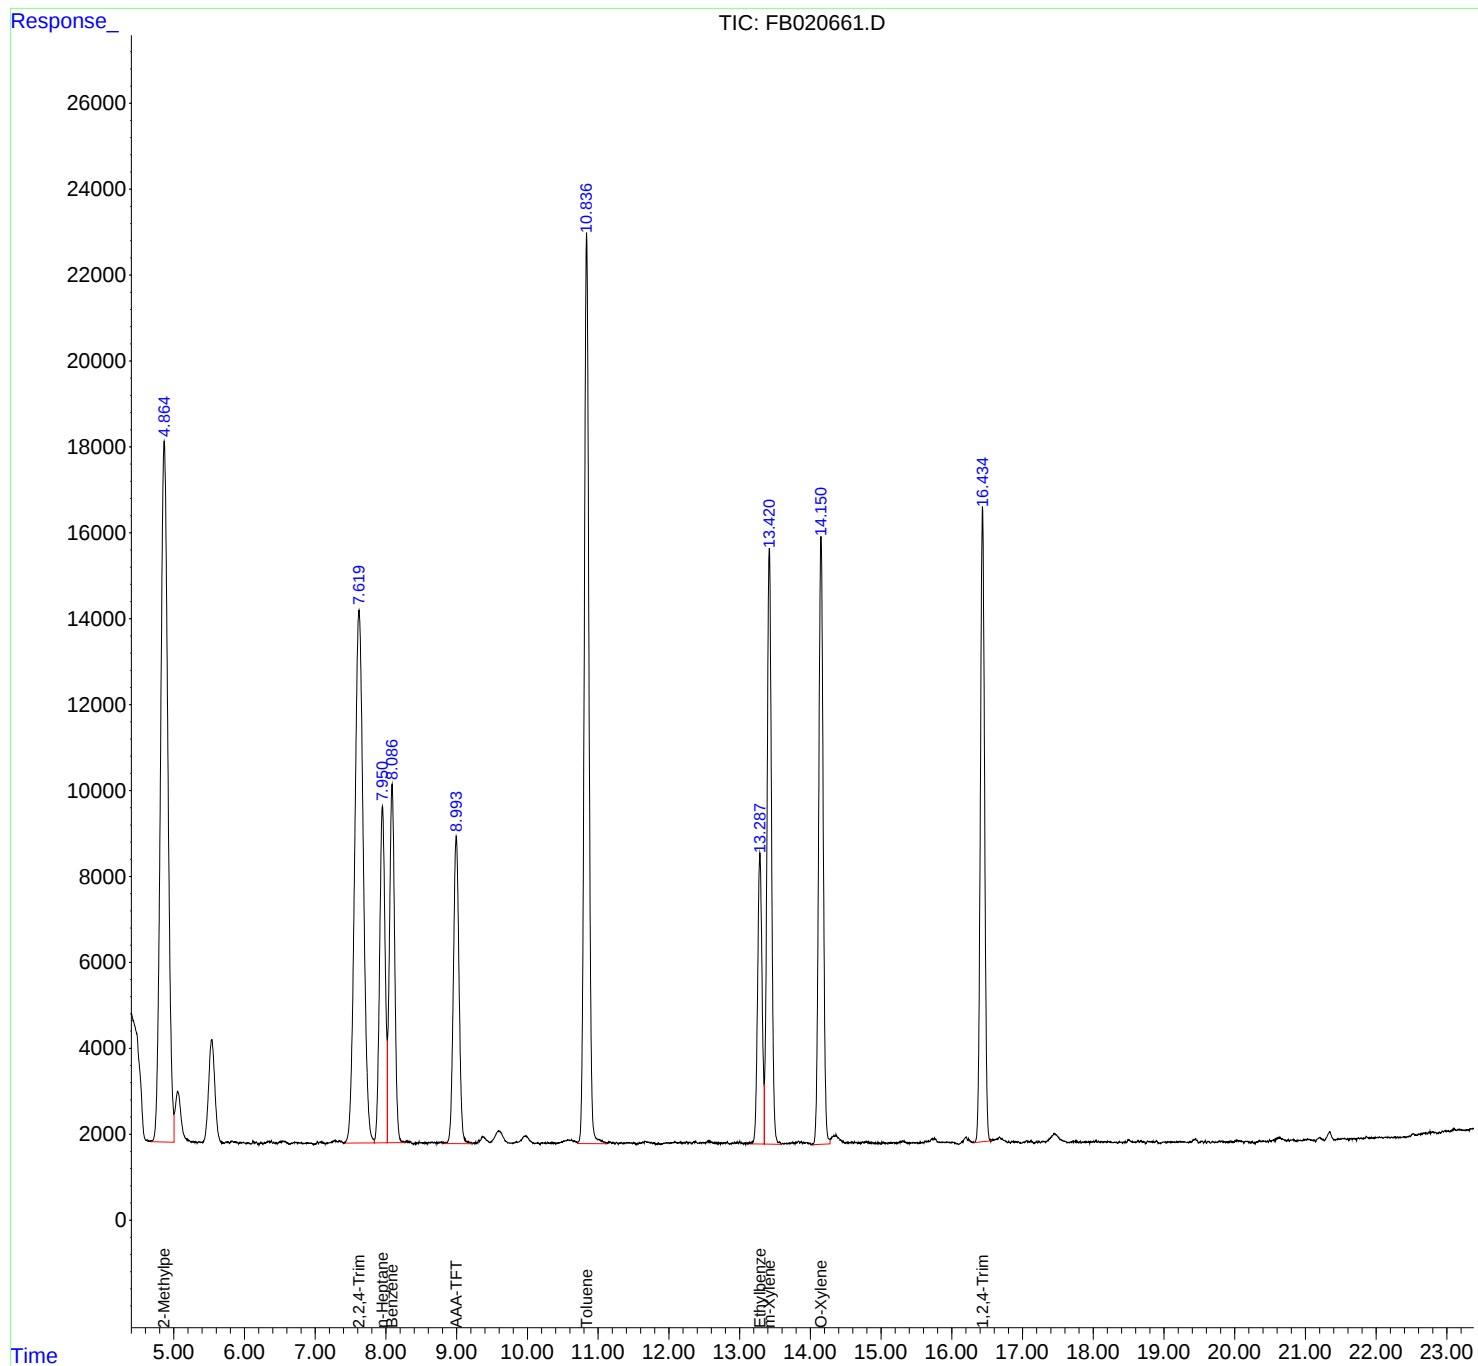

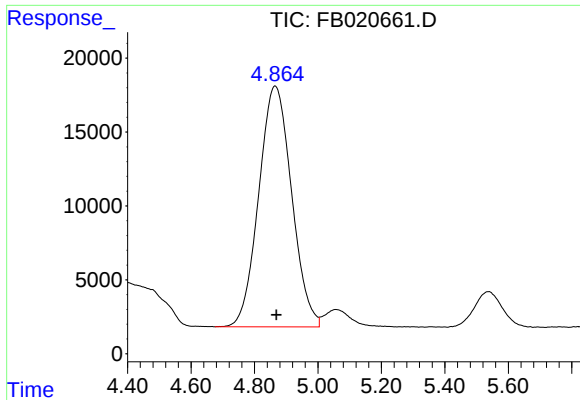


#1 2-Methylpentane

R.T.: 4.866 min
 Delta R.T.: -0.003 min
 Response: 1174171
 Conc: 33.35 ng/ml

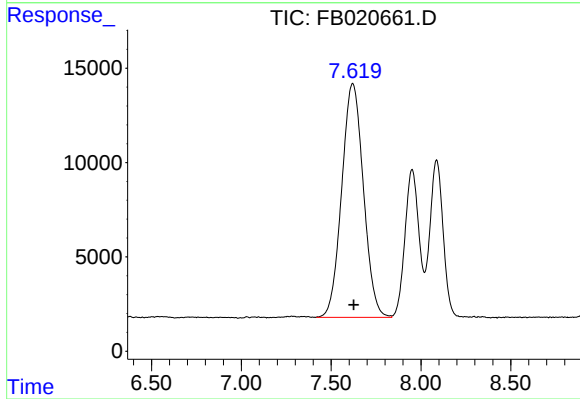


#2 2,2,4-Trimethylpentane

R.T.: 7.620 min
 Delta R.T.: -0.007 min
 Response: 1040312
 Conc: 34.89 ng/ml

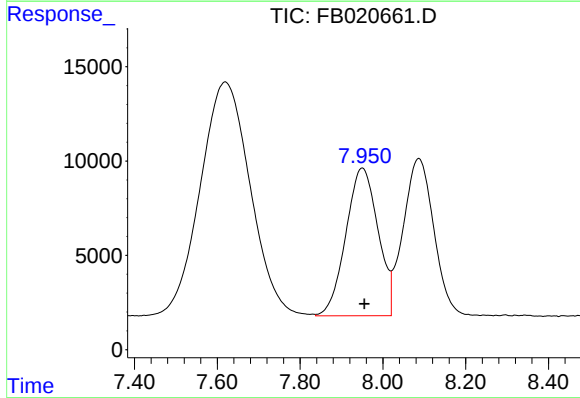


#3 n-Heptane

R.T.: 7.951 min
 Delta R.T.: -0.004 min
 Response: 422353
 Conc: 10.76 ng/ml

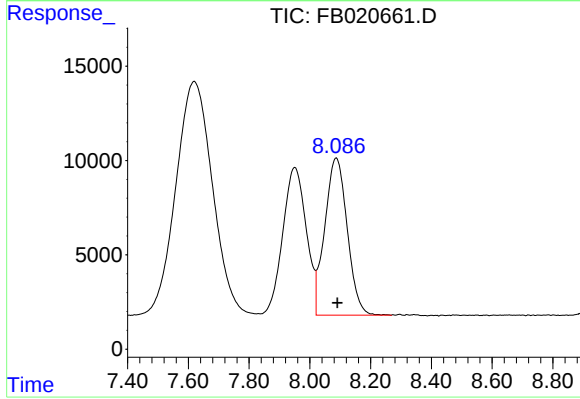


#4 Benzene

R.T.: 8.087 min
 Delta R.T.: -0.004 min
 Response: 428403
 Conc: 10.43 ng/ml

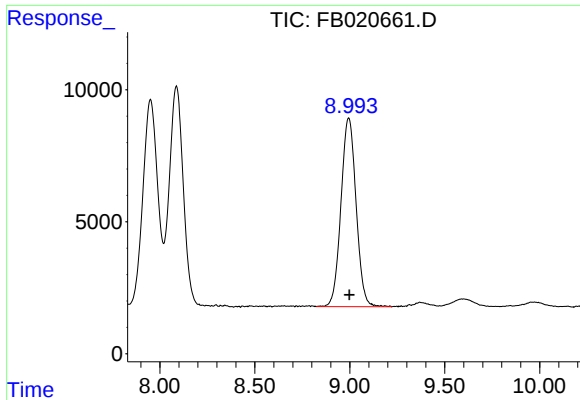


#5 AAA-TFT

R.T.: 8.994 min
Delta R.T.: -0.004 min
Response: 395623
Conc: 21.45 ng/ml

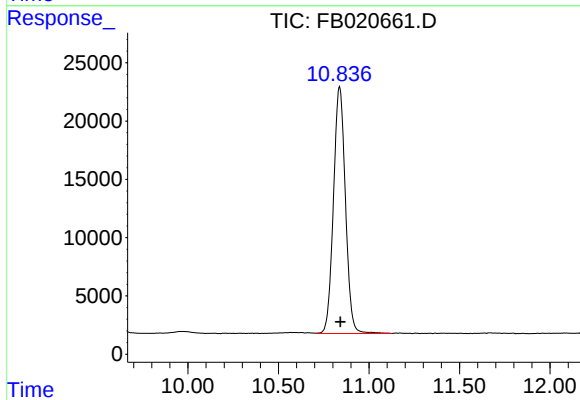


#6 Toluene

R.T.: 10.838 min
Delta R.T.: -0.005 min
Response: 973475
Conc: 32.22 ng/ml

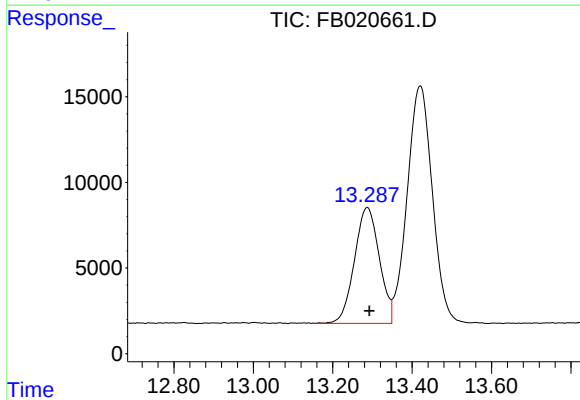


#7 Ethylbenzene

R.T.: 13.288 min
Delta R.T.: -0.005 min
Response: 293904
Conc: 11.49 ng/ml

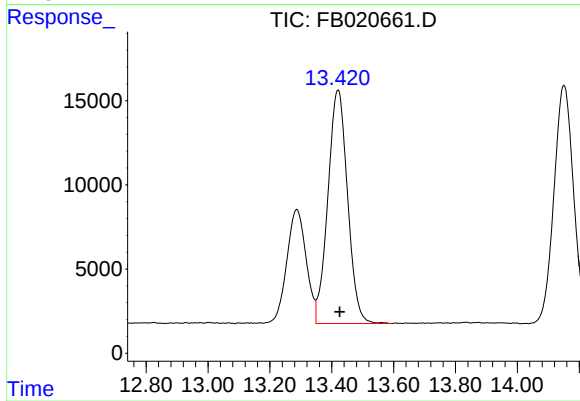

#8 m-Xylene

R.T.: 13.421 min
Delta R.T.: -0.005 min
Response: 613237
Conc: 23.20 ng/ml

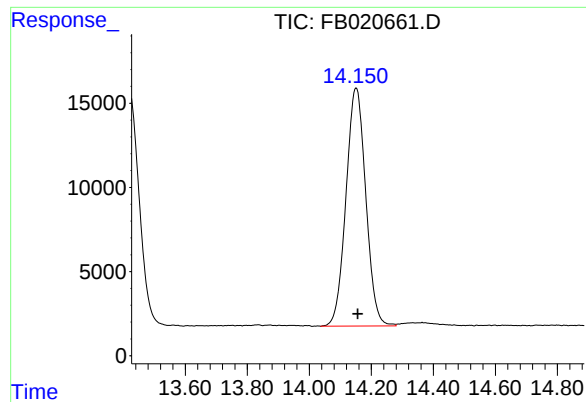


#9 O-Xylene

R.T.: 14.151 min

Delta R.T.: -0.005 min

Response: 626520

Conc: 23.14 ng/ml

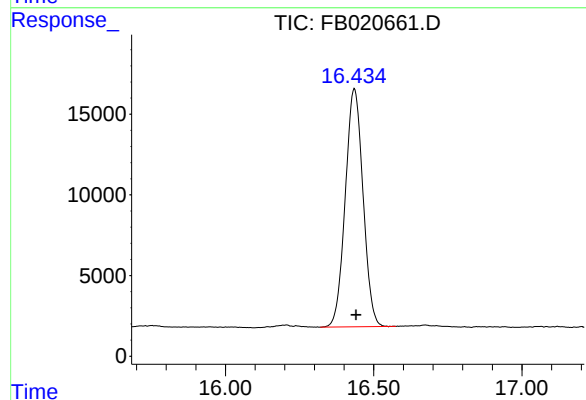

#10 1,2,4-Trimethylbenzene

R.T.: 16.435 min

Delta R.T.: -0.005 min

Response: 614113

Conc: 23.50 ng/ml