

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026985.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 14:05
Operator : AJ/MA
Sample : N2335-02 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 12 14:27:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	332129	29.378 ng/ml
Target Compounds			
4) t Benzene	7.935	6045	0.274 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026985.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 14:05
Operator : AJ/MA
Sample : N2335-02 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 12 14:27:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

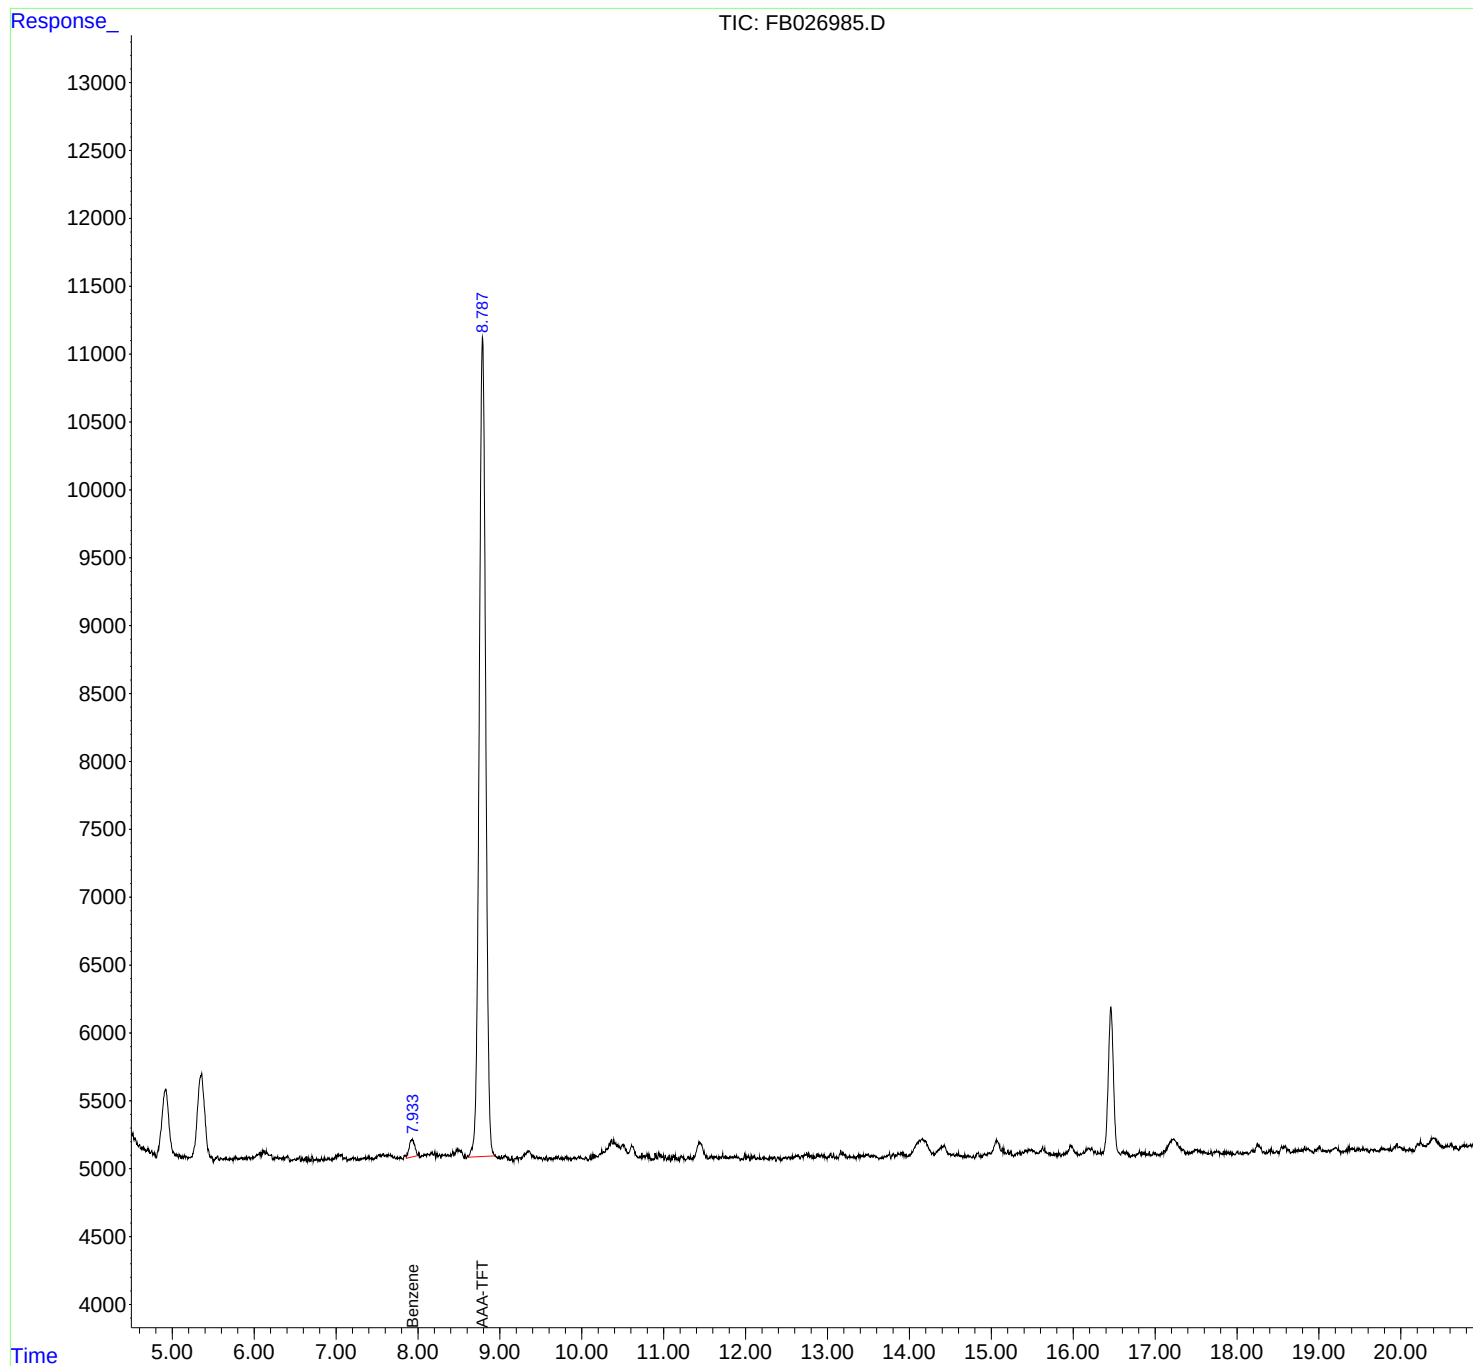


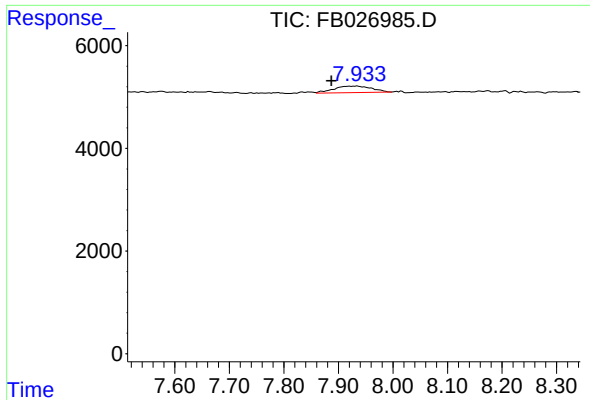

#4 Benzene

R.T.: 7.935 min
Delta R.T.: 0.048 min
Response: 6045
Conc: 0.27 ng/ml

Instrument :
FID_B
ClientSampleId :

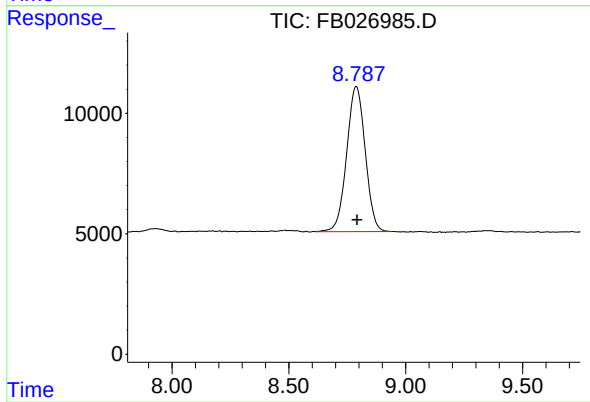

#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 332129
Conc: 29.38 ng/ml