

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026989.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 16:30
Operator : AJ/MA
Sample : N2337-02 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 12 16:50:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.791	256539	22.692 ng/ml
Target Compounds			
4) t Benzene	7.926	7197	0.326 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB026989.D
Signal(s) : FID2B.CH
Acq On : 12 Apr 2022 16:30
Operator : AJ/MA
Sample : N2337-02 50X
Misc : 5.03G/5.00 ML DI WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 12 16:50:56 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

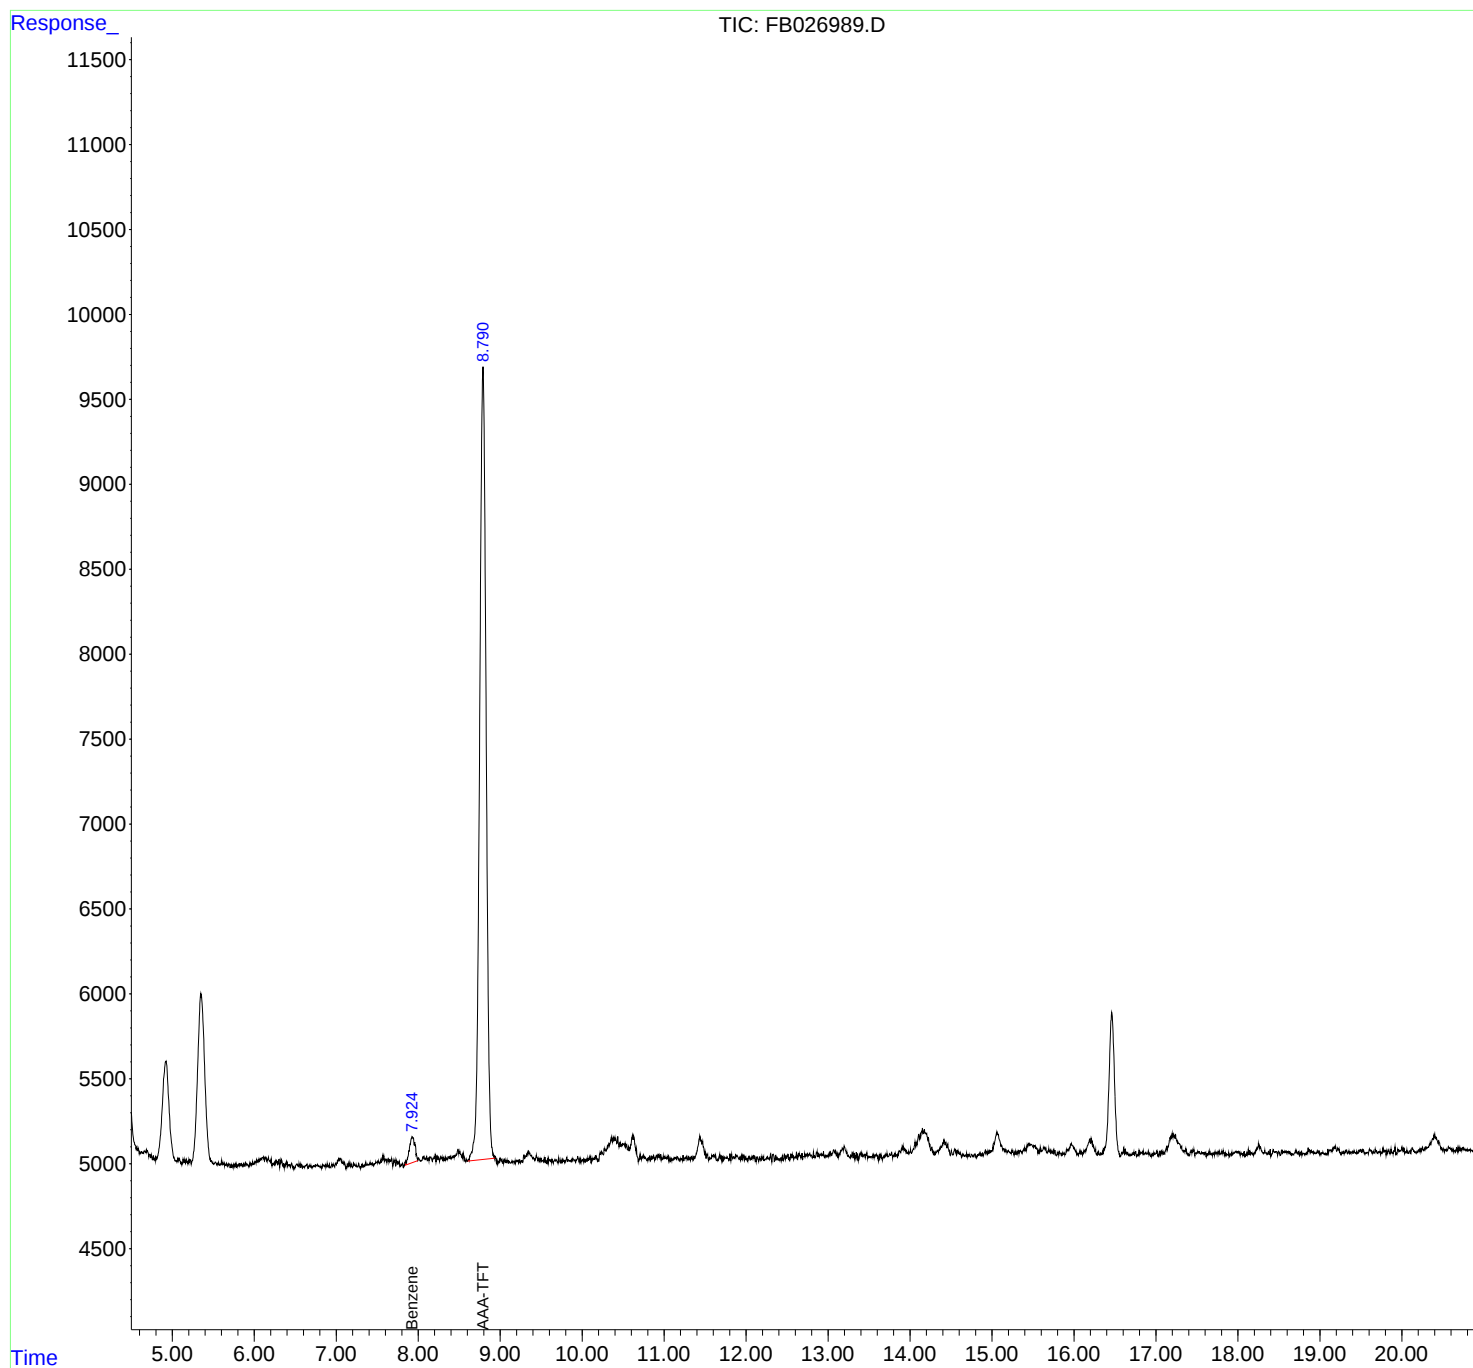


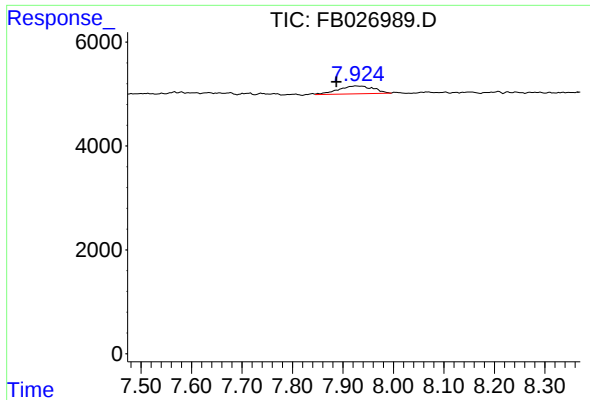

#4 Benzene

R.T.: 7.926 min
Delta R.T.: 0.039 min
Response: 7197
Conc: 0.33 ng/ml

Instrument :
FID_B
ClientSampleId :

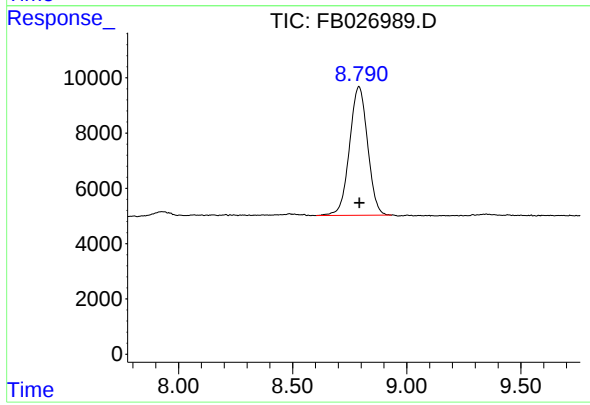

#5 AAA-TFT

R.T.: 8.791 min
Delta R.T.: 0.000 min
Response: 256539
Conc: 22.69 ng/ml