

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
 Data File : FB027001.D
 Signal(s) : FID2B.CH
 Acq On : 13 Apr 2022 00:20
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 13 03:11:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
 Quant Title :
 QLast Update : Sat Apr 09 04:06:25 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	297332	26.300 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	564825	30.006 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	610002	30.492 ng/ml
3) t n-Heptane	7.748	203107	10.383 ng/ml
4) t Benzene	7.885	229265	10.388 ng/ml
6) t Toluene	10.618	645745	31.316 ng/ml
7) t Ethylbenzene	13.054	203785	10.666 ng/ml
8) t m-Xylene	13.187	401167	21.237 ng/ml
9) t O-Xylene	13.914	387549	21.395 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	389166	21.114 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB041222\
Data File : FB027001.D
Signal(s) : FID2B.CH
Acq On : 13 Apr 2022 00:20
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 13 03:11:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB040922.M
Quant Title :
QLast Update : Sat Apr 09 04:06:25 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

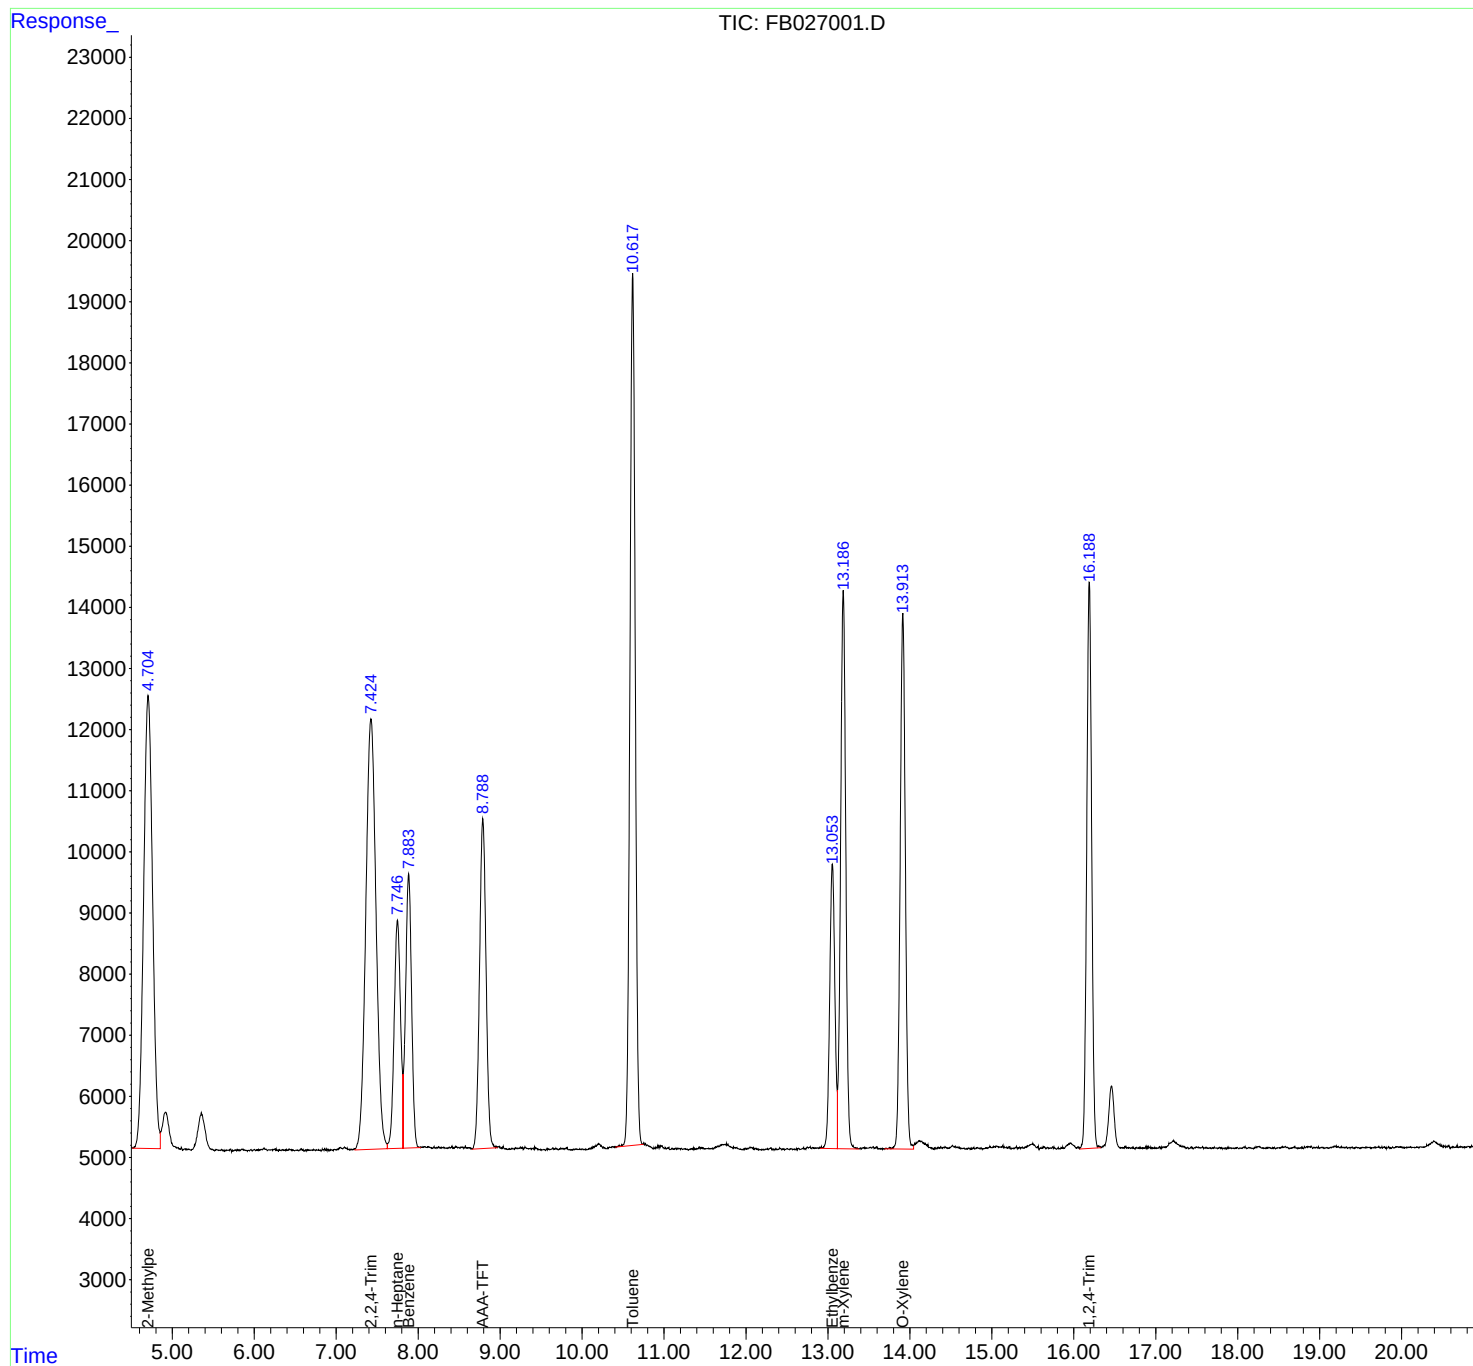


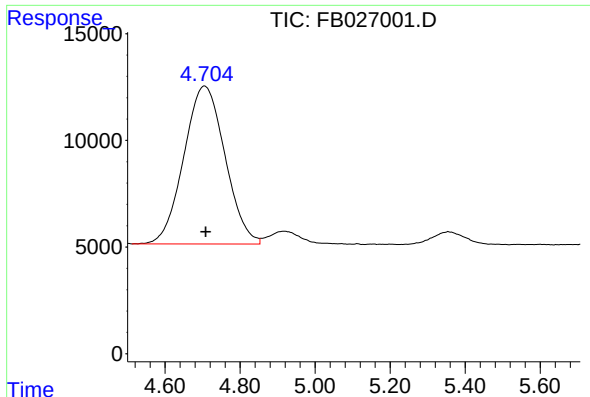

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.004 min
Response: 564825
Conc: 30.01 ng/ml

Instrument :
FID_B
ClientSampleId :

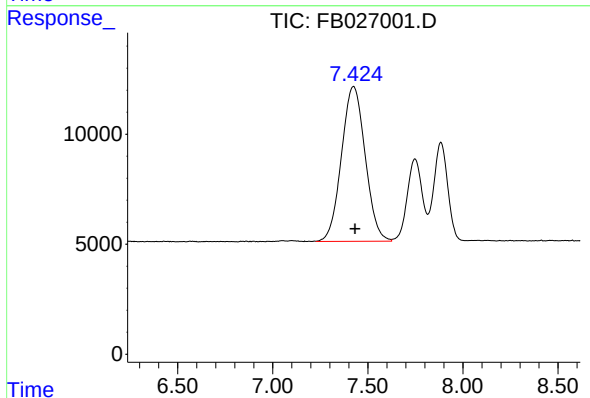


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.008 min
Response: 610002
Conc: 30.49 ng/ml

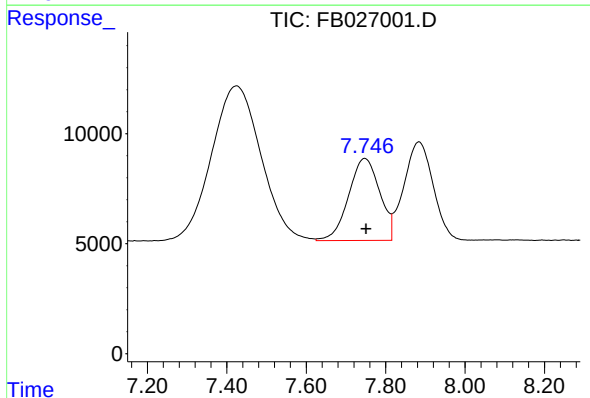


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.003 min
Response: 203107
Conc: 10.38 ng/ml

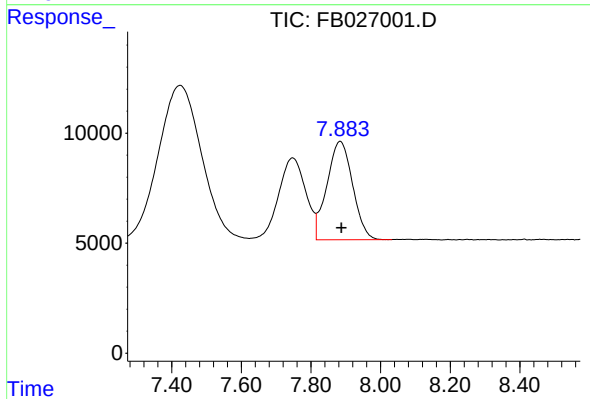

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.002 min
Response: 229265
Conc: 10.39 ng/ml

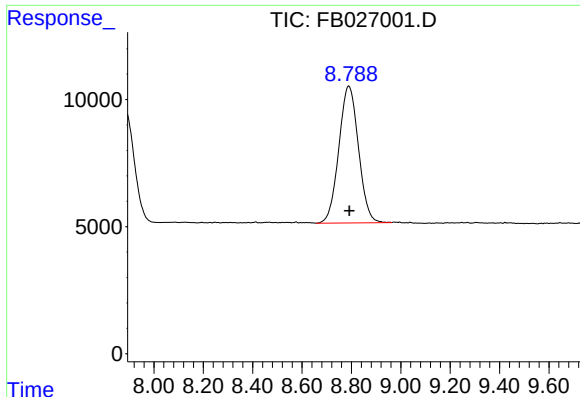

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 297332
Conc: 26.30 ng/ml

Instrument :
FID_B
ClientSampleId :

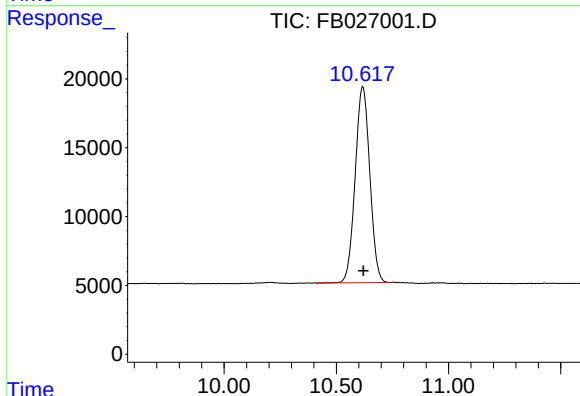


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 645745
Conc: 31.32 ng/ml

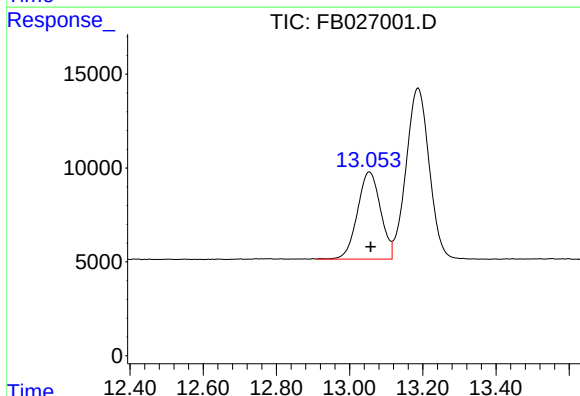


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.004 min
Response: 203785
Conc: 10.67 ng/ml

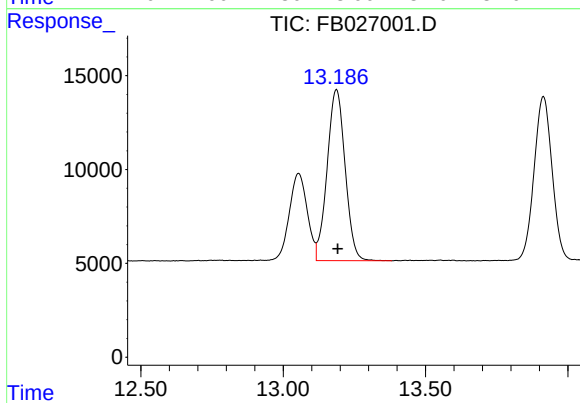

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 401167
Conc: 21.24 ng/ml

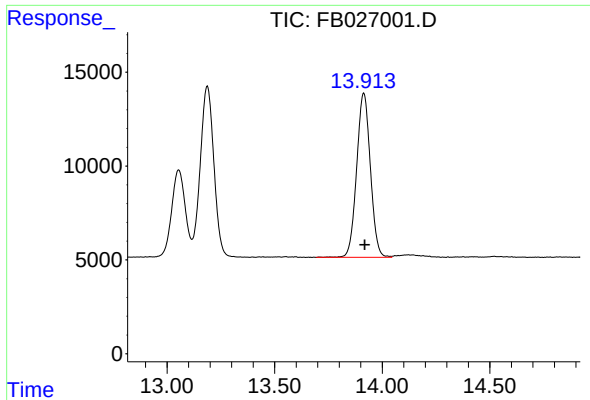

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 387549
Conc: 21.40 ng/ml

Instrument :
FID_B
ClientSampleId :

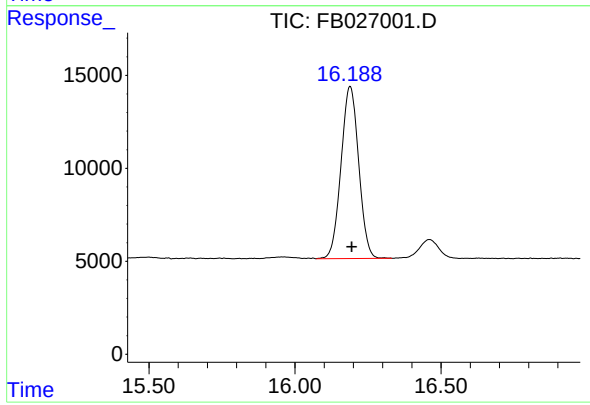

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 389166
Conc: 21.11 ng/ml